



Ethyl methacrylate

Response Ratio

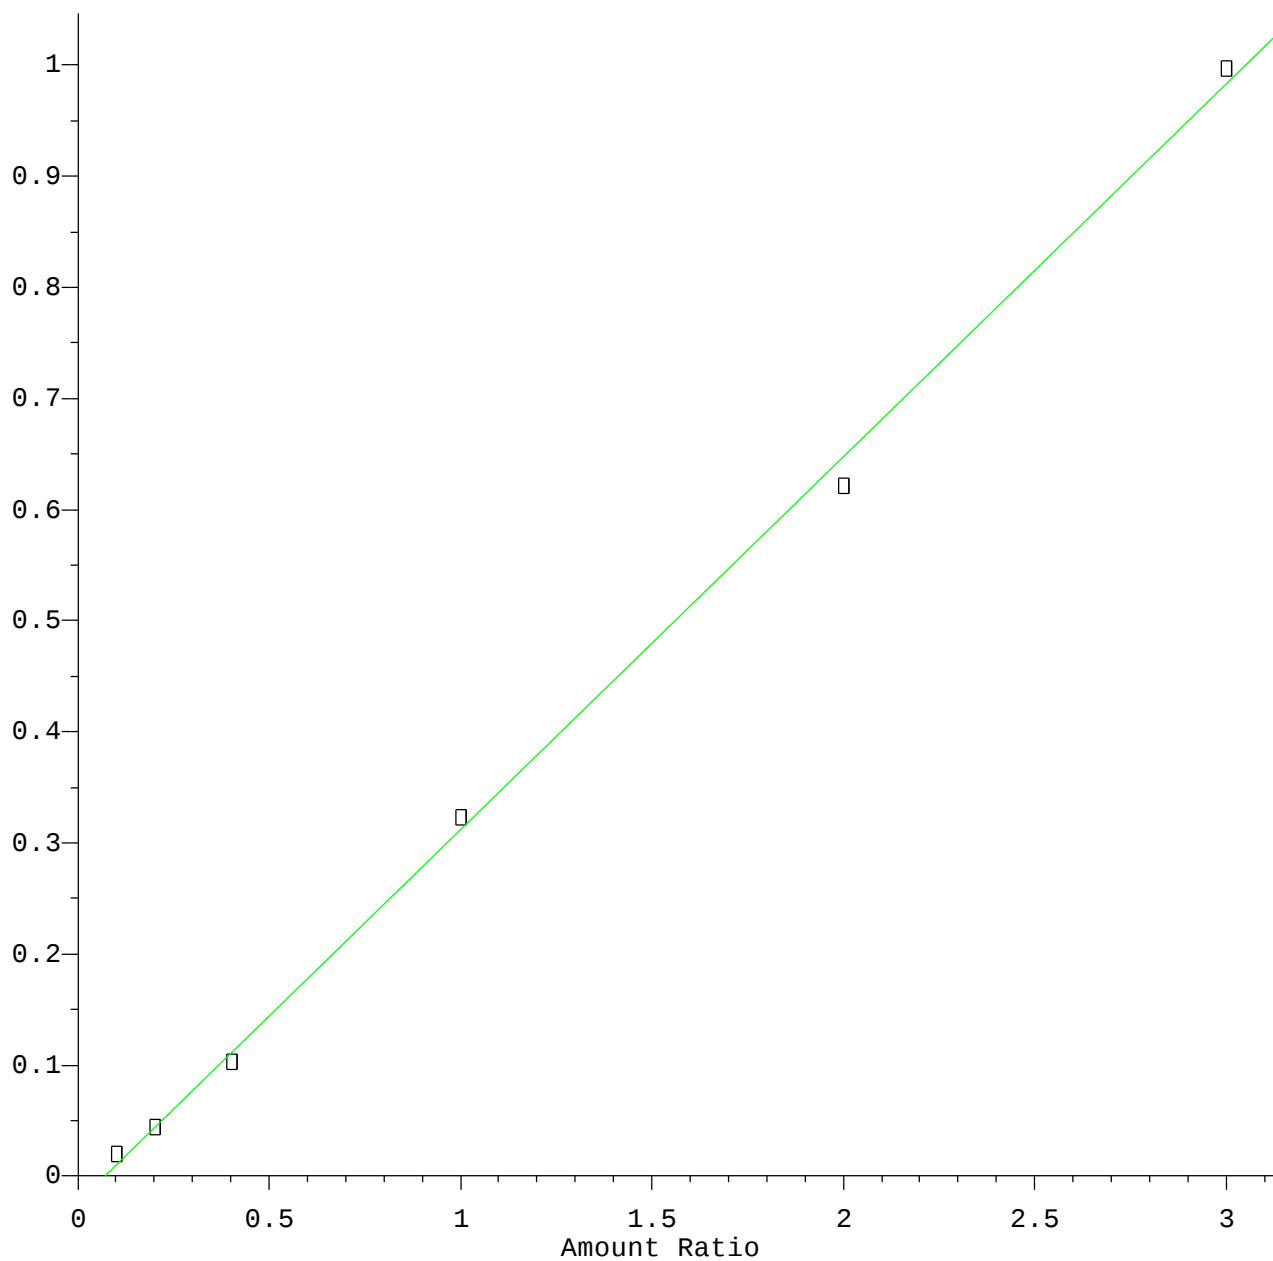

Resp Ratio = $3.35 \times 10^{-1} \times \text{Amt} - 2.33 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D041520S.M
Calibration Table Last Updated: Wed Apr 15 19:43:39 2020

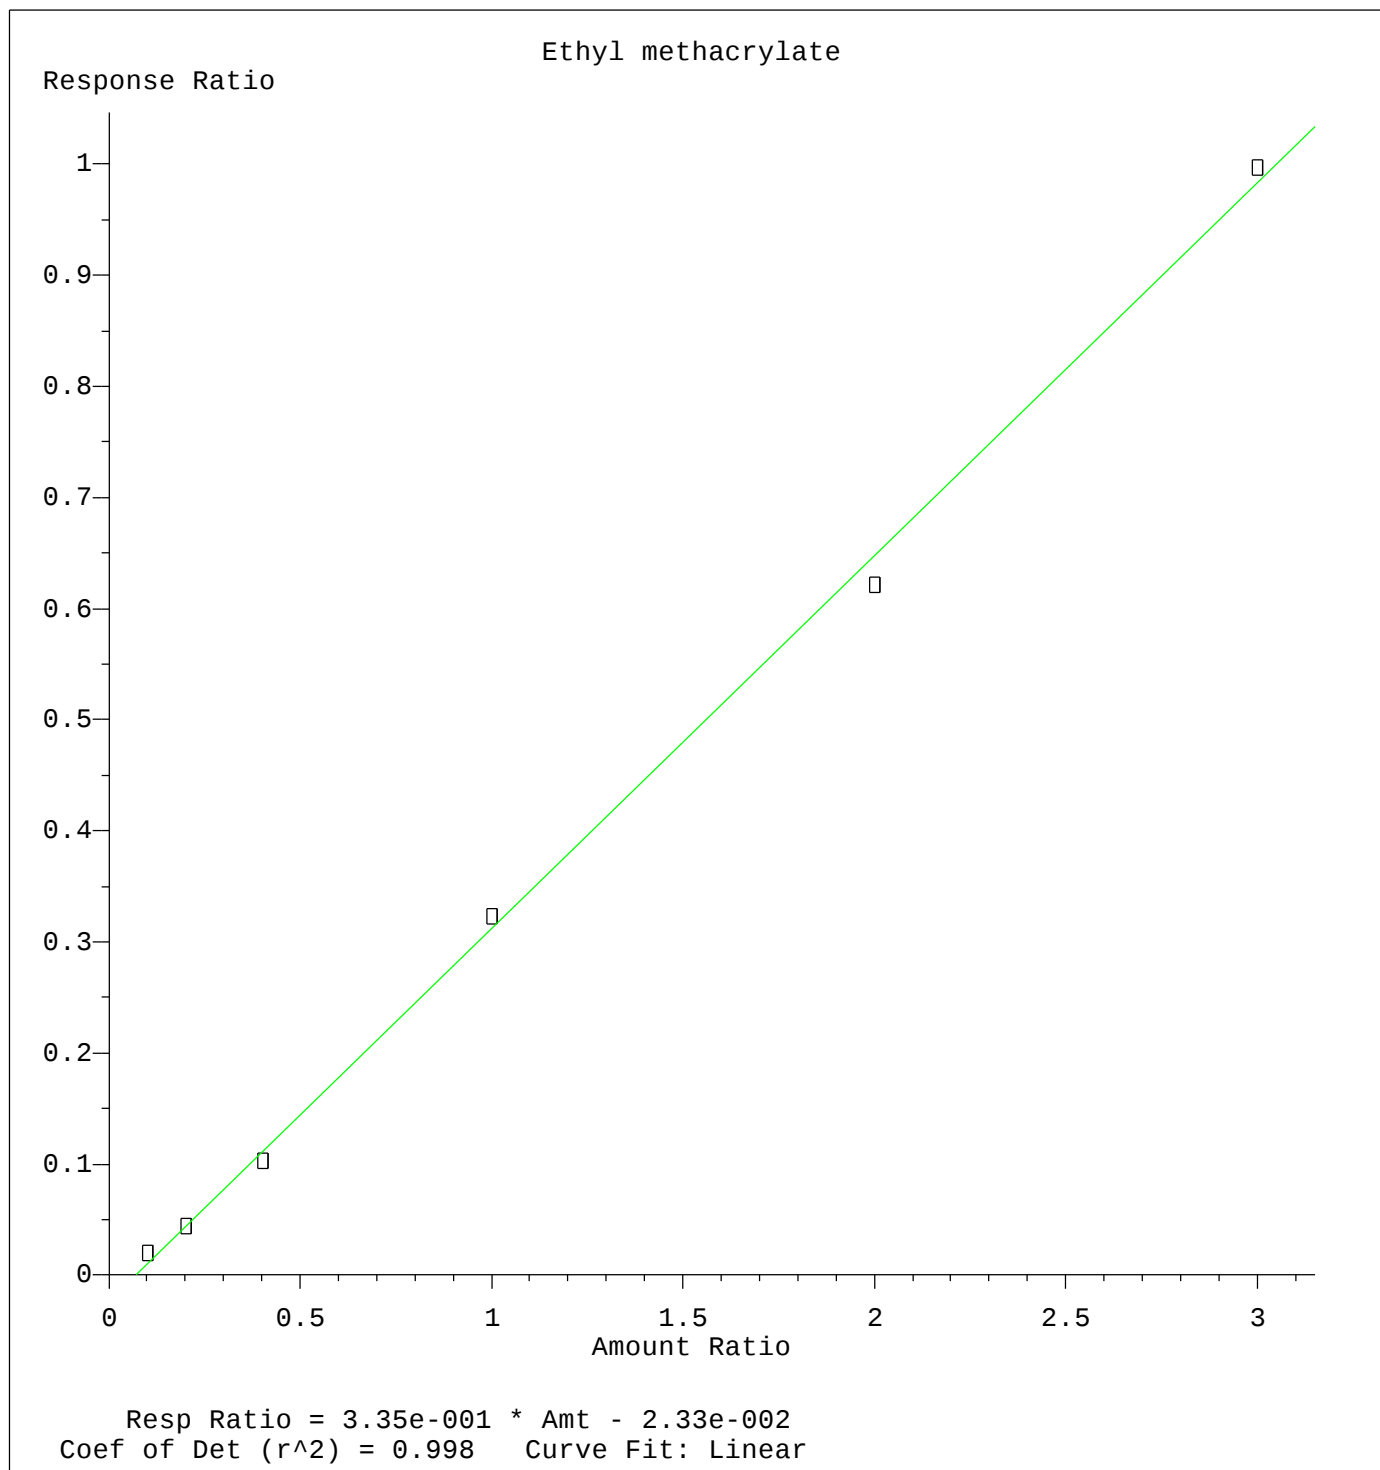

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D041520S.M
Calibration Table Last Updated: Wed Apr 15 19:43:39 2020

2-Chloroethyl Vinyl ether

Response Ratio

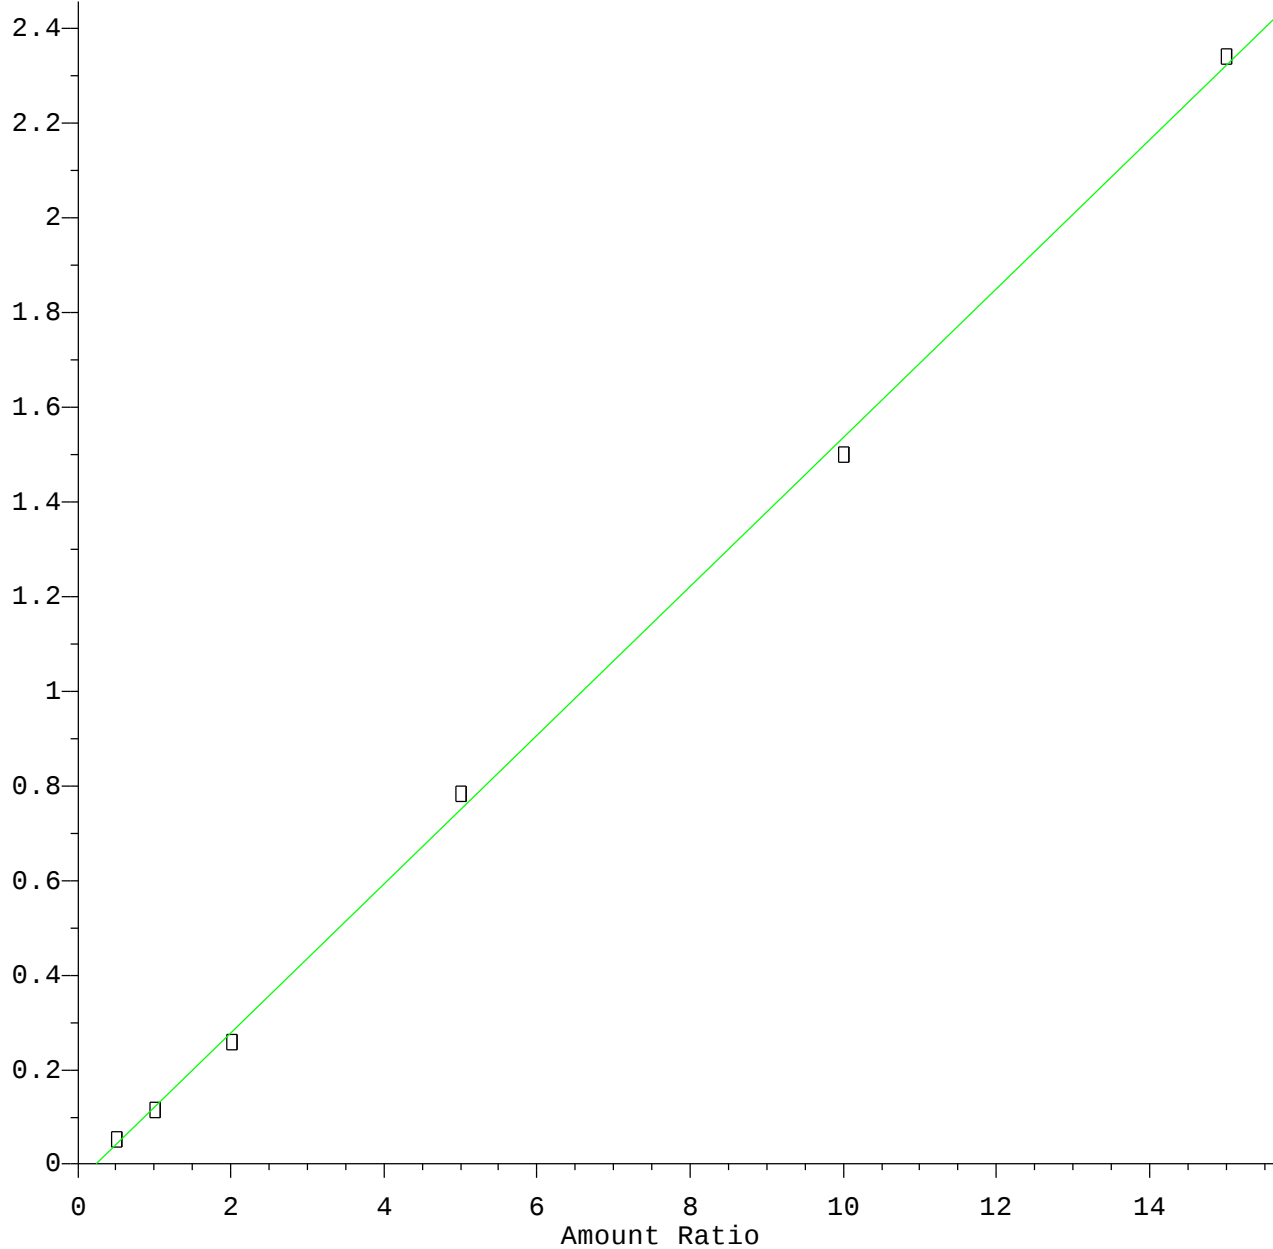


Resp Ratio = $1.57 \times 10^{-1} \times \text{Amt} - 3.86 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D041520S.M
Calibration Table Last Updated: Wed Apr 15 19:43:39 2020

2-Hexanone

Response Ratio

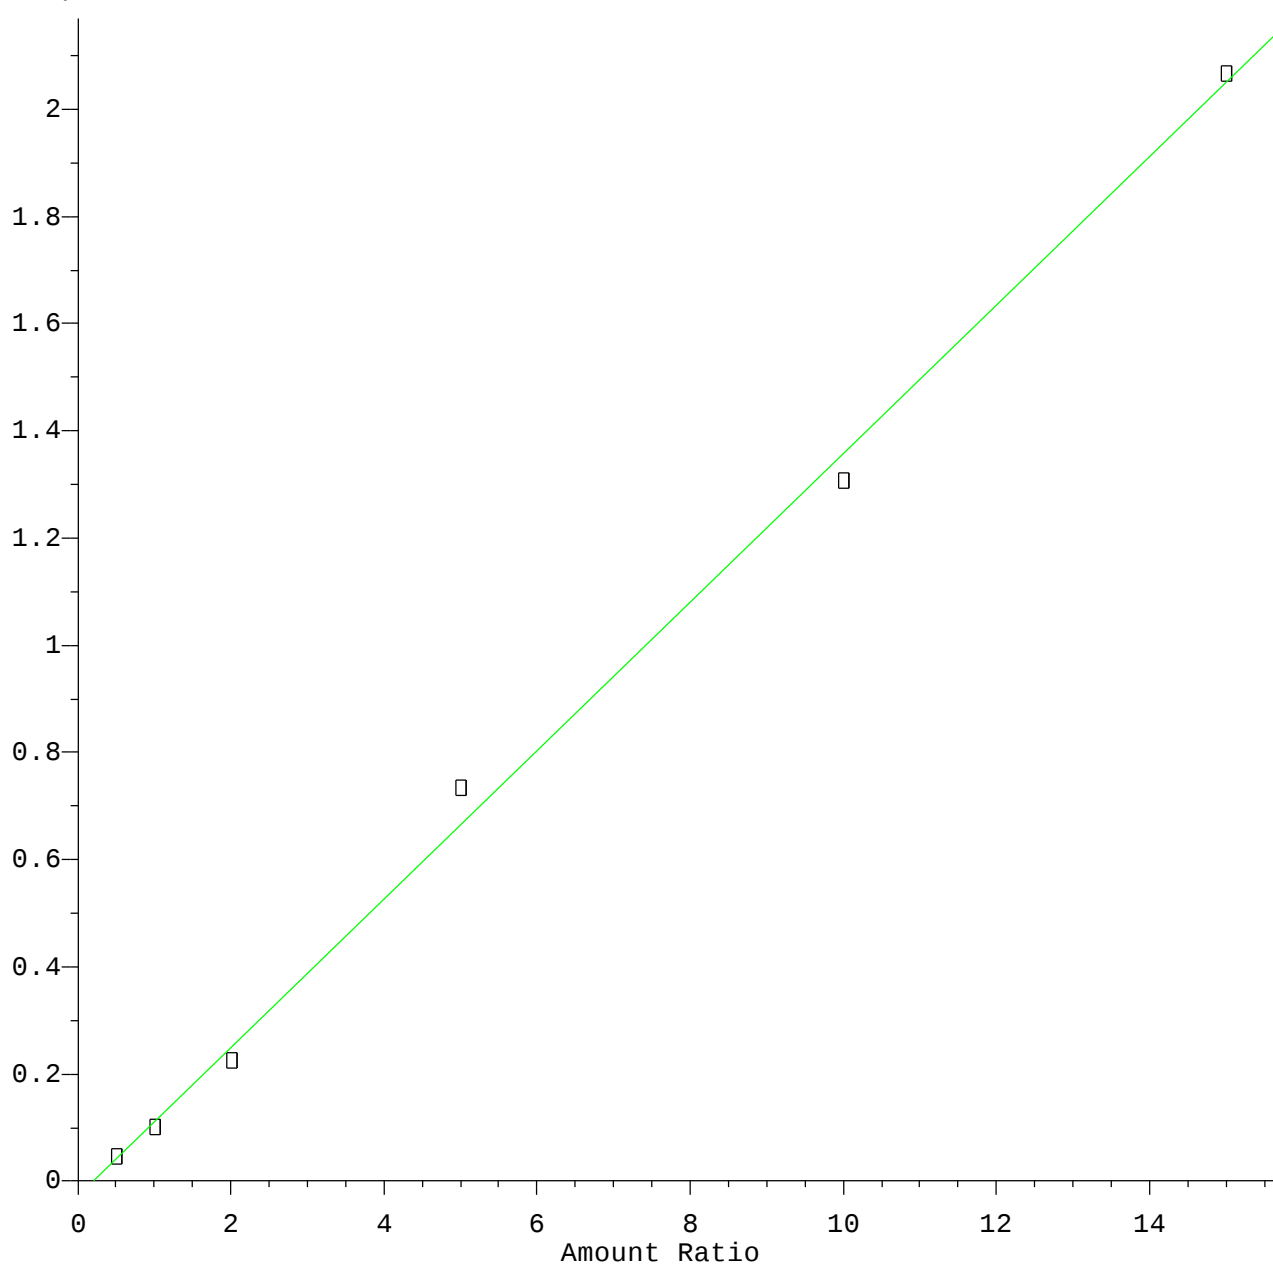


Resp Ratio = $1.38 \times 10^{-1} \times \text{Amt} - 2.76 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D041520S.M
Calibration Table Last Updated: Wed Apr 15 19:43:39 2020


2-Hexanone

Response Ratio

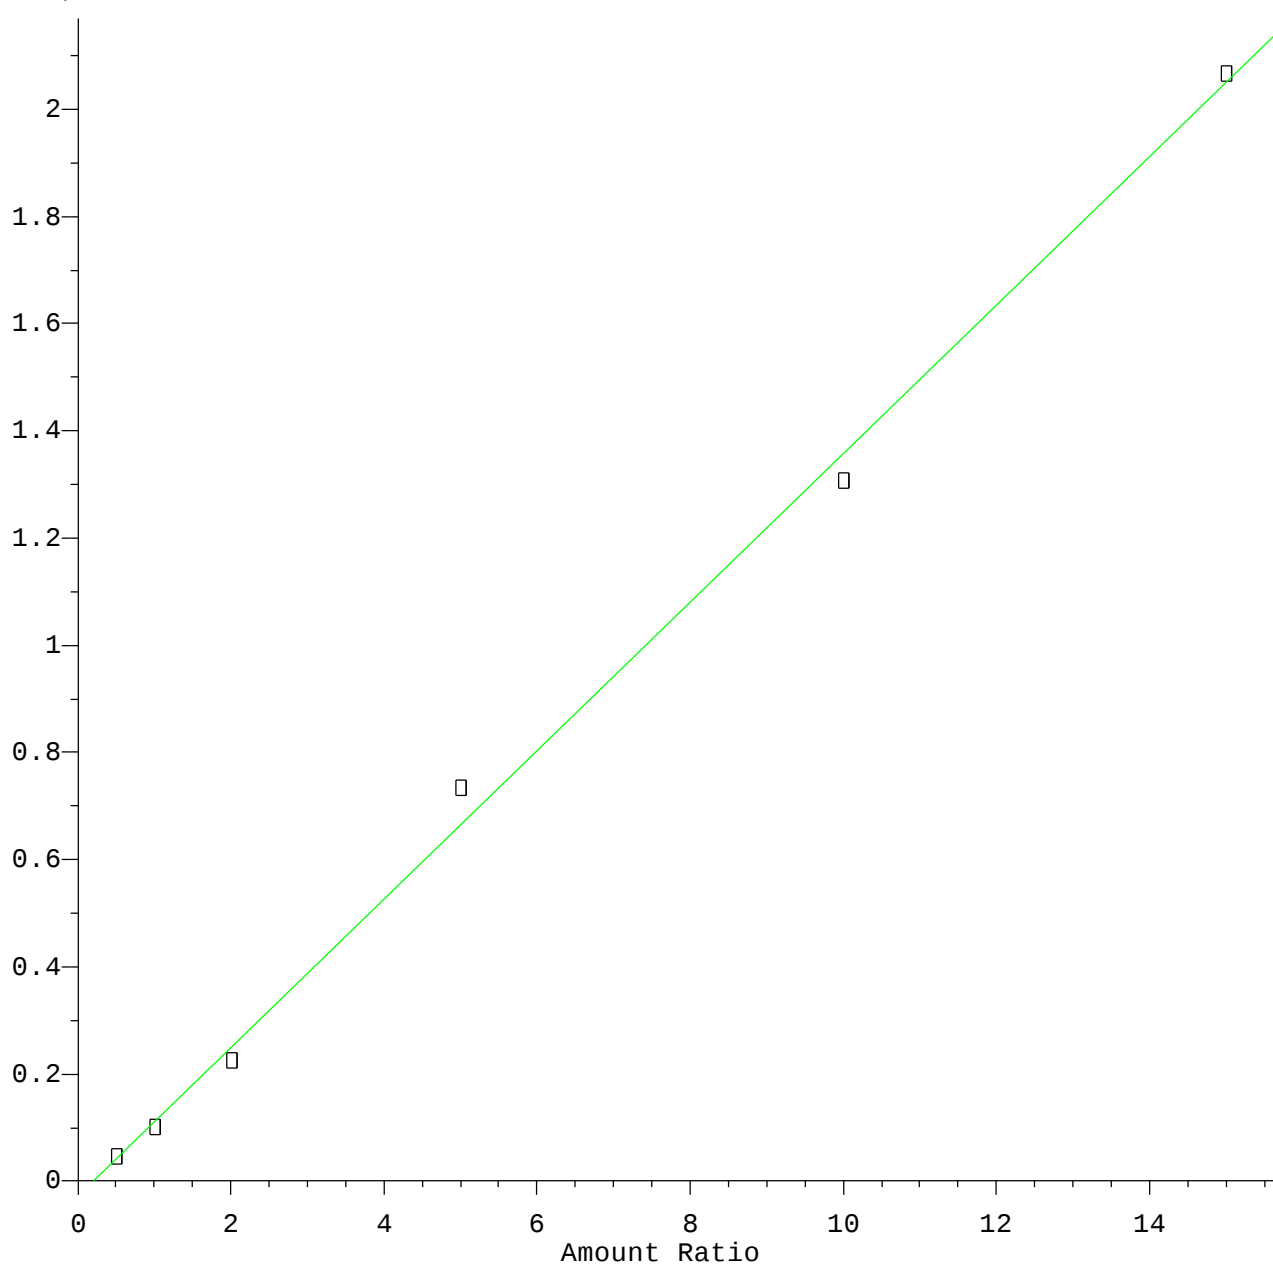

Resp Ratio = $1.38 \times 10^{-1} \times \text{Amt} - 2.76 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D041520S.M
Calibration Table Last Updated: Wed Apr 15 19:43:39 2020

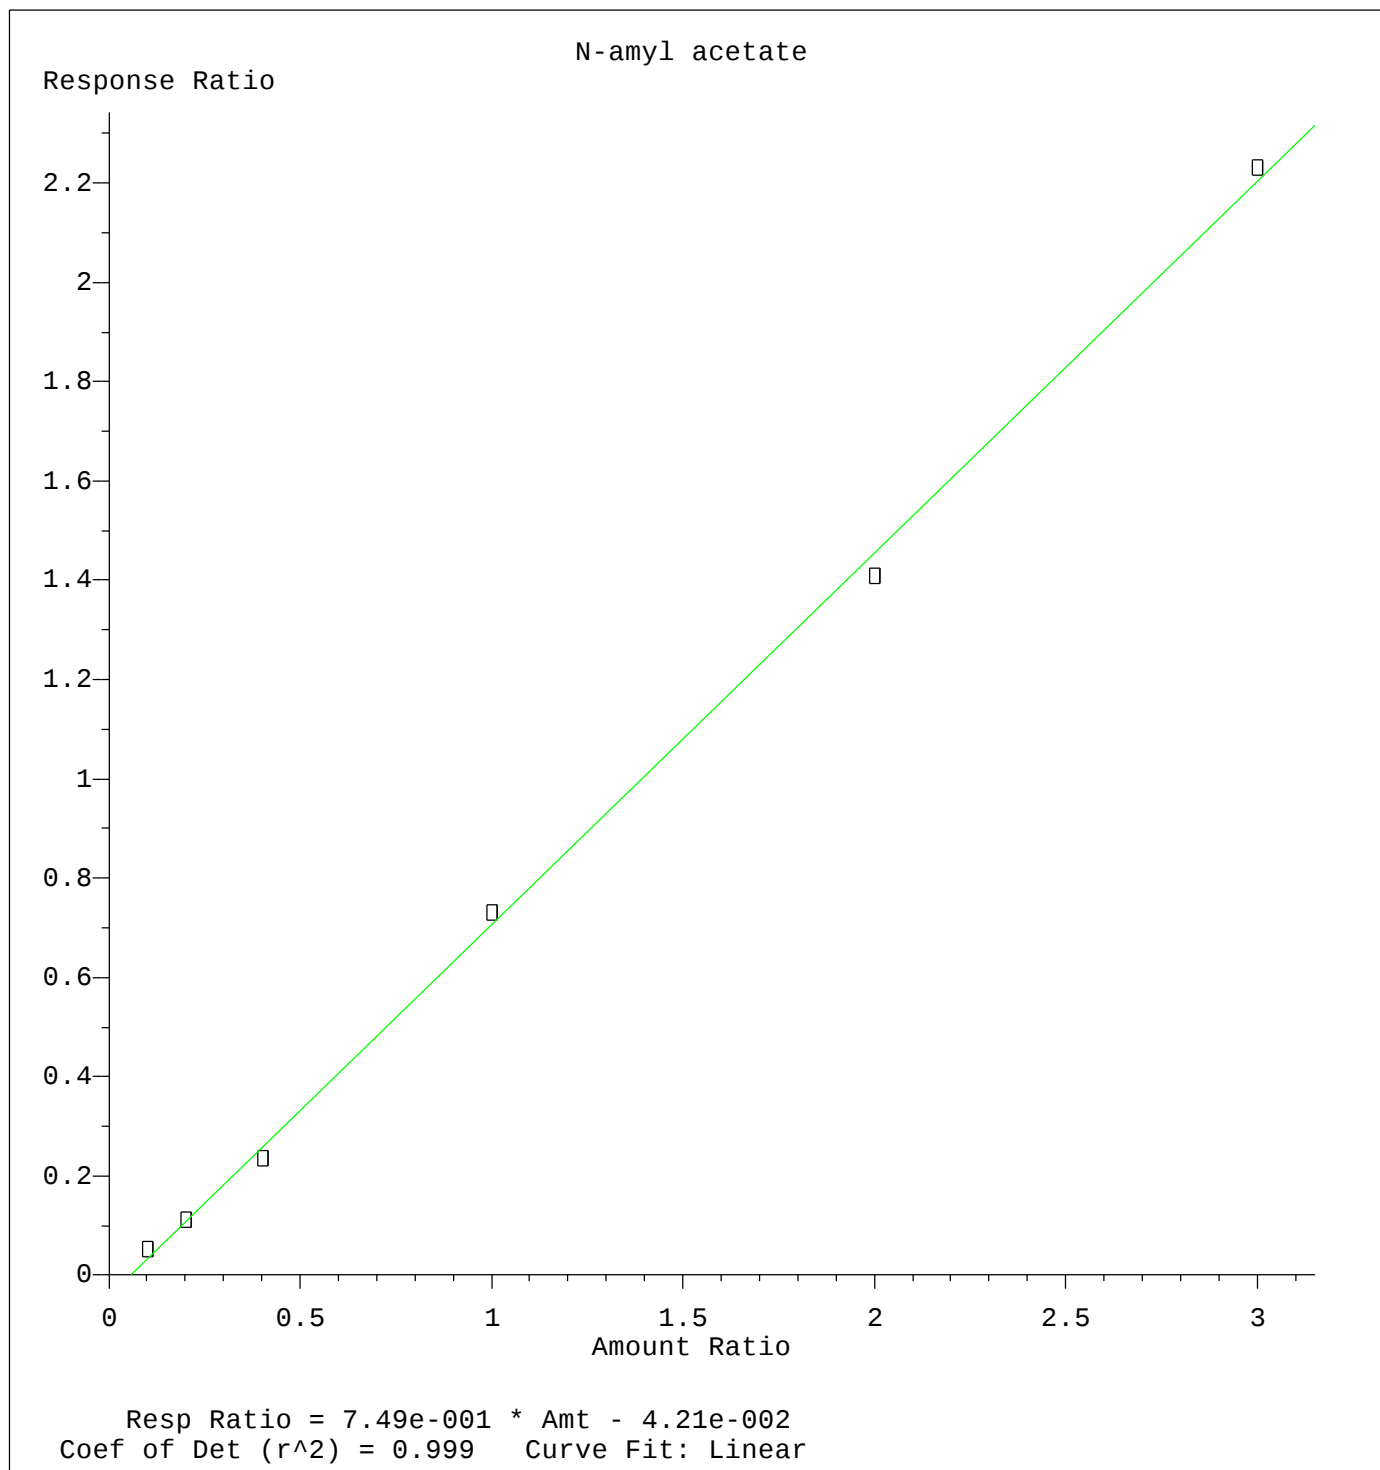

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D041520S.M
Calibration Table Last Updated: Wed Apr 15 19:43:39 2020


Naphthalene

Response Ratio

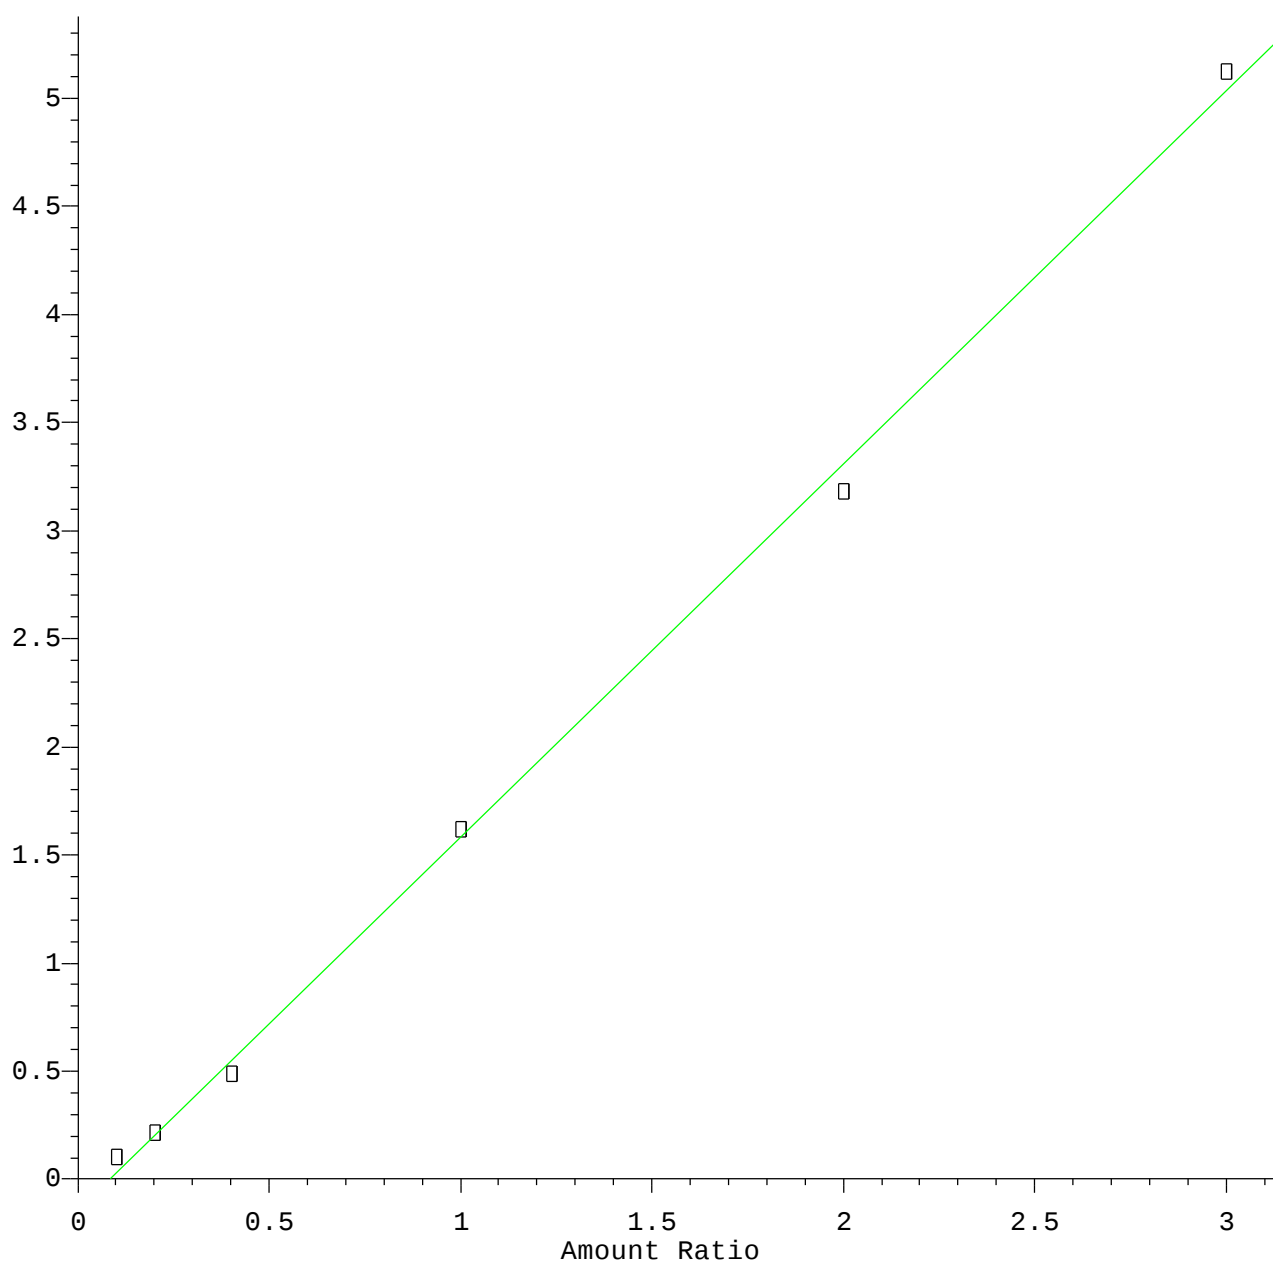


Resp Ratio = 1.73e+000 * Amt - 1.42e-001
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D041520S.M
Calibration Table Last Updated: Wed Apr 15 19:43:39 2020

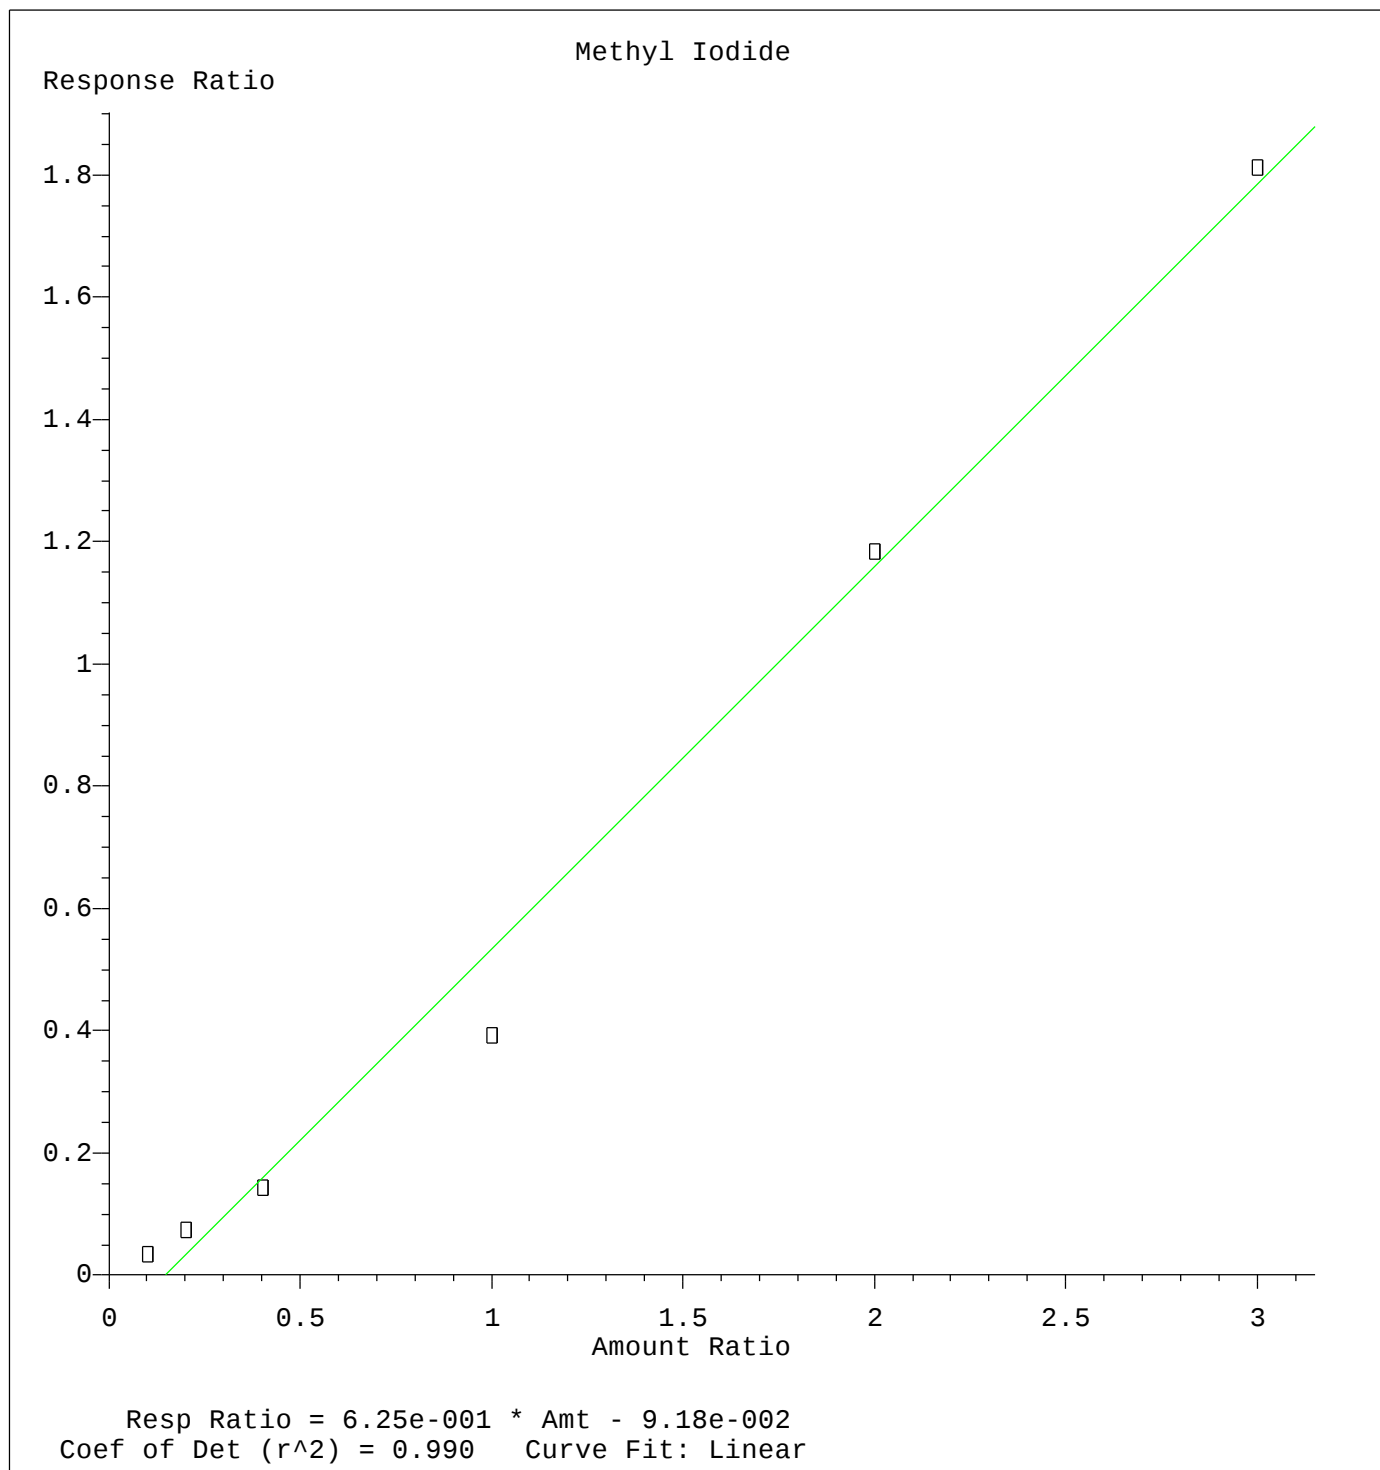


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D041520S.M
Calibration Table Last Updated: Wed Apr 15 19:43:39 2020

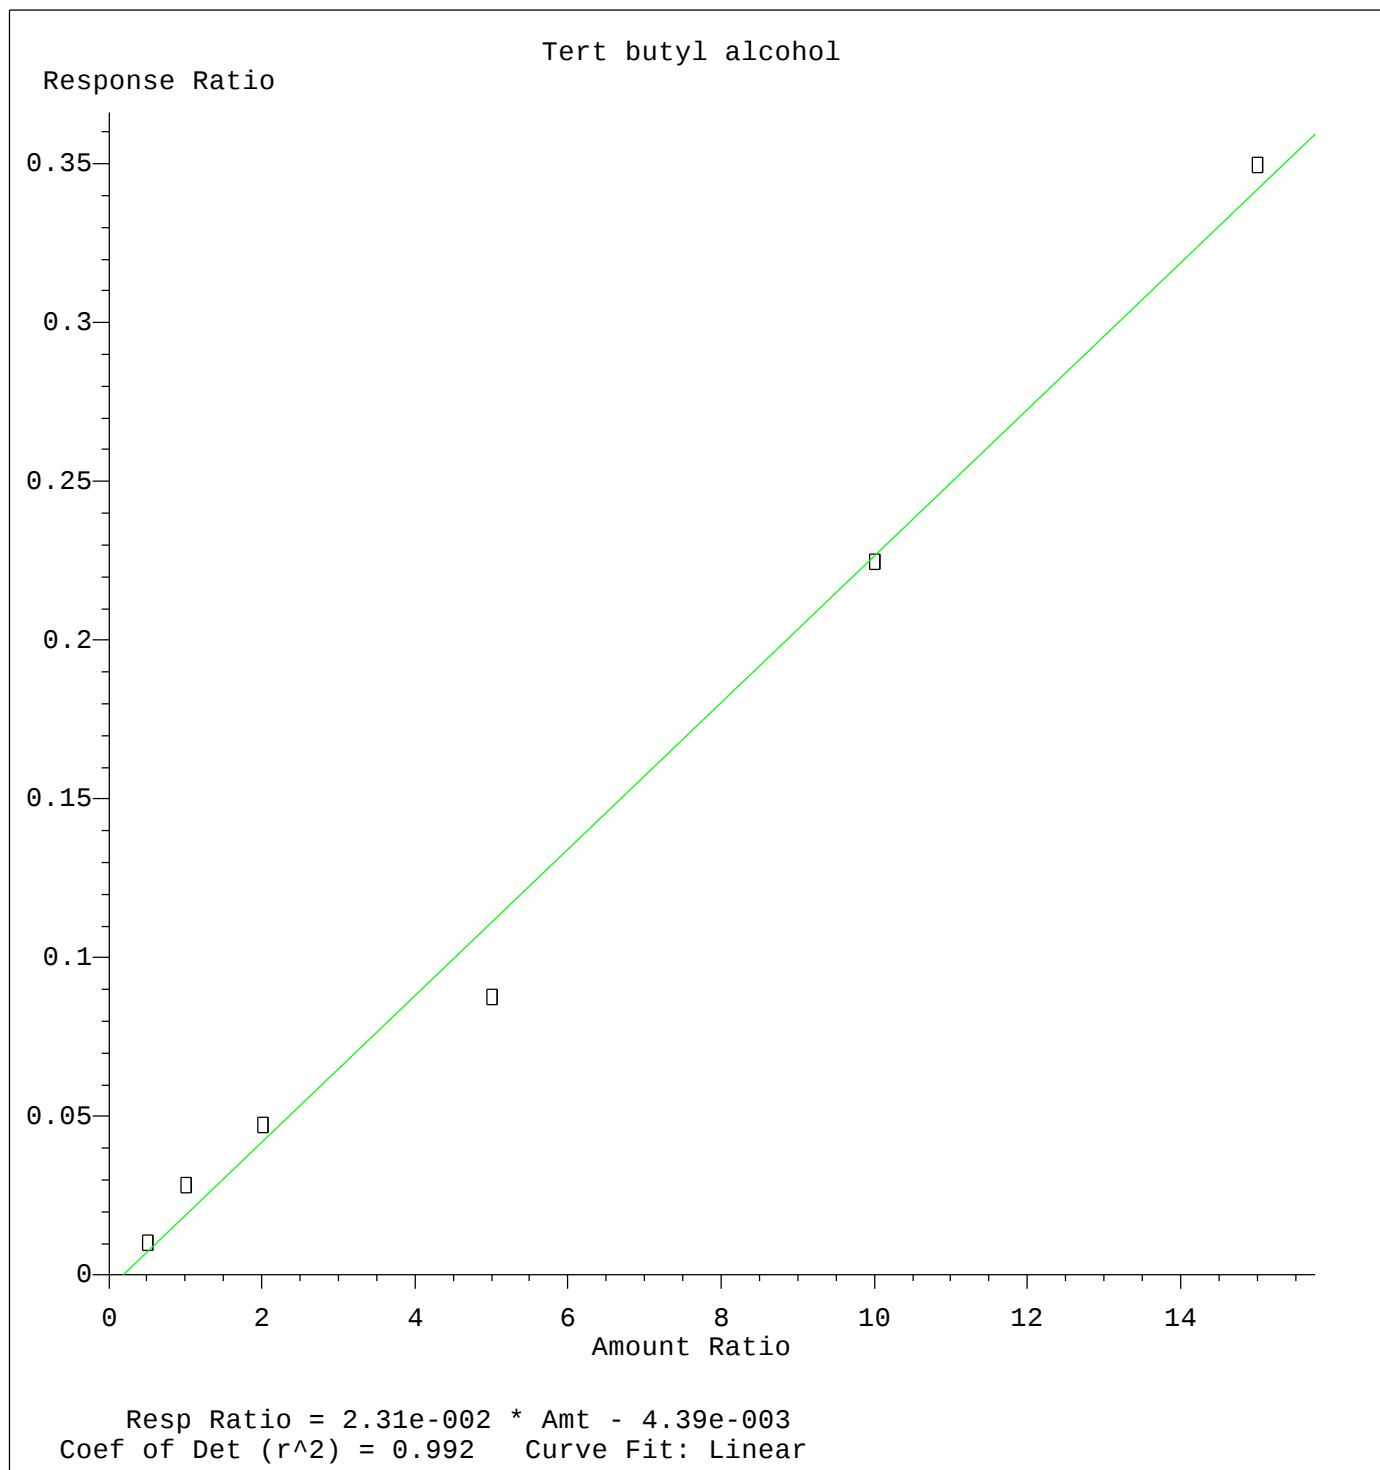

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D041520S.M
Calibration Table Last Updated: Wed Apr 15 19:43:39 2020


Allyl chloride

Response Ratio

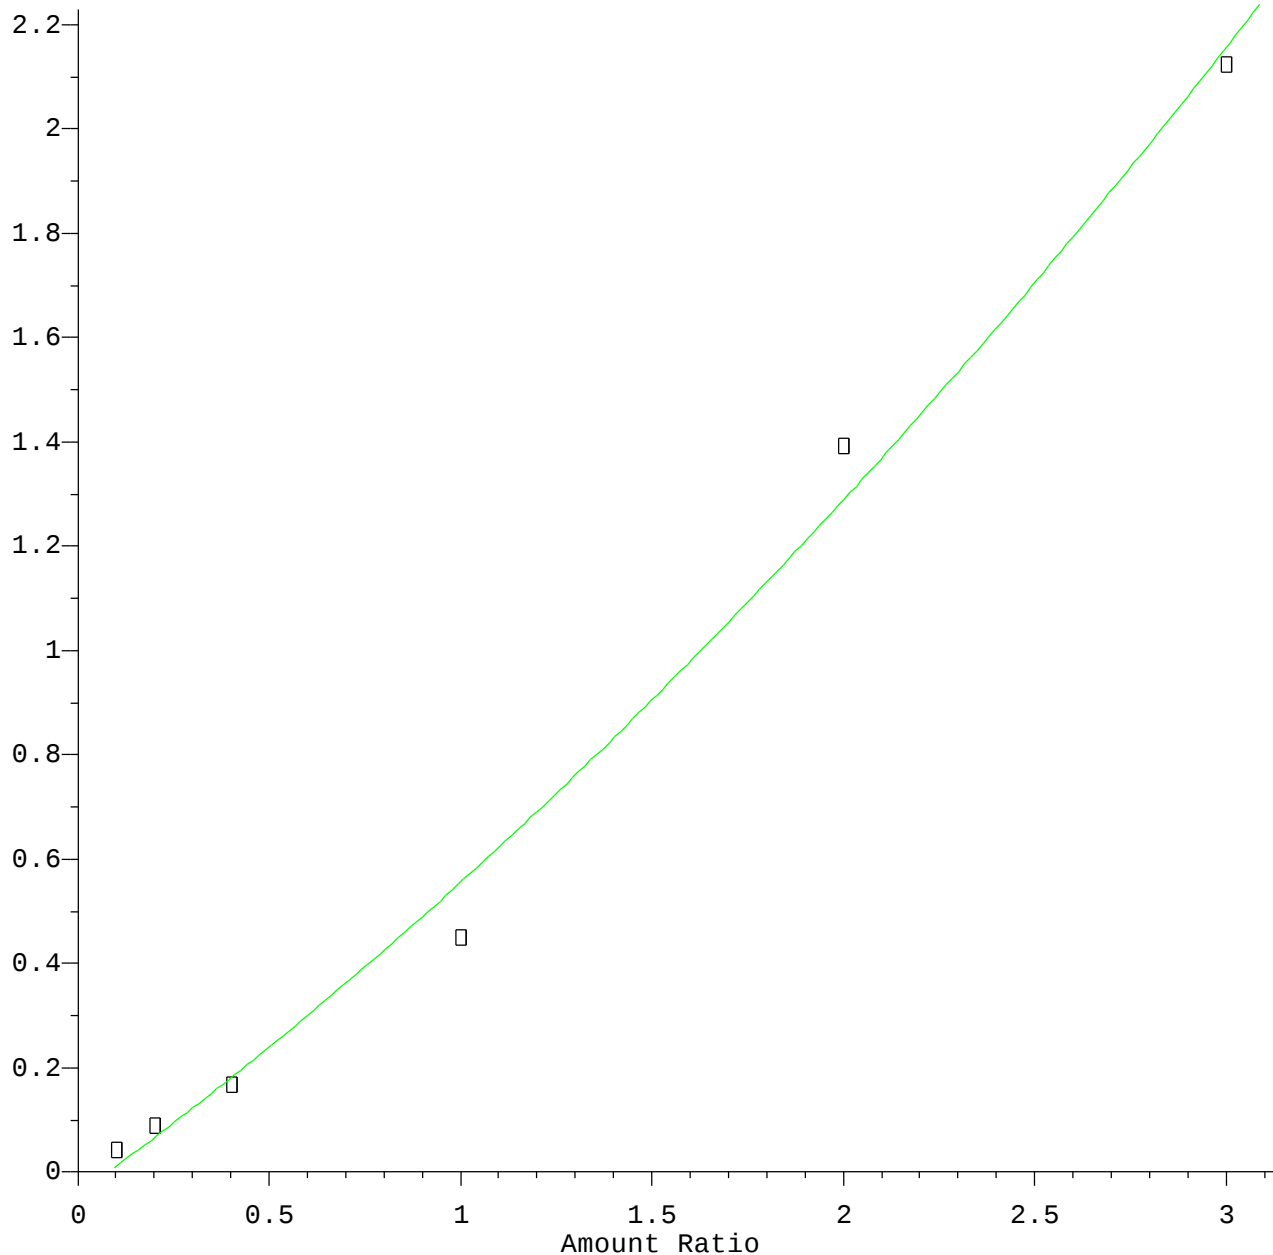


$R = 6.75e-002 A^2 + 5.31e-001 A - 4.24e-002$
Coef of Det (r^2) = 0.993 Curve Fit: Quadratic

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D041520S.M
Calibration Table Last Updated: Wed Apr 15 19:43:39 2020

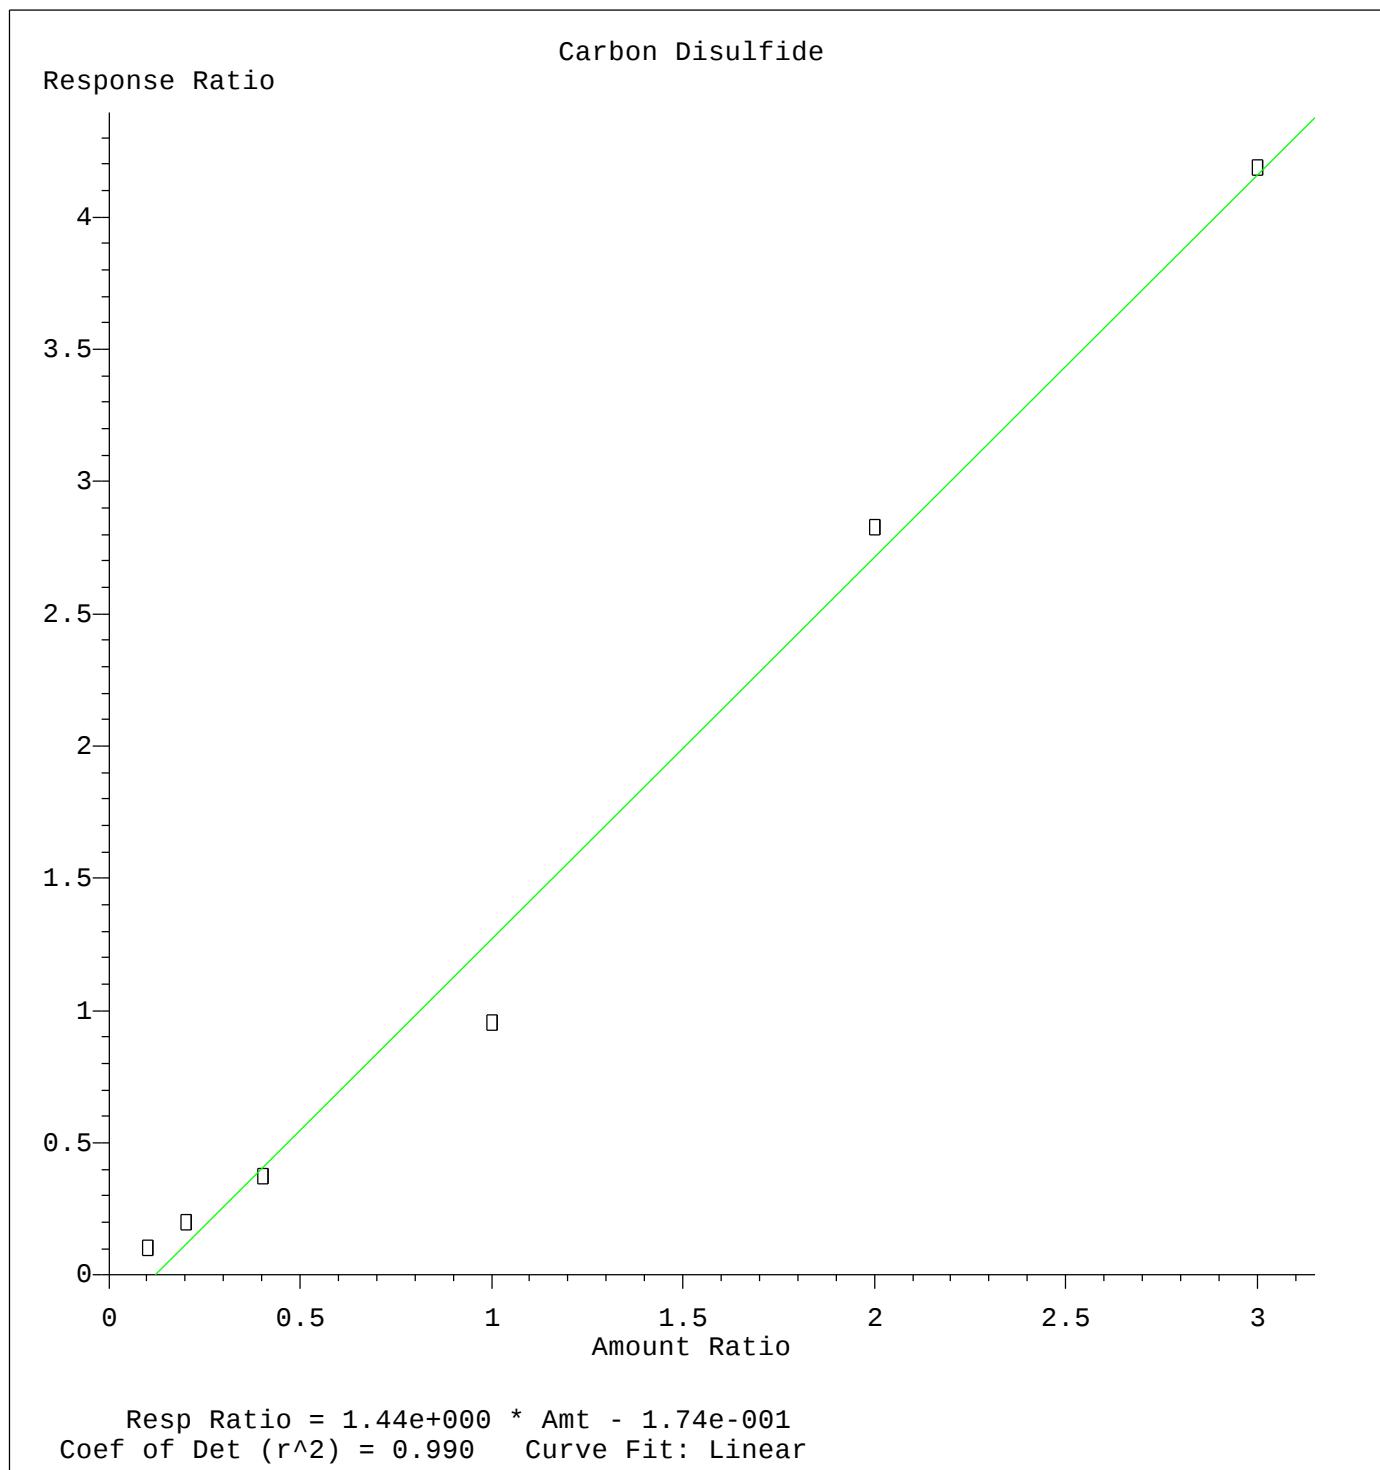


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D041520S.M
Calibration Table Last Updated: Wed Apr 15 19:43:39 2020

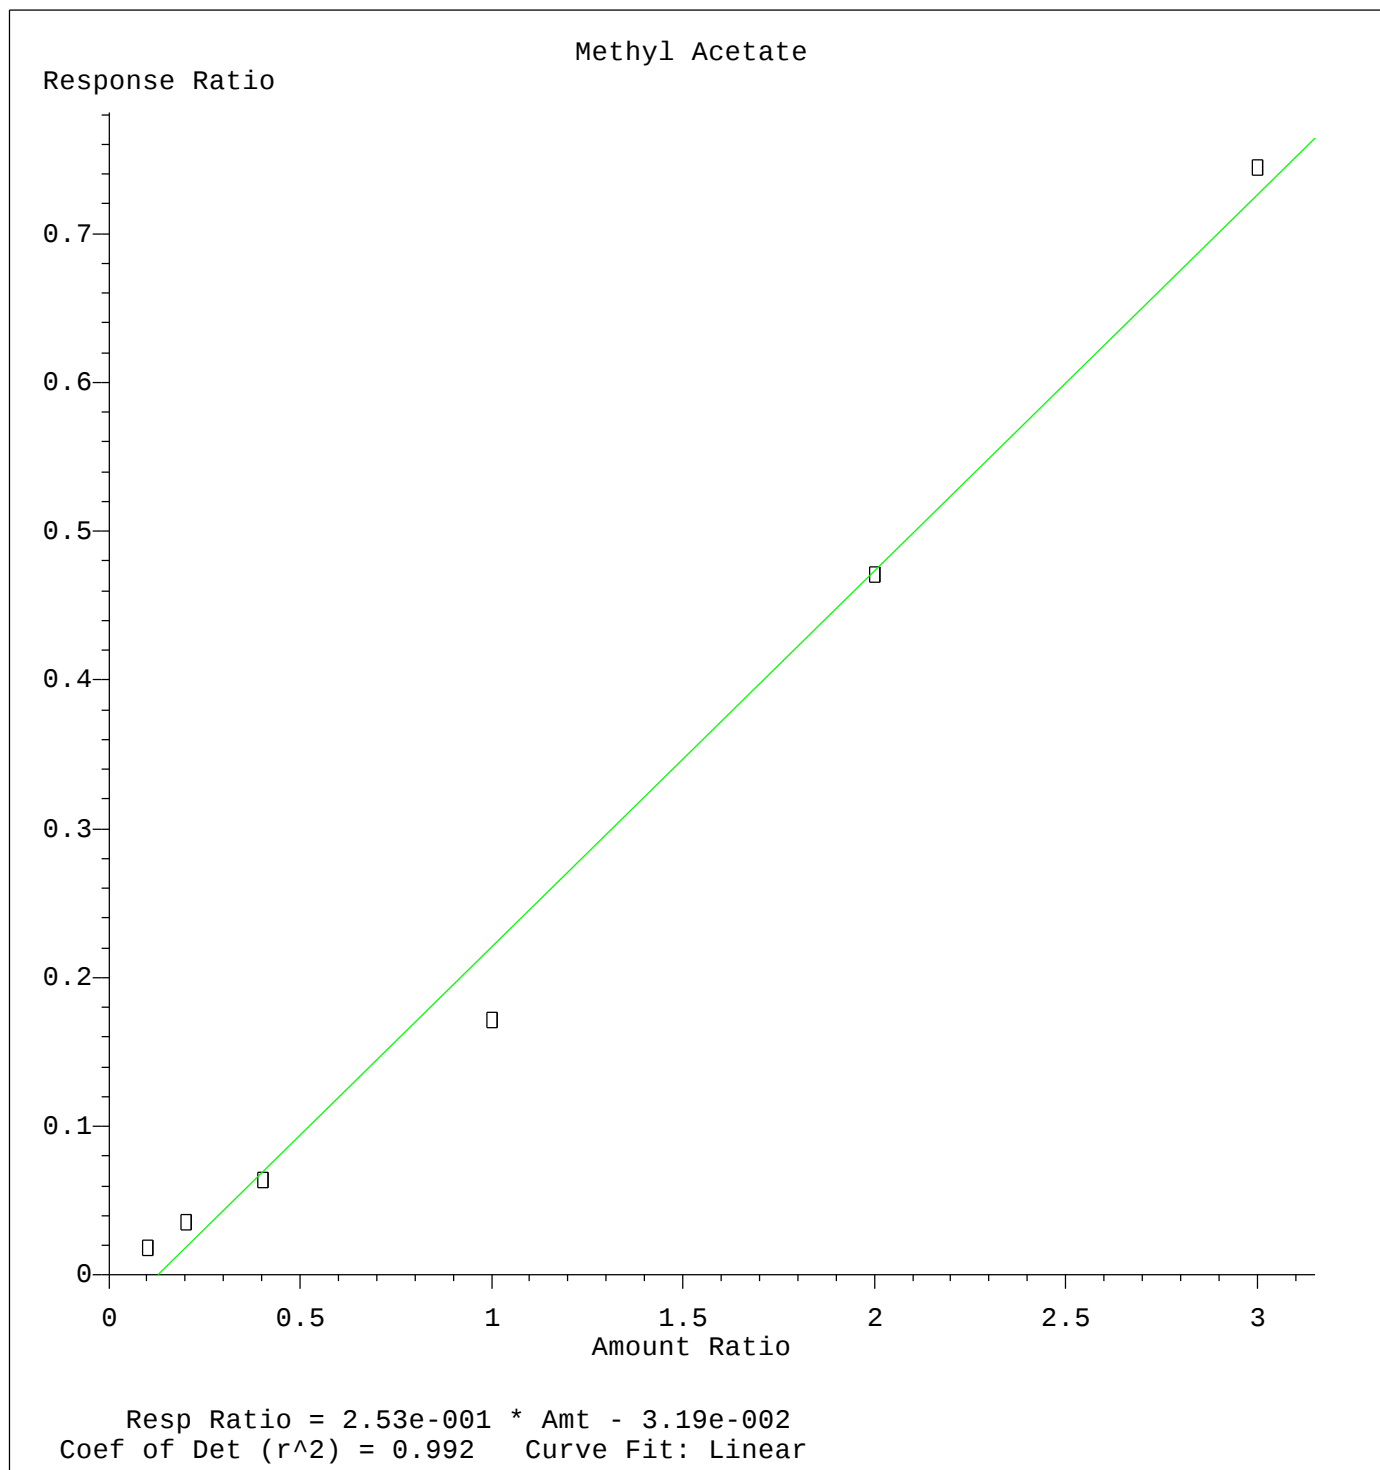

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D041520S.M
Calibration Table Last Updated: Wed Apr 15 19:43:39 2020

Methylene Chloride

Response Ratio

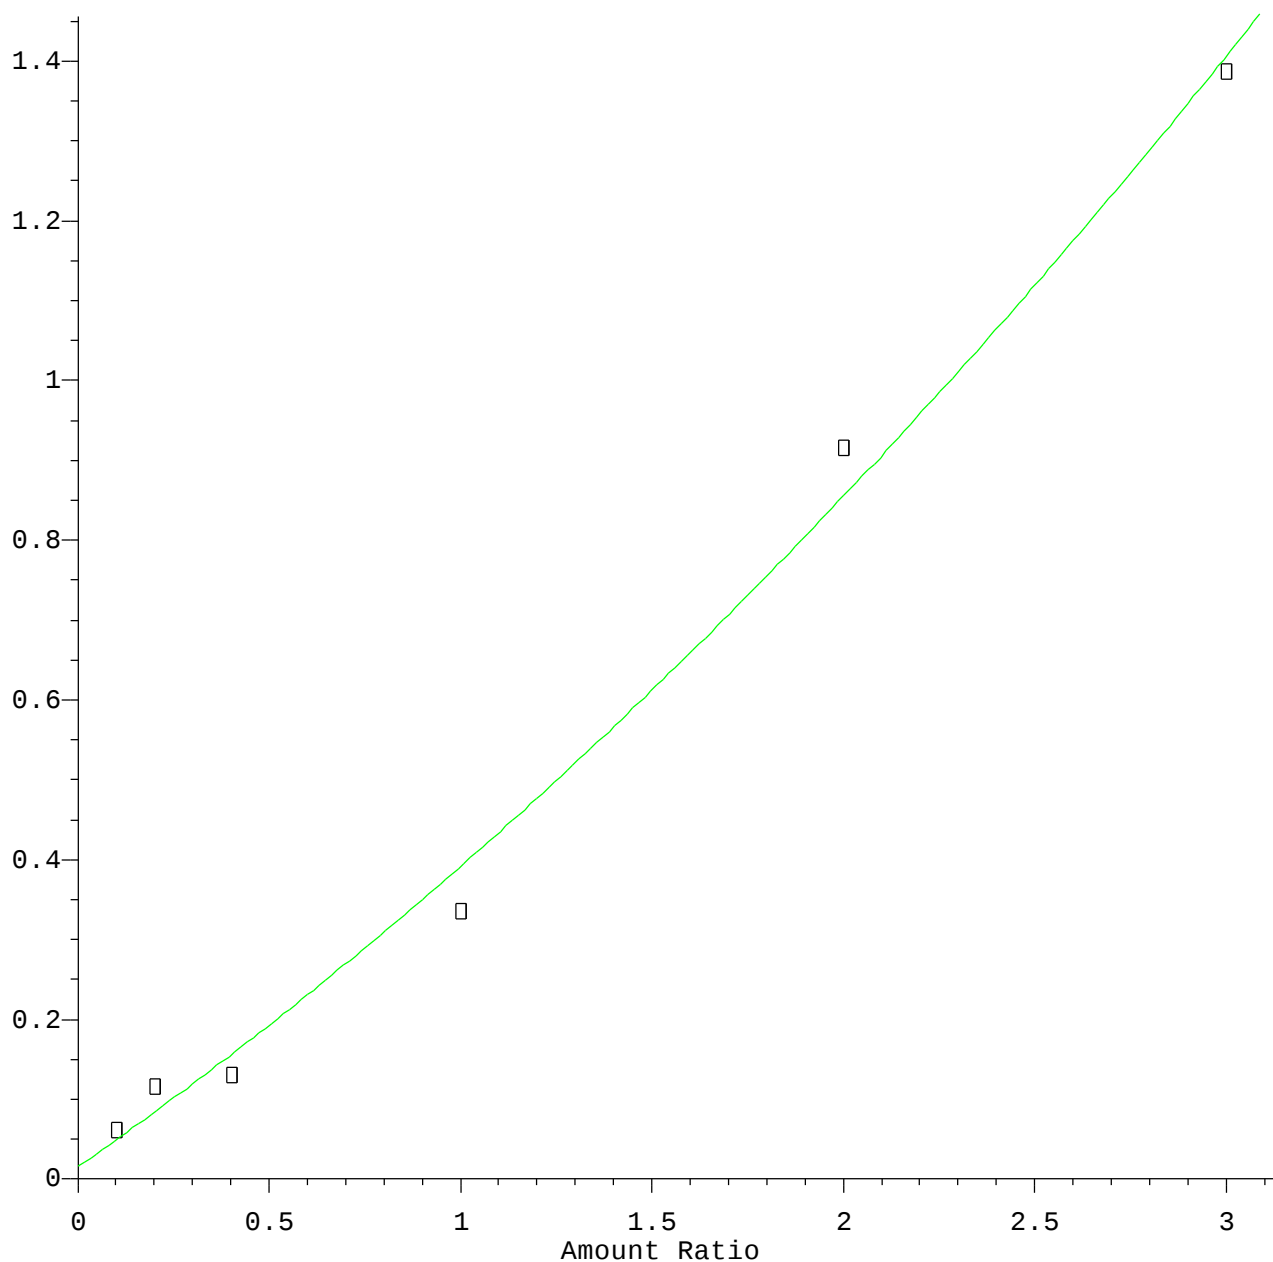


$R = 4.37e-002 A^2 + 3.32e-001 A + 1.56e-002$
Coef of Det (r^2) = 0.994 Curve Fit: Quadratic

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D041520S.M
Calibration Table Last Updated: Wed Apr 15 19:43:39 2020

Methylene Chloride

Response Ratio

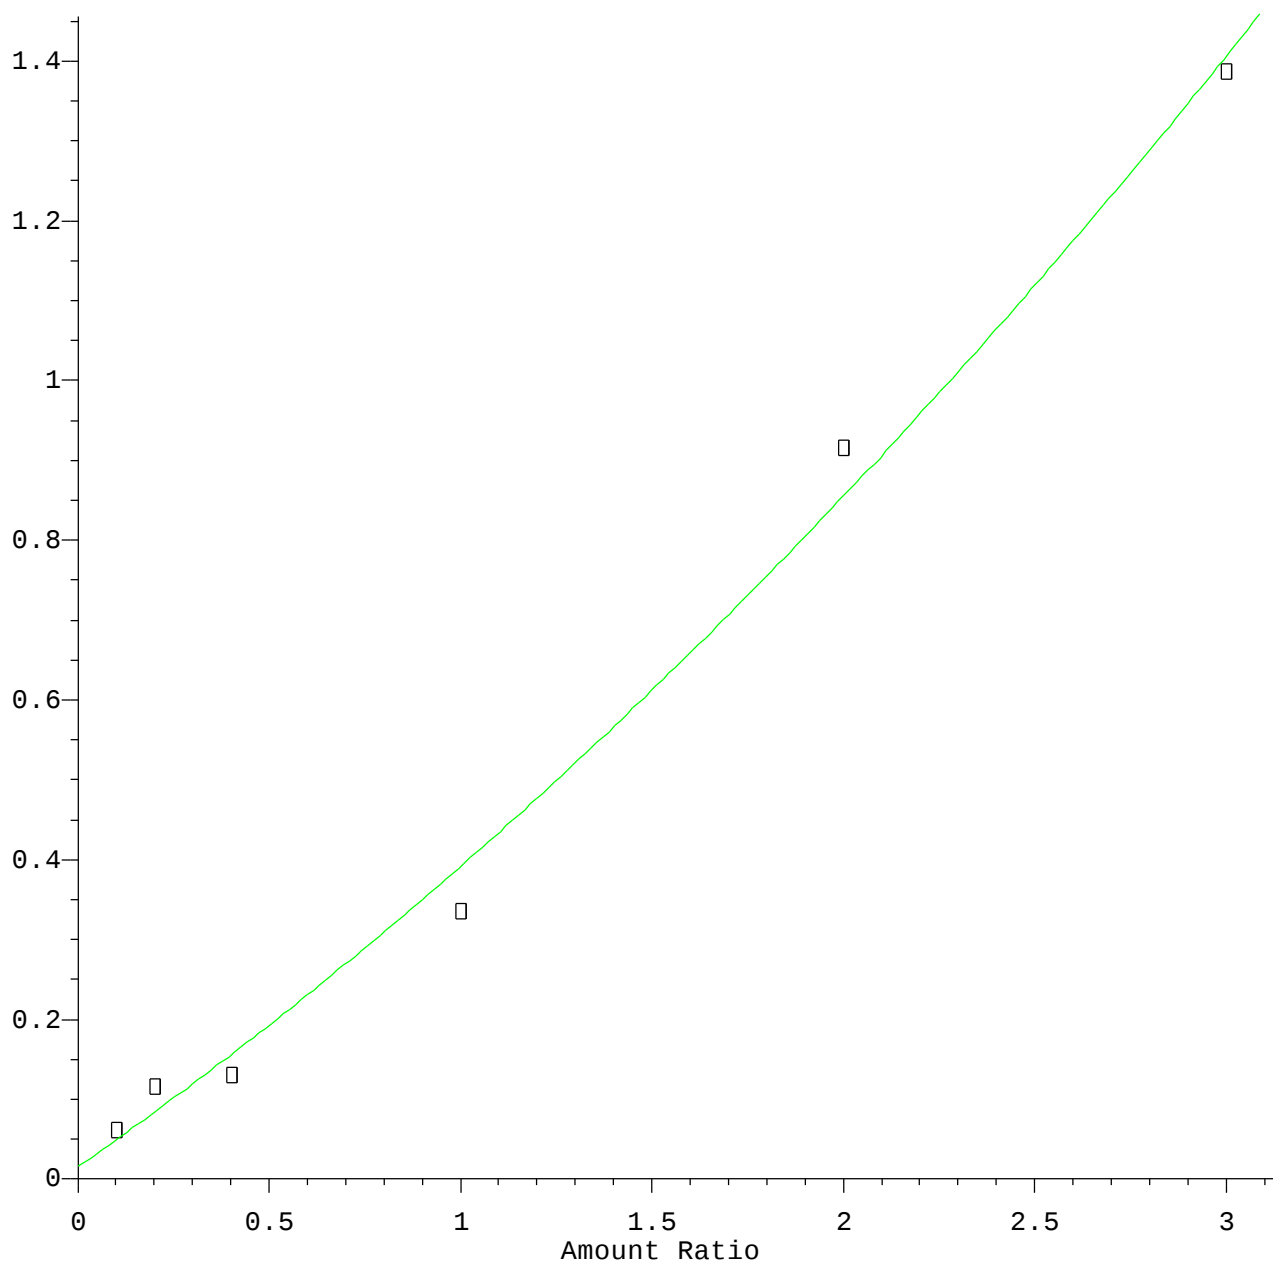


$R = 4.37e-002 A^2 + 3.32e-001 A + 1.56e-002$
Coef of Det (r^2) = 0.994 Curve Fit: Quadratic

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D041520S.M
Calibration Table Last Updated: Wed Apr 15 19:43:39 2020


Vinyl Acetate

Response Ratio

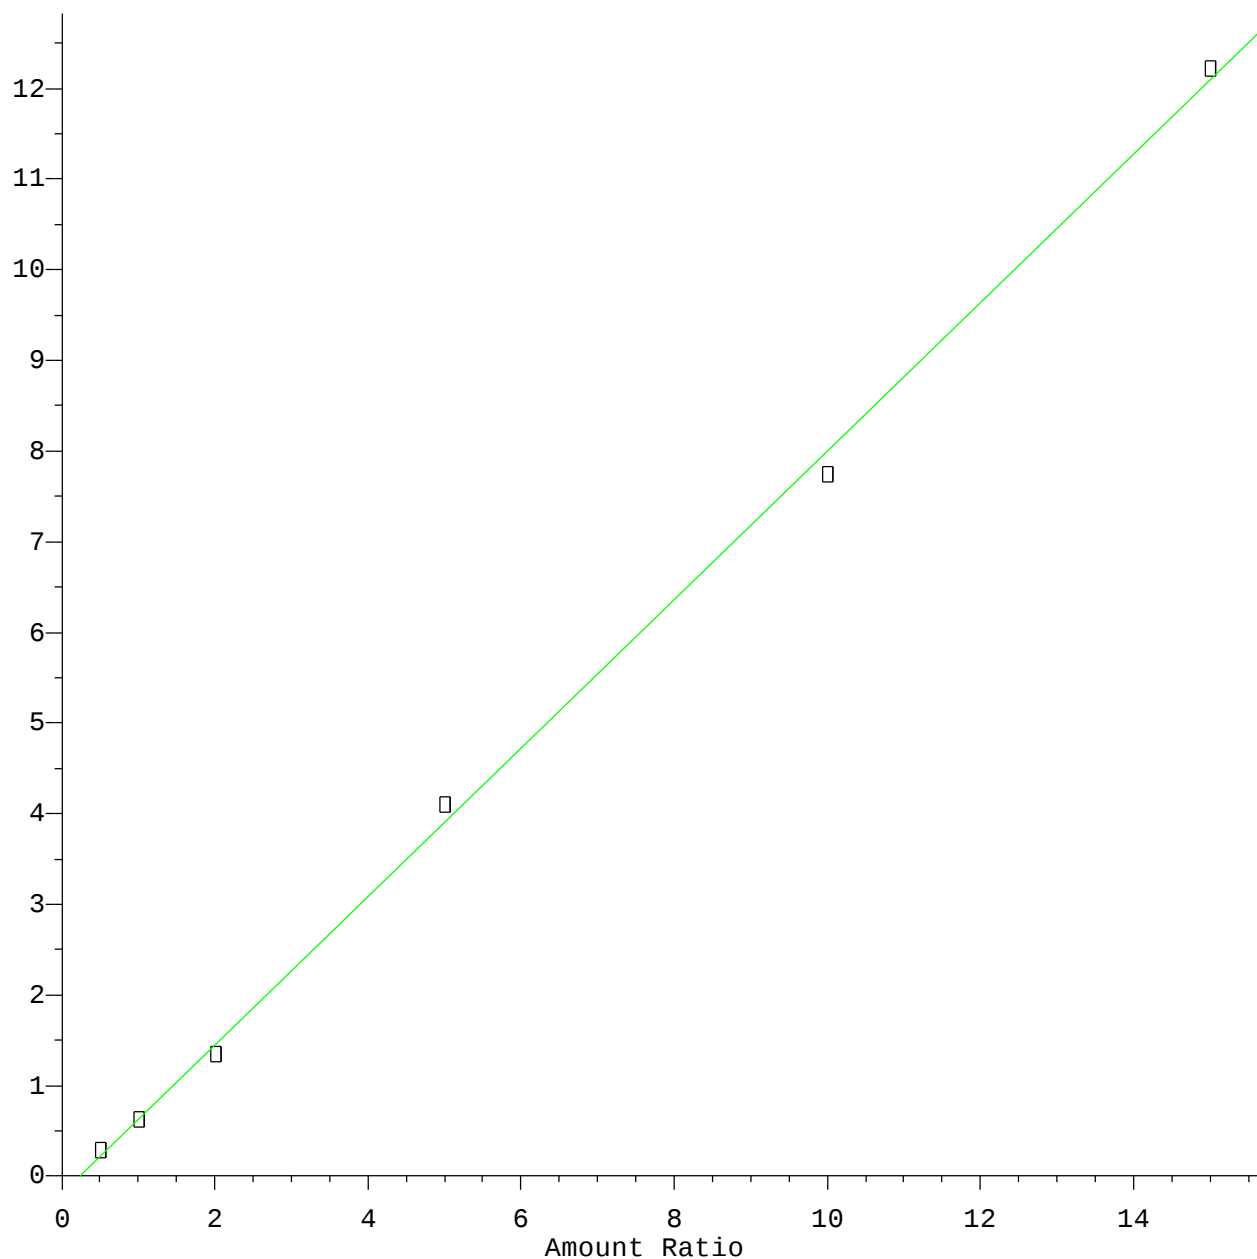


Resp Ratio = $8.19 \times 10^{-1} \times \text{Amt} - 1.90 \times 10^{-1}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D041520S.M
Calibration Table Last Updated: Wed Apr 15 19:43:39 2020

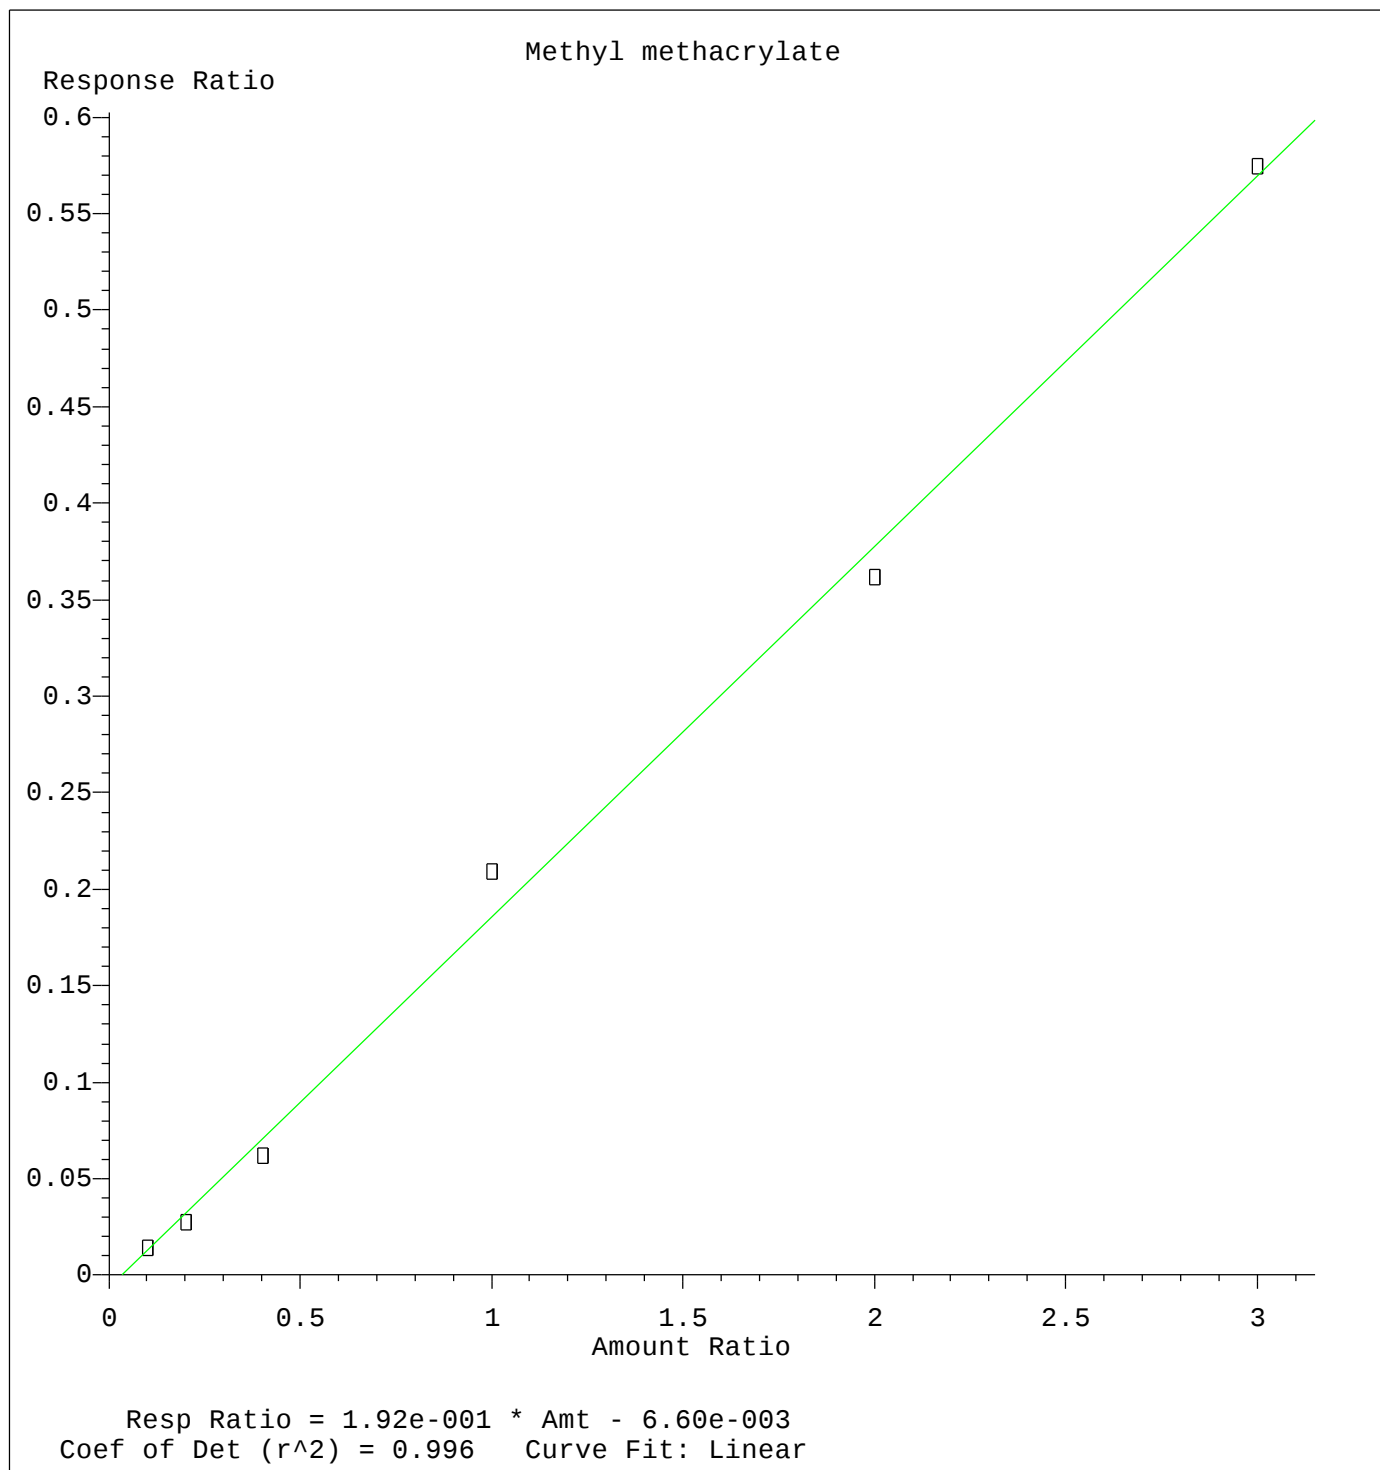

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D041520S.M
Calibration Table Last Updated: Wed Apr 15 19:43:39 2020

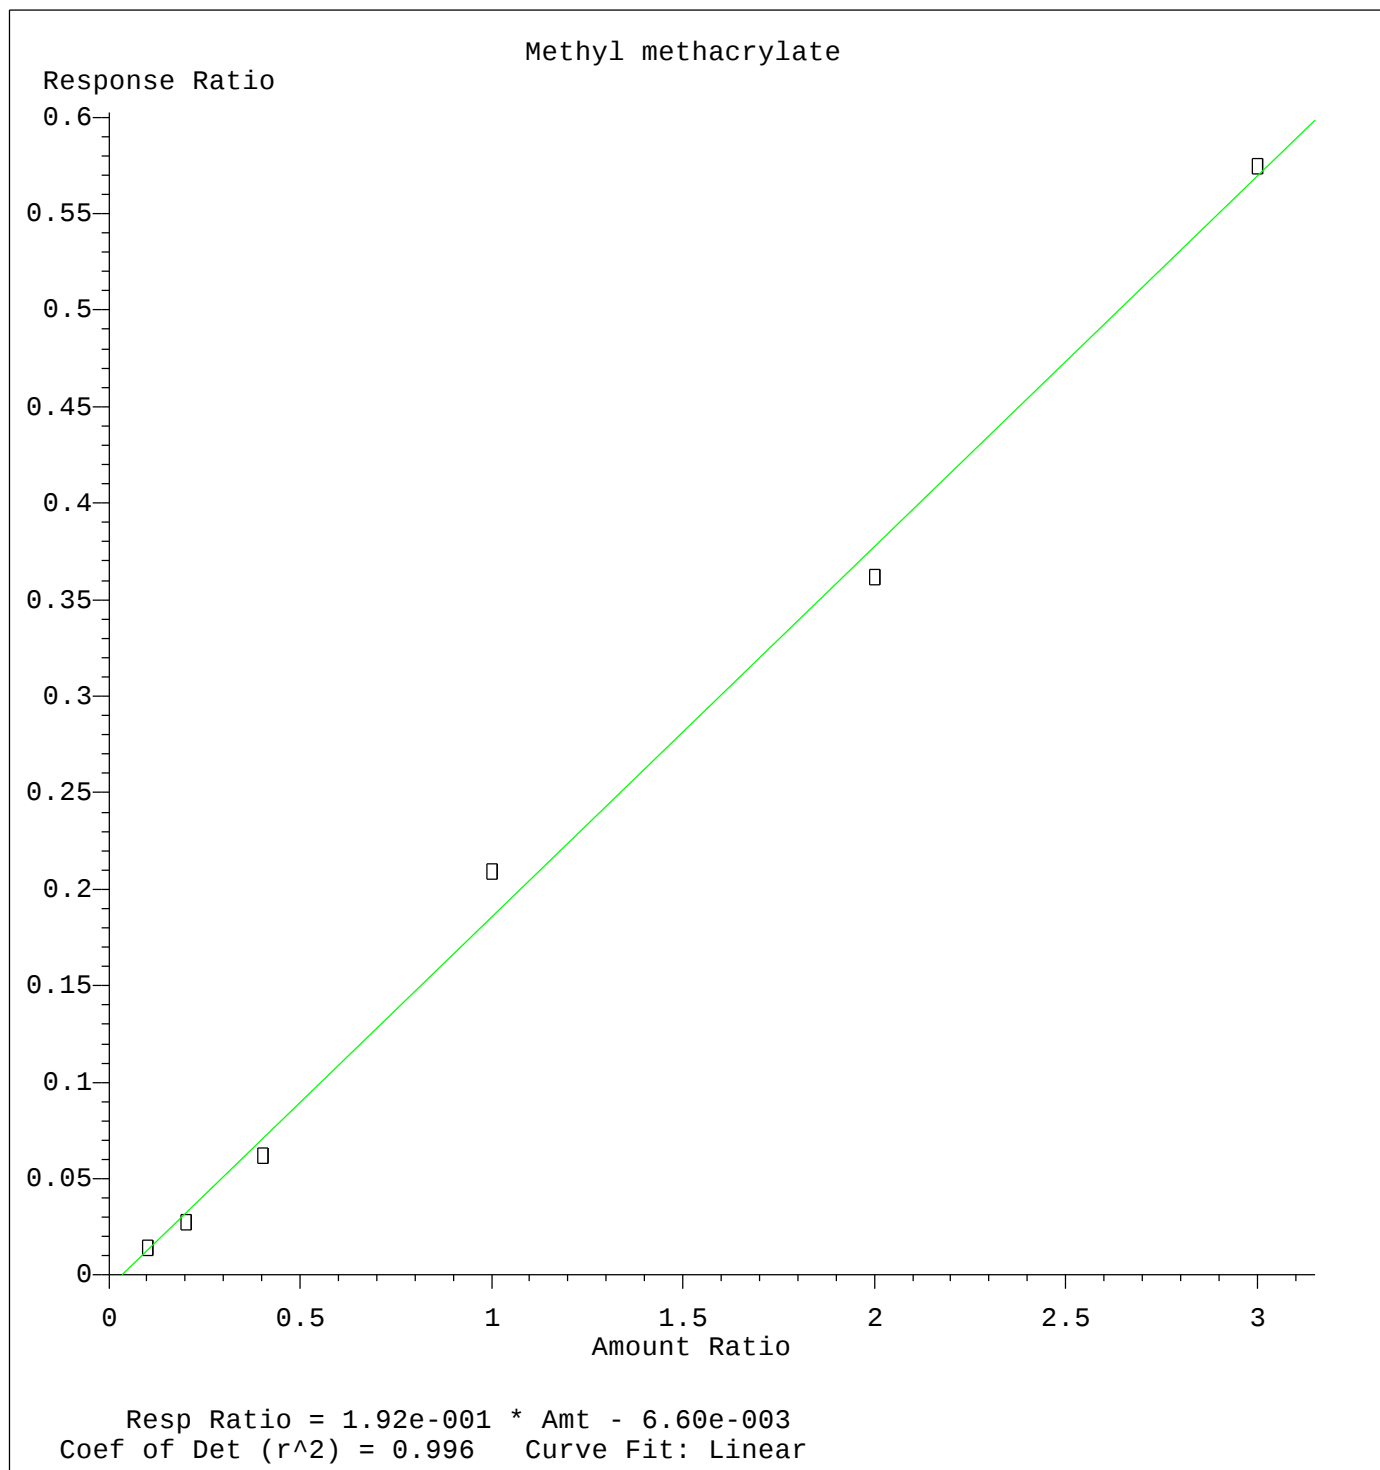


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D041520S.M
Calibration Table Last Updated: Wed Apr 15 19:43:39 2020

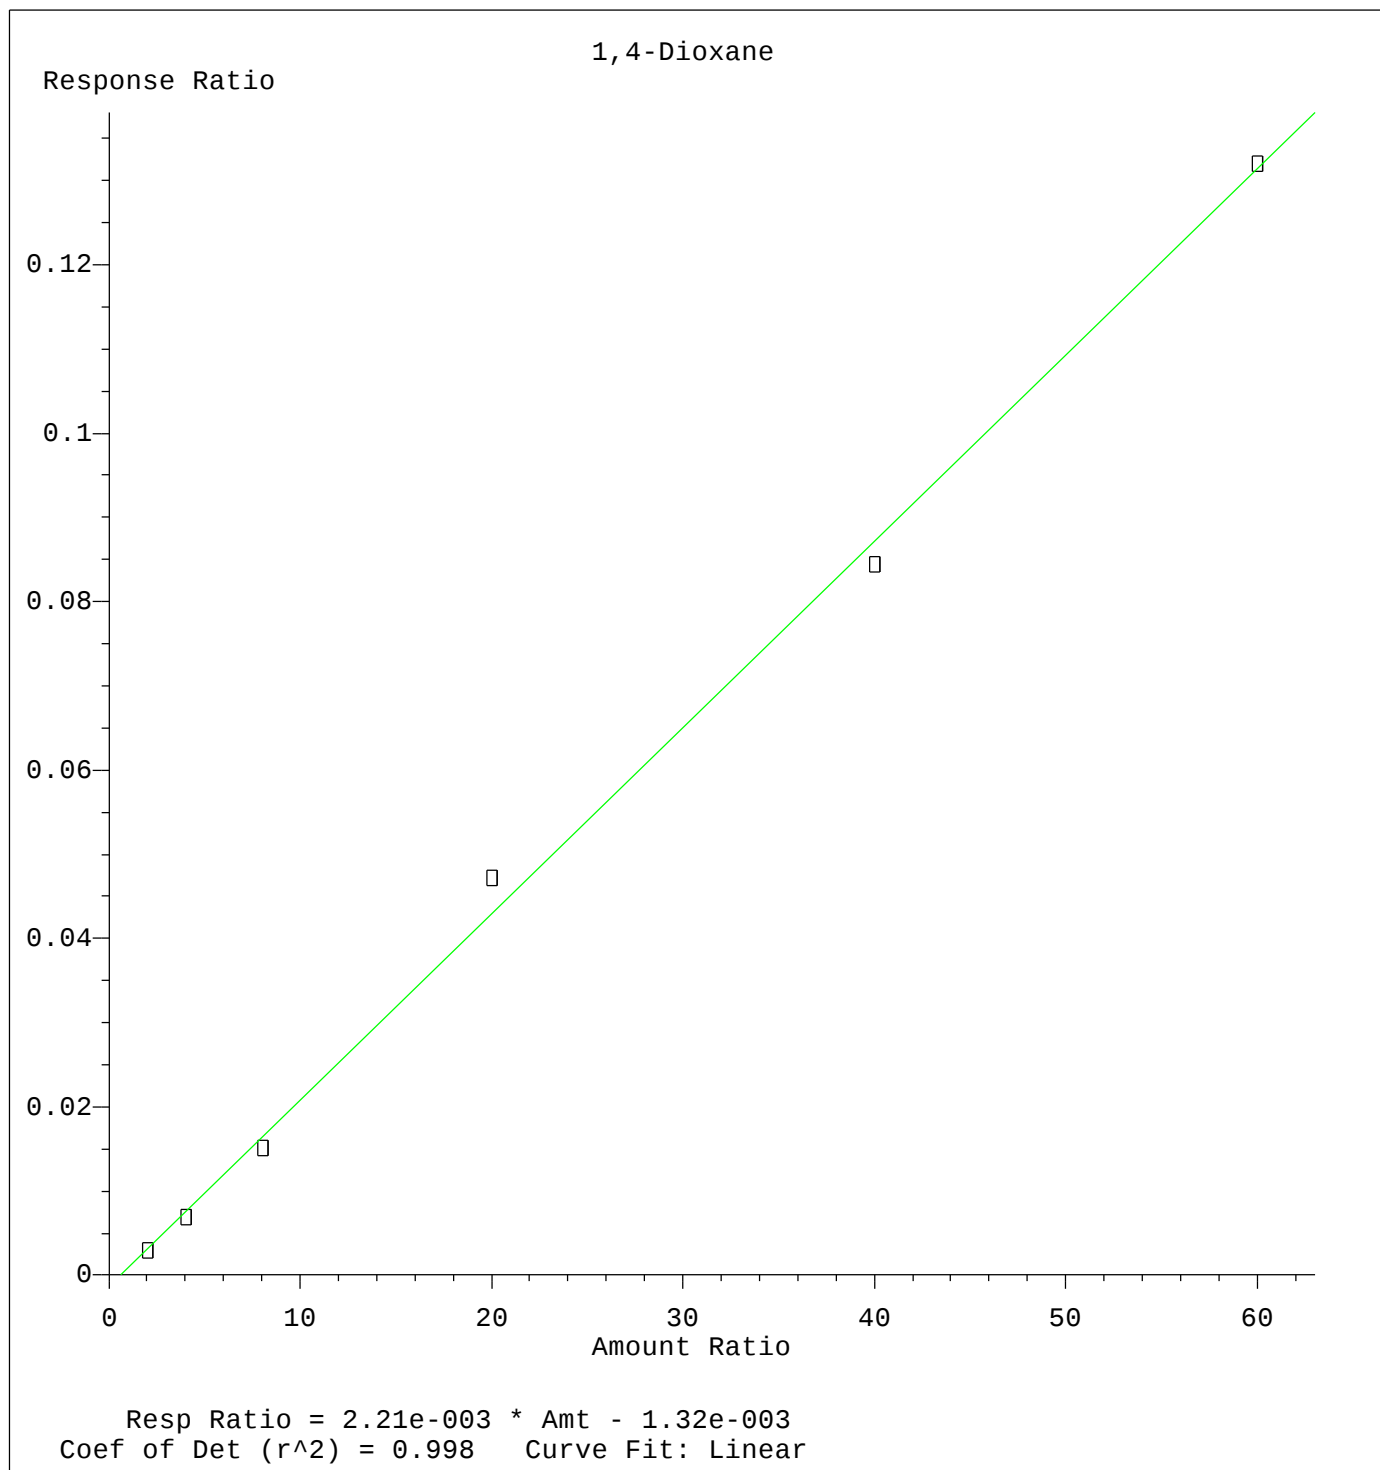

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D041520S.M
Calibration Table Last Updated: Wed Apr 15 19:43:39 2020

4-Methyl-2-Pentanone

Response Ratio

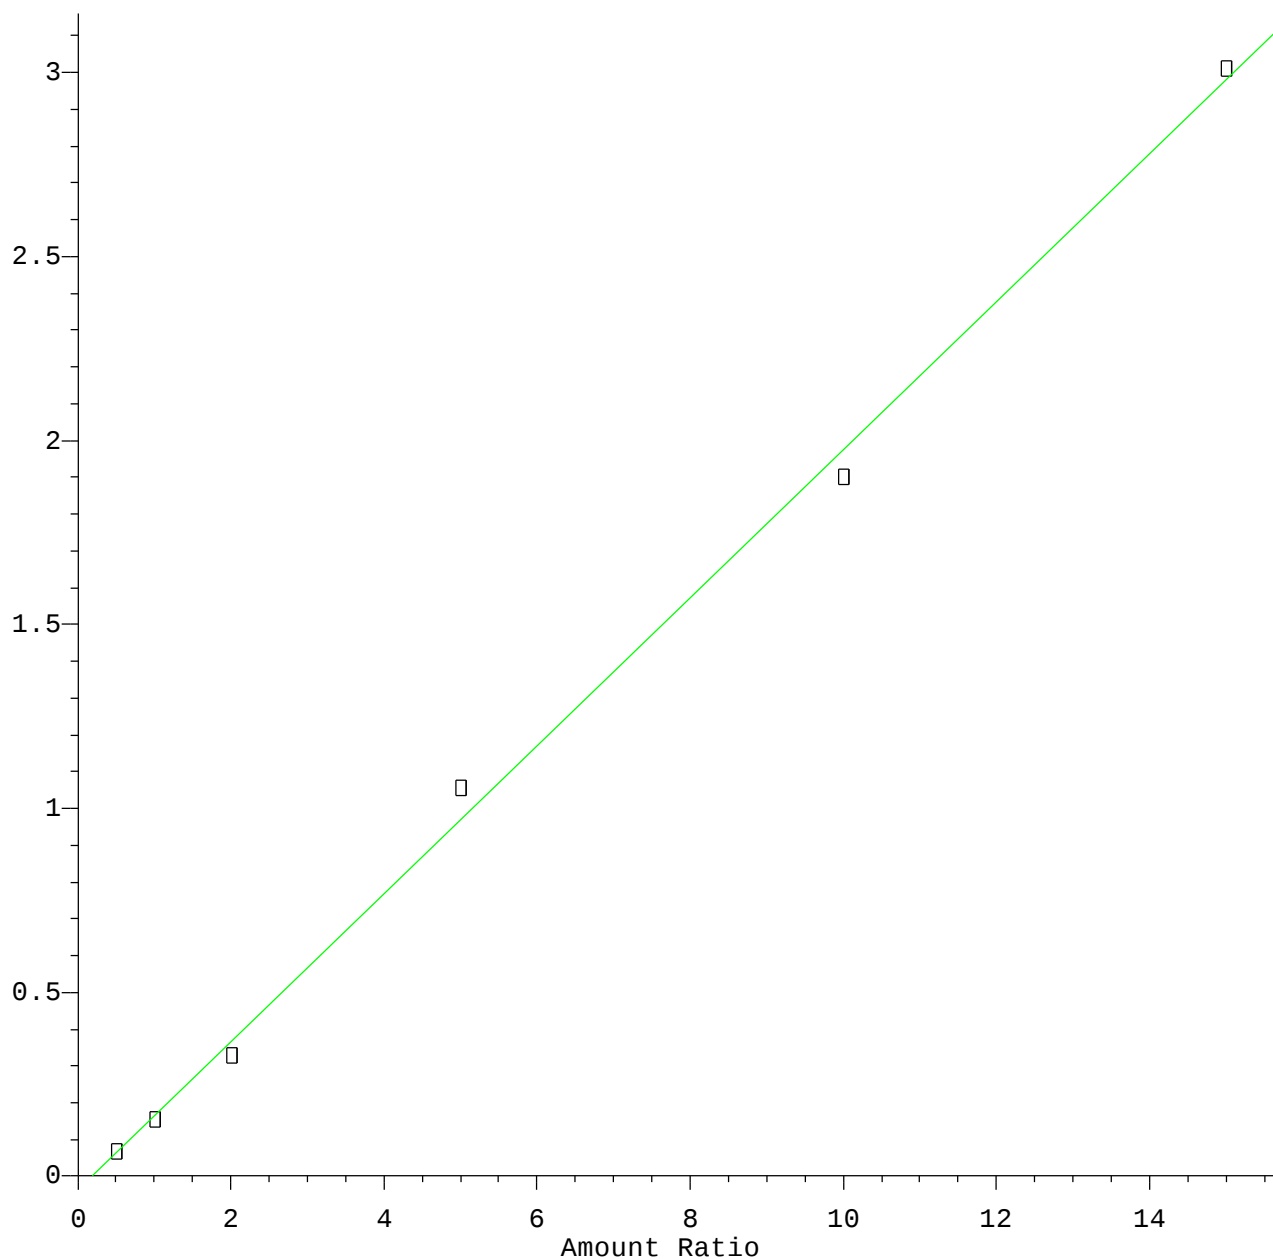

Resp Ratio = $2.01 \times 10^{-1} \times \text{Amt} - 3.90 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D041520S.M
Calibration Table Last Updated: Wed Apr 15 19:43:39 2020