

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD041521\
 Data File : VD068848.D
 Acq On : 15 Apr 2021 11:19
 Operator : VA/SY
 Sample : VD0415SBL01
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VD0415SBL01

Quant Time: Apr 16 01:05:06 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D040721S.M
 Quant Title : SW846 8260
 QLast Update : Thu Apr 08 03:50:31 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.979	168	195177	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	372415	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.644	117	396112	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.573	152	205854	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	93167	45.17	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	90.34%
35) Dibromofluoromethane	7.914	113	111439	46.00	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	92.00%
50) Toluene-d8	10.338	98	471903	51.64	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	103.28%
62) 4-Bromofluorobenzene	12.632	95	178693	58.88	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	117.76%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD041521\
Data File : VD068848.D
Acq On : 15 Apr 2021 11:19
Operator : VA/SY
Sample : VD0415SBL01
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VD0415SBL01

Quant Time: Apr 16 01:05:06 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D040721S.M
Quant Title : SW846 8260
QLast Update : Thu Apr 08 03:50:31 2021
Response via : Initial Calibration




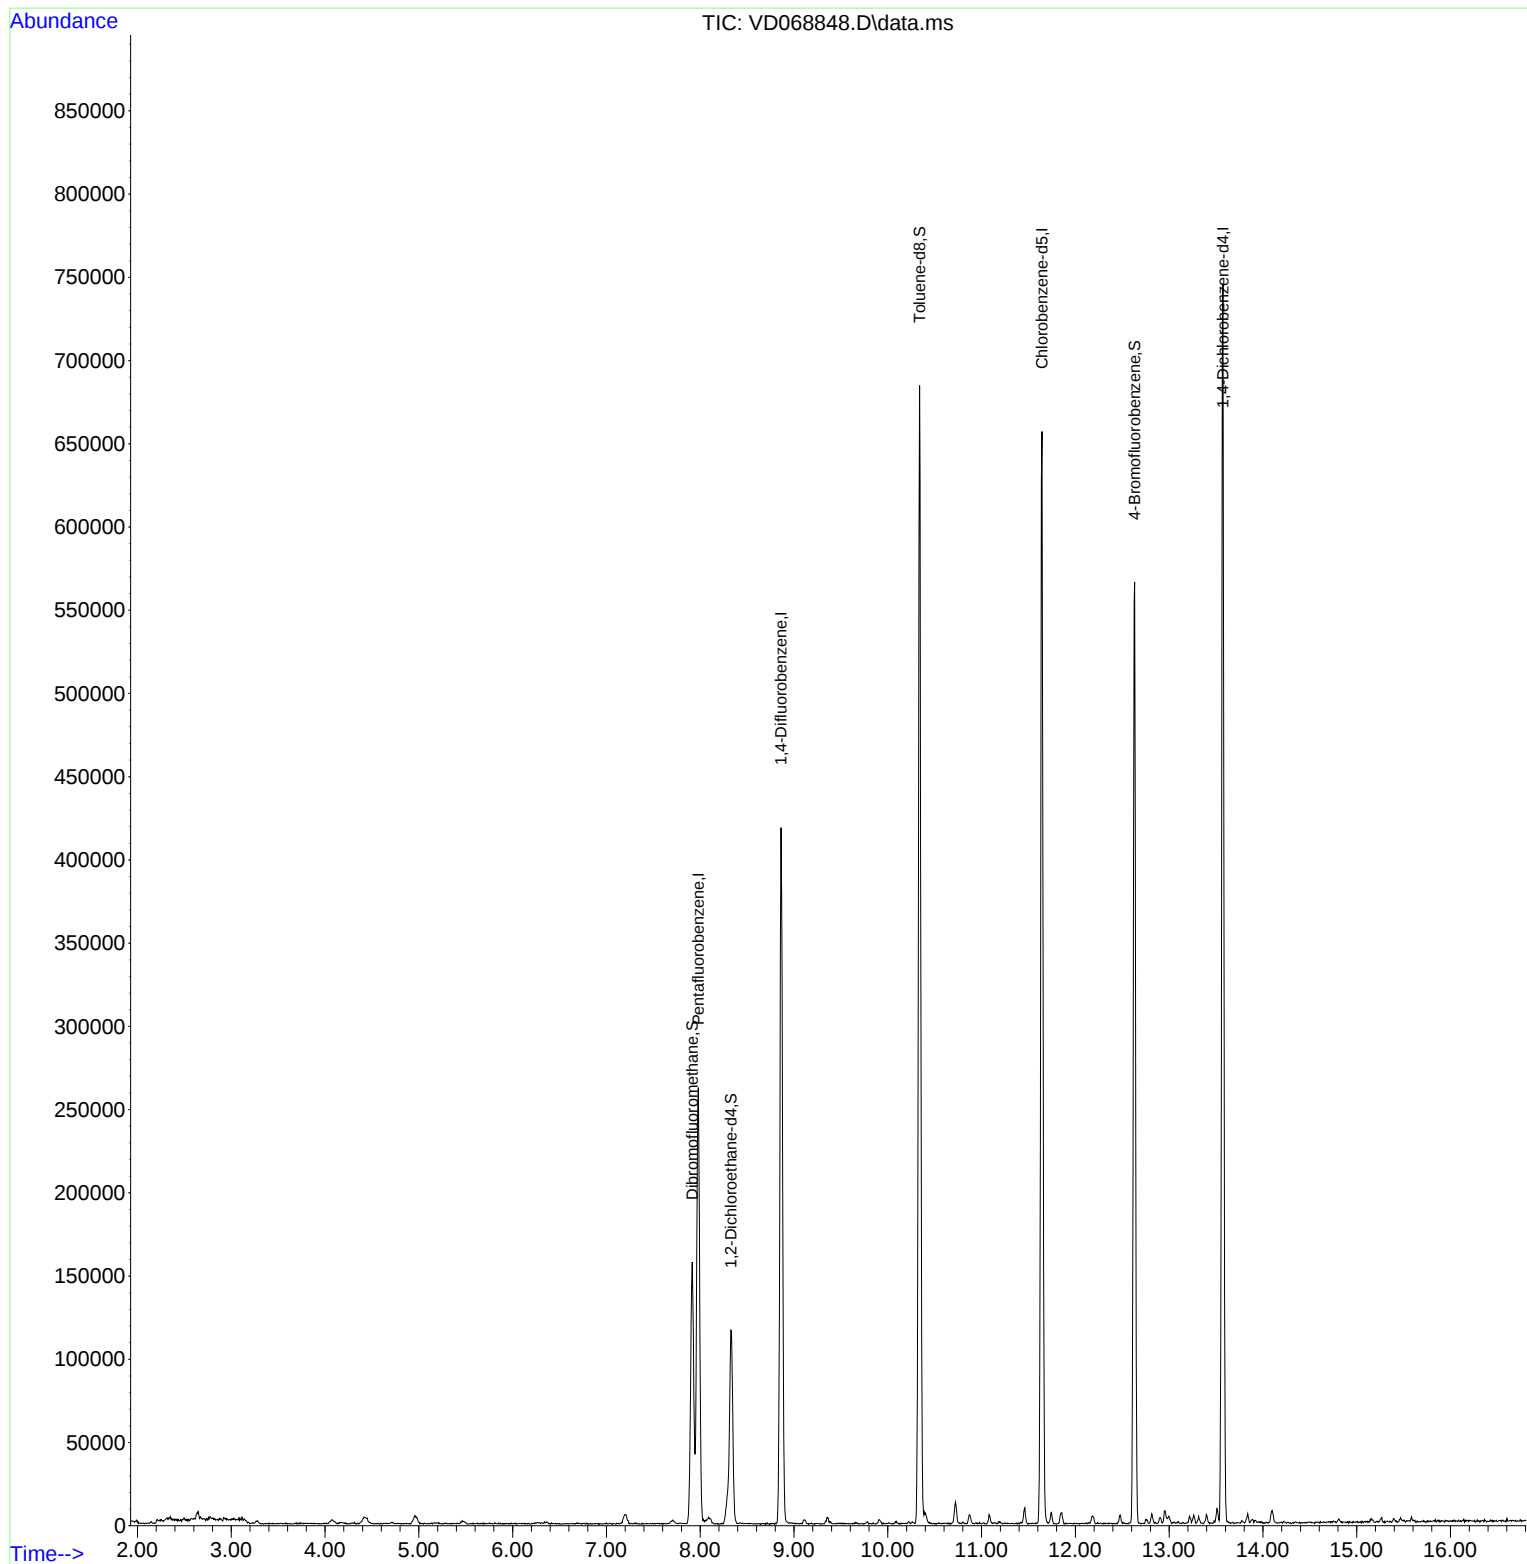


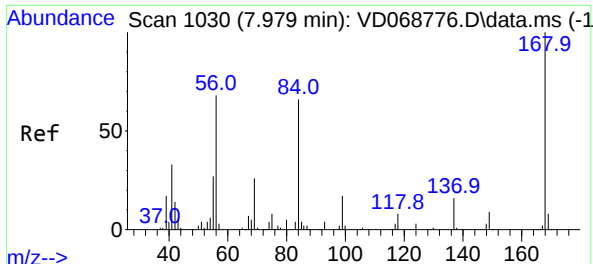

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. 0.000 min
Lab File: VD068848.D
Acq: 15 Apr 2021 11:19




Instrument :
MSVOA_D
ClientSampleId :
VD0415SBL01


Tgt Ion:168 Resp: 195177
Ion Ratio Lower Upper
168 100
99 55.1 46.2 69.2

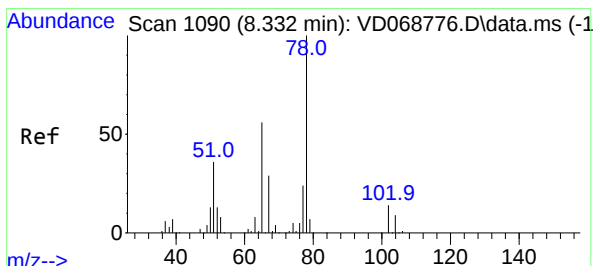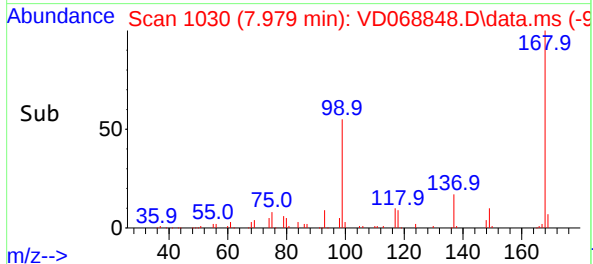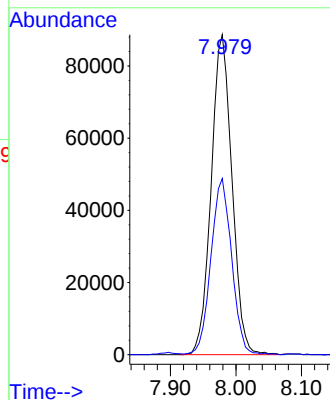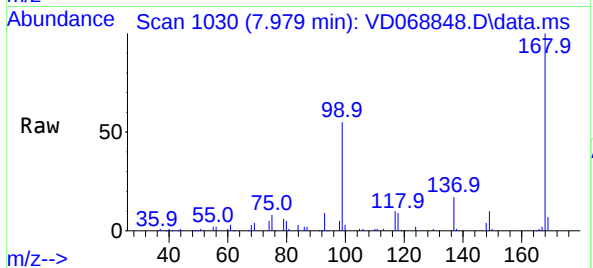

#33
1,2-Dichloroethane-d4
Concen: 45.17 ug/l
RT: 8.326 min Scan# 1089
Delta R.T. -0.006 min
Lab File: VD068848.D
Acq: 15 Apr 2021 11:19

Tgt Ion: 65 Resp: 93167
Ion Ratio Lower Upper
65 100
67 53.6 0.0 106.0

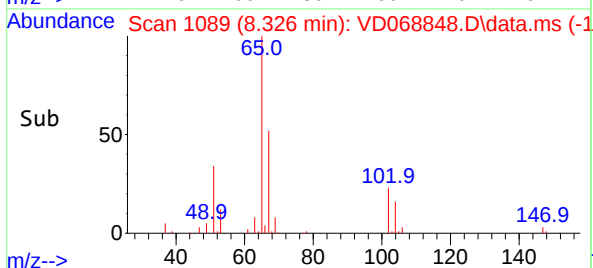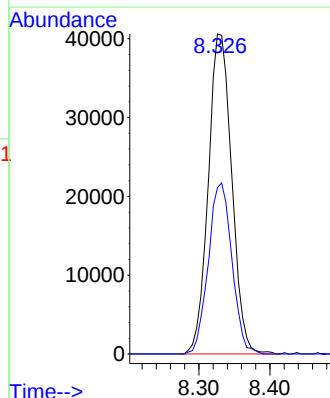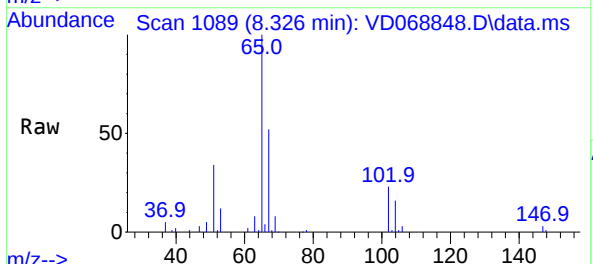




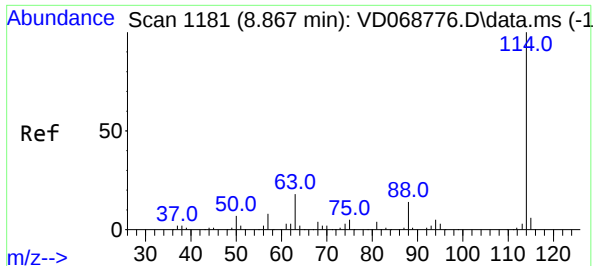


#34

1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.861 min Scan# 1180
Delta R.T. -0.006 min
Lab File: VD068848.D
Acq: 15 Apr 2021 11:19

Instrument :
MSVOA_D
ClientSampleId :
VD0415SBL01




Tgt Ion:114 Resp: 372415
Ion Ratio Lower Upper
114 100
63 17.5 0.0 38.2
88 15.0 0.0 29.4

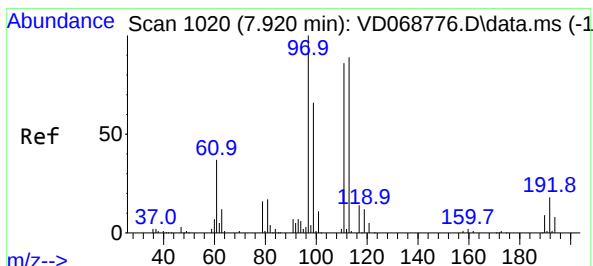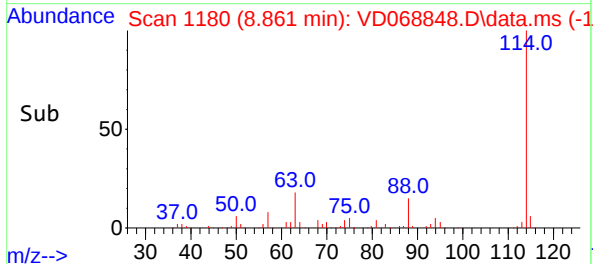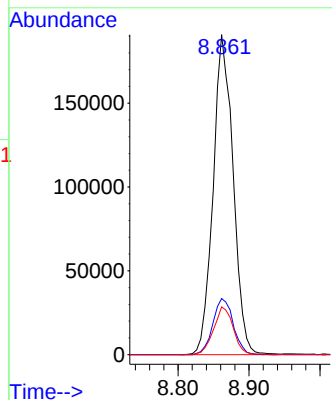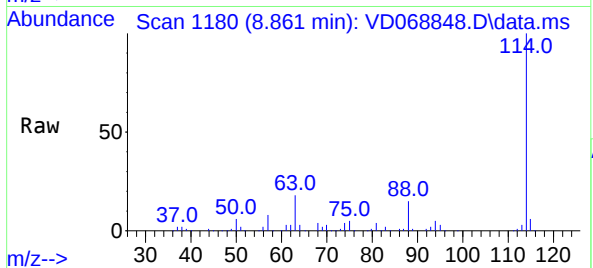


#35

Dibromofluoromethane
Concen: 46.00 ug/l
RT: 7.914 min Scan# 1019
Delta R.T. -0.006 min
Lab File: VD068848.D
Acq: 15 Apr 2021 11:19

Tgt Ion:113 Resp: 111439
Ion Ratio Lower Upper
113 100
111 101.0 82.5 123.7
192 18.4 15.1 22.7


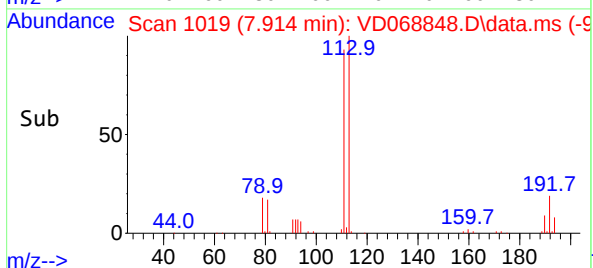
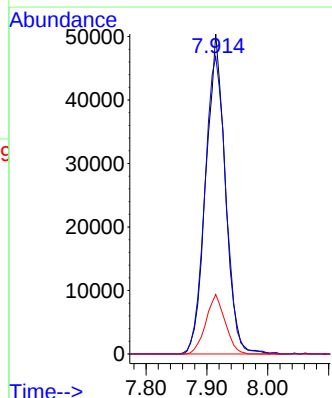
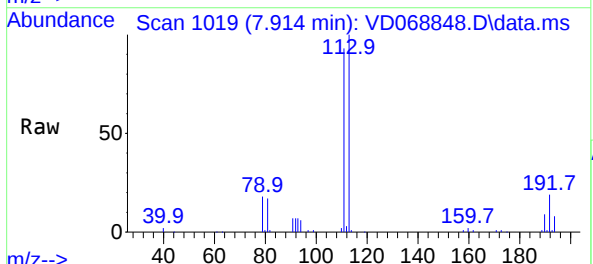


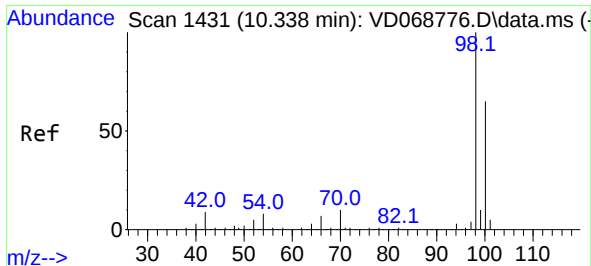

#50
Toluene-d8
Concen: 51.64 ug/l
RT: 10.338 min Scan# 1431
Delta R.T. -0.000 min
Lab File: VD068848.D
Acq: 15 Apr 2021 11:19




Instrument :
MSVOA_D
ClientSampleId :
VD0415SBL01


Tgt Ion: 98 Resp: 471903
Ion Ratio Lower Upper
98 100
100 64.9 51.8 77.6

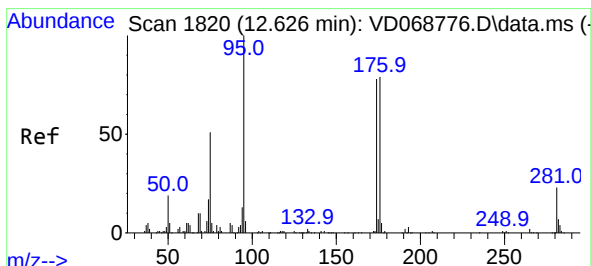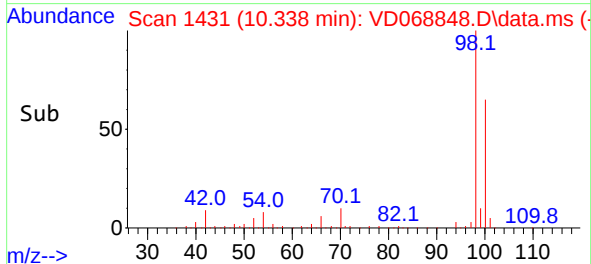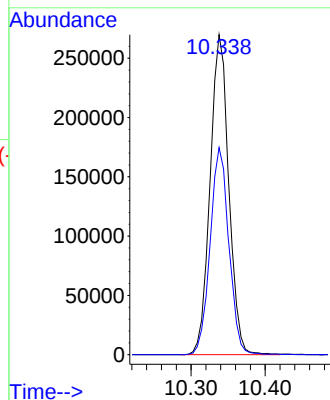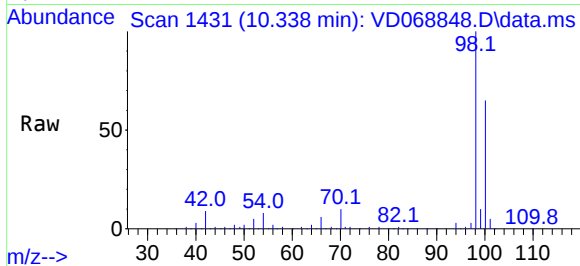

#62
4-Bromofluorobenzene
Concen: 58.88 ug/l
RT: 12.632 min Scan# 1821
Delta R.T. 0.006 min
Lab File: VD068848.D
Acq: 15 Apr 2021 11:19

Tgt Ion: 95 Resp: 178693
Ion Ratio Lower Upper
95 100
174 86.8 0.0 168.0
176 83.8 0.0 160.2


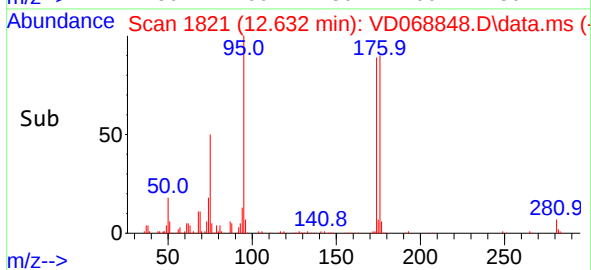
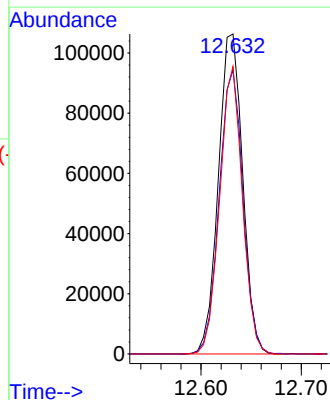
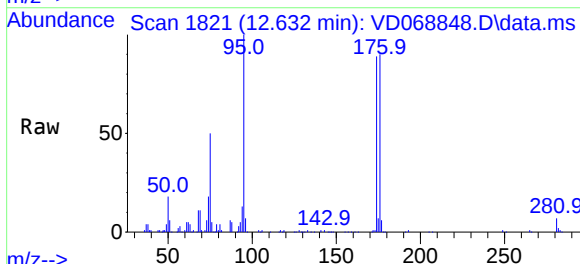


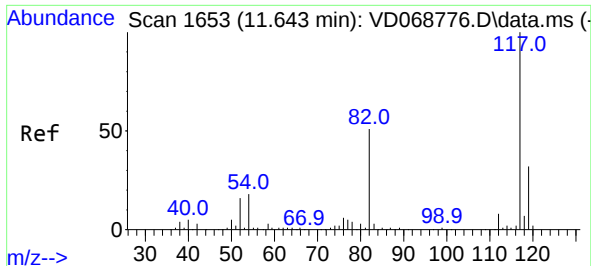

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.644 min Scan# 1653
Delta R.T. 0.001 min
Lab File: VD068848.D
Acq: 15 Apr 2021 11:19

Instrument :
MSVOA_D
ClientSampleId :
VD0415SBL01

Tgt Ion:	117	Resp:	396112
Ion	Ratio	Lower	Upper
117	100		
82	49.3	43.5	65.3
119	31.3	26.7	40.1

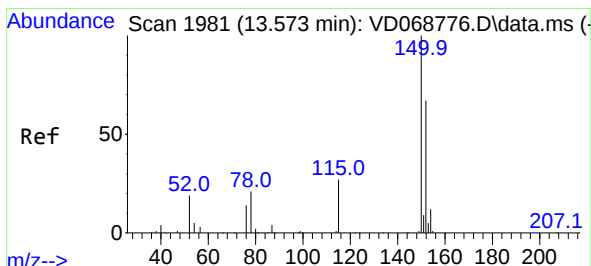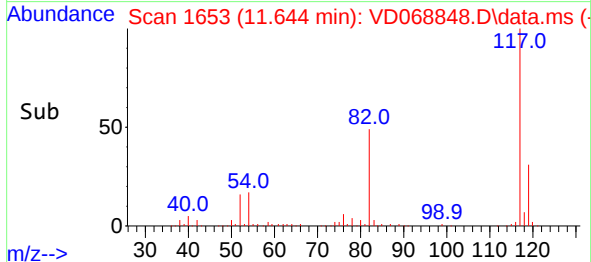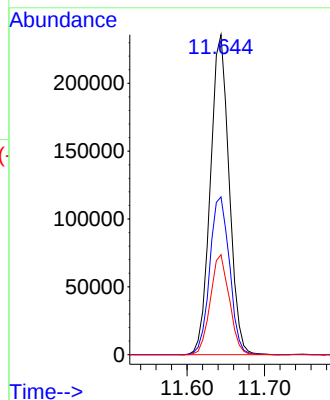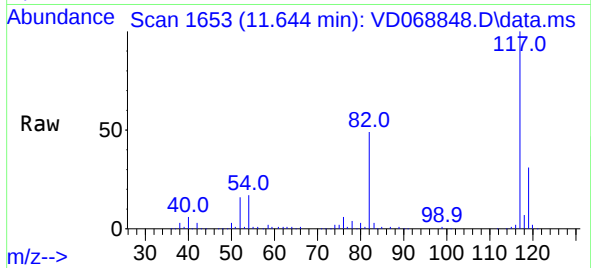

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.573 min Scan# 1981
Delta R.T. -0.000 min
Lab File: VD068848.D
Acq: 15 Apr 2021 11:19

Tgt Ion:	152	Resp:	205854
Ion	Ratio	Lower	Upper
152	100		
115	58.5	29.3	87.8
150	156.7	0.0	347.6

