
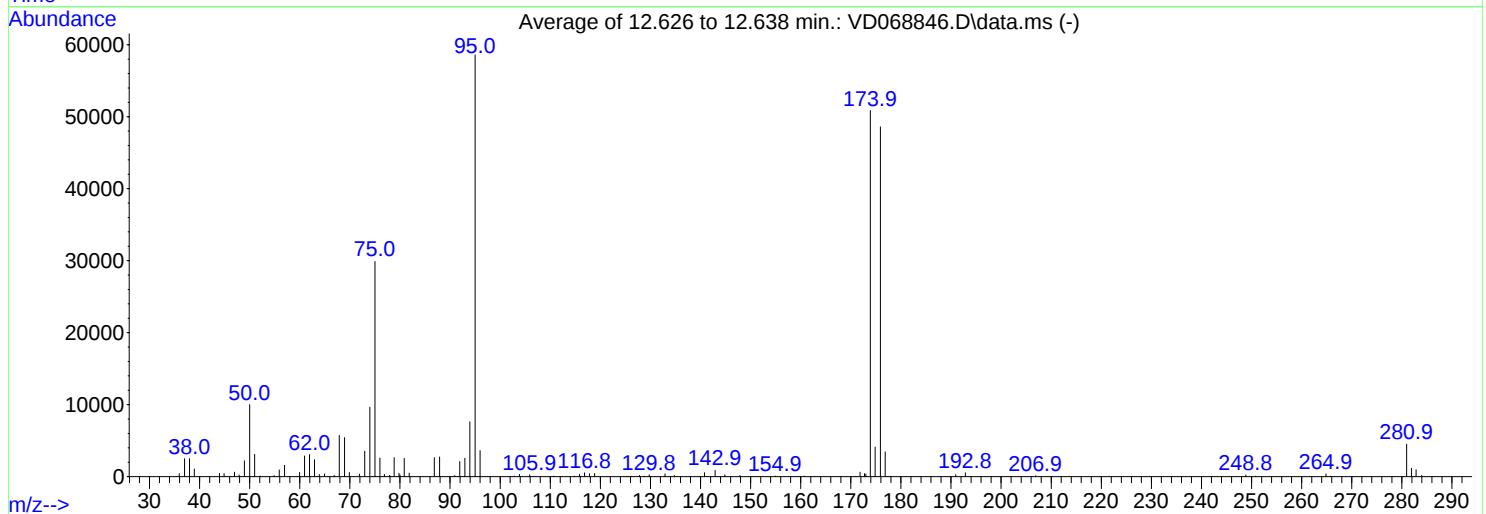


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD041521\
Data File : VD068846.D
Acq On : 15 Apr 2021 09:25
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D040721S.M
Title : SW846 8260
Last Update : Thu Apr 08 03:50:31 2021

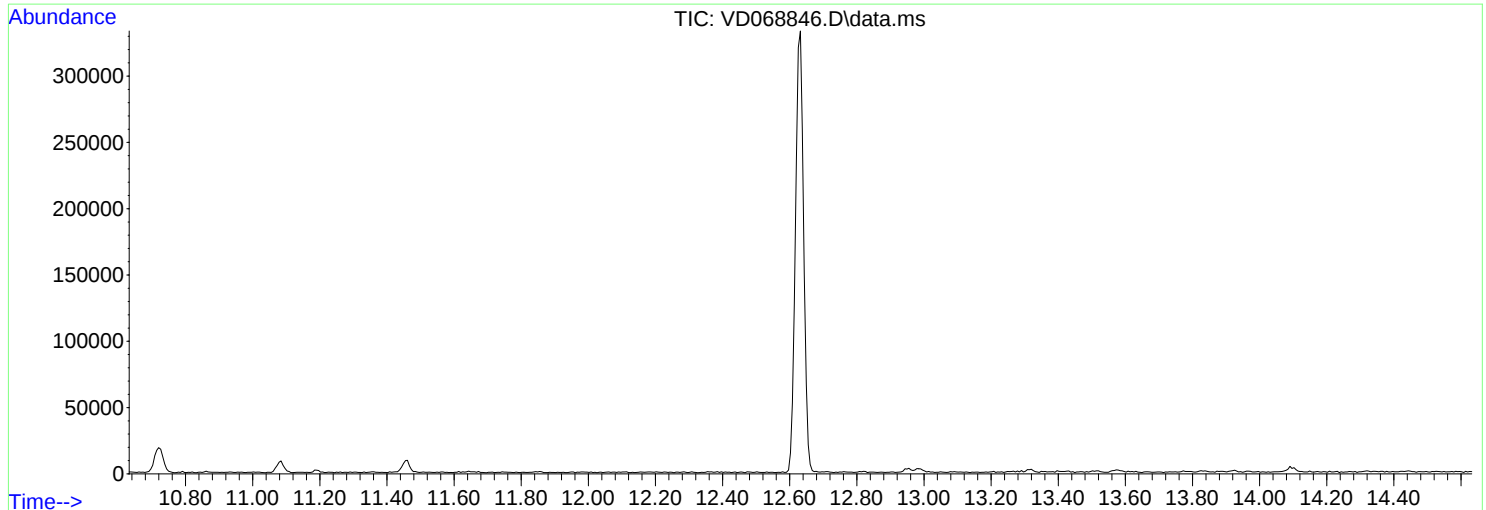

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1812

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.1	10005	PASS
75	95	30	60	51.0	29907	PASS
95	95	100	100	100.0	58595	PASS
96	95	5	9	6.2	3614	PASS
173	174	0.00	2	0.8	425	PASS
174	95	50	100	86.8	50848	PASS
175	174	5	9	8.1	4111	PASS
176	174	95	101	95.5	48584	PASS
177	176	5	9	7.1	3440	PASS