


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD041619\  
Data File : VD061823.D  
Acq On : 16 Apr 2019 22:09  
Operator : VA/AP  
Sample : BFB  
Misc : 5.00µl/5ml/MSVOA D/SOIL  
ALS Vial : 25 Sample Multiplier: 1

Instrument :  
MSVOA\_D  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_D\METHOD\82D041519S.M  
Title : SW846 8260  
Last Update : Tue Apr 16 08:53:01 2019

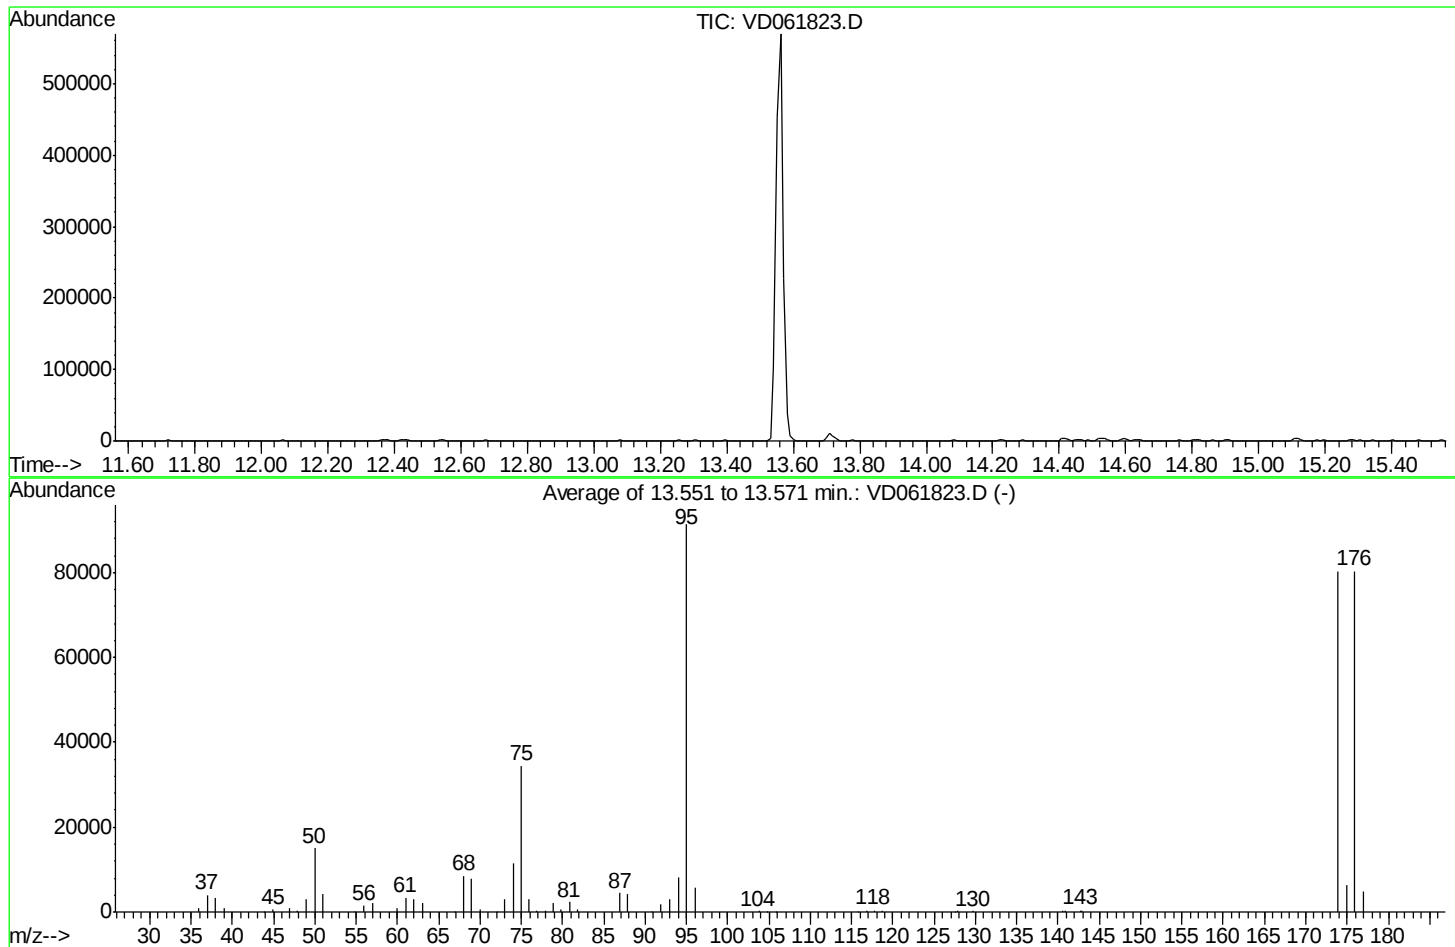

AutoFind: Scans 1232, 1233, 1234; Background Corrected with Scan 1227

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 16.5      | 15078   | PASS             |
| 75          | 95           | 30           | 60           | 37.6      | 34400   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 91378   | PASS             |
| 96          | 95           | 5            | 9            | 6.3       | 5789    | PASS             |
| 173         | 174          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 174         | 95           | 50           | 100          | 87.7      | 80152   | PASS             |
| 175         | 174          | 5            | 9            | 7.8       | 6218    | PASS             |
| 176         | 174          | 95           | 101          | 100.2     | 80282   | PASS             |
| 177         | 176          | 5            | 9            | 6.2       | 4977    | PASS             |