


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD041720\
 Data File : VD065640.D
 Acq On : 17 Apr 2020 12:01
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D041520S.M
 Title : SW846 8260
 Last Update : Wed Apr 15 19:43:39 2020

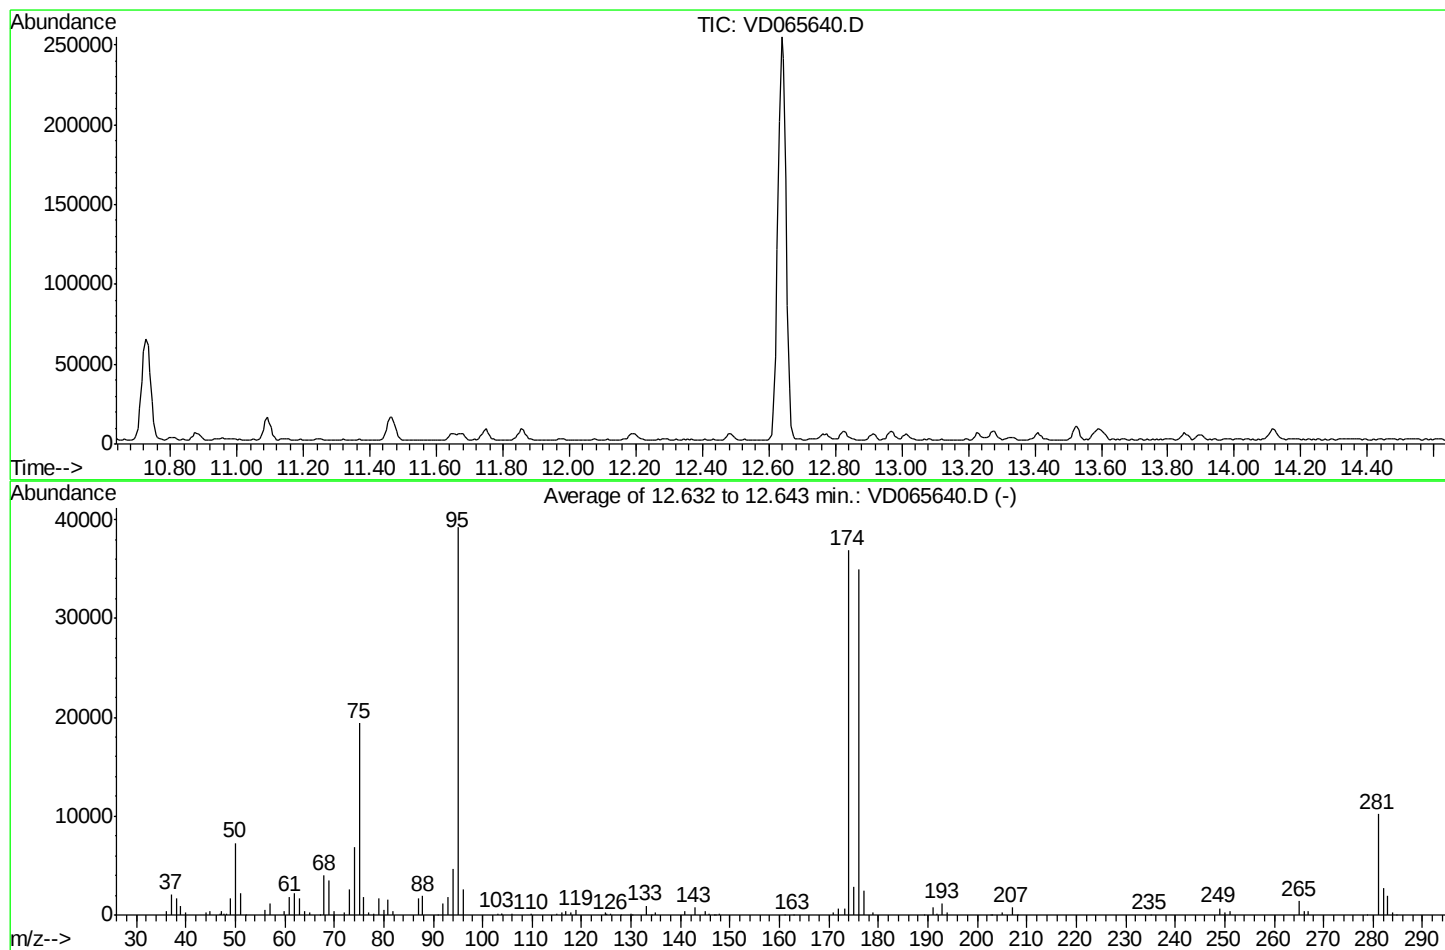

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1814

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	7257	PASS
75	95	30	60	49.4	19384	PASS
95	95	100	100	100.0	39213	PASS
96	95	5	9	6.8	2651	PASS
173	174	0.00	2	1.6	596	PASS
174	95	50	100	94.0	36866	PASS
175	174	5	9	7.7	2849	PASS
176	174	95	101	95.0	35010	PASS
177	176	5	9	7.1	2503	PASS