


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD041819\
Data File : VD061887.D
Acq On : 18 Apr 2019 22:23
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D041519S.M
Title : SW846 8260
Last Update : Thu Apr 18 13:49:04 2019

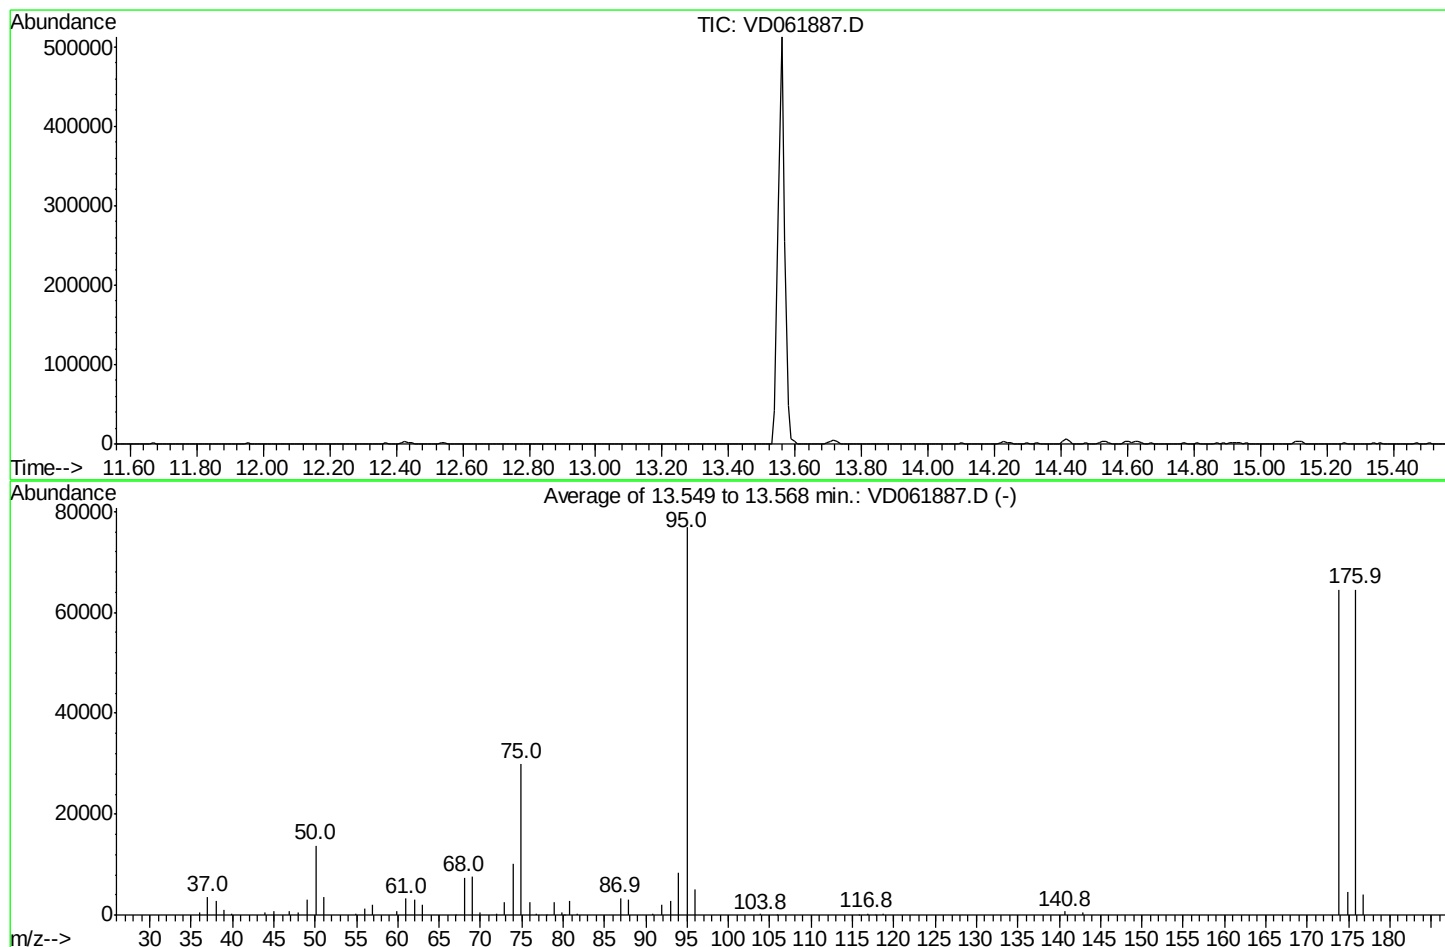

AutoFind: Scans 1232, 1233, 1234; Background Corrected with Scan 1228

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	13740	PASS
75	95	30	60	39.0	30005	PASS
95	95	100	100	100.0	76898	PASS
96	95	5	9	6.6	5073	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	84.0	64568	PASS
175	174	5	9	7.1	4609	PASS
176	174	95	101	100.1	64613	PASS
177	176	5	9	6.2	4029	PASS