


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD041919\
 Data File : VD061903.D
 Acq On : 19 Apr 2019 10:26
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00g/5ml/MSVOA D/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D041519S.M
 Title : SW846 8260
 Last Update : Thu Apr 18 13:49:04 2019

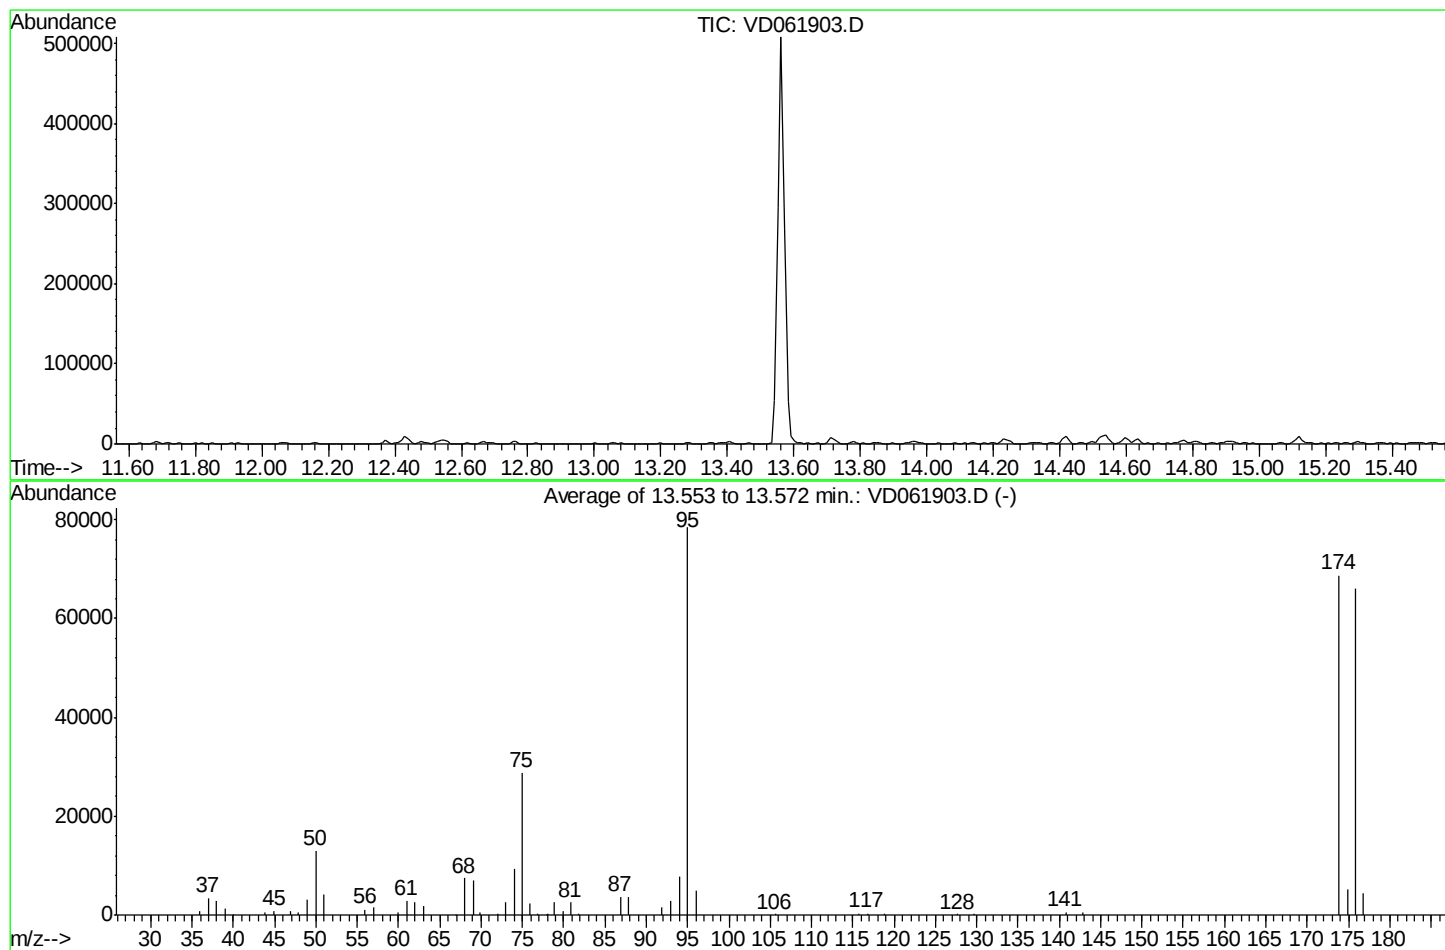

AutoFind: Scans 1232, 1233, 1234; Background Corrected with Scan 1227

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	13089	PASS
75	95	30	60	36.7	28786	PASS
95	95	100	100	100.0	78466	PASS
96	95	5	9	6.3	4905	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	87.6	68749	PASS
175	174	5	9	7.5	5130	PASS
176	174	95	101	96.0	65986	PASS
177	176	5	9	6.7	4452	PASS