


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD041919\
 Data File : VD061925.D
 Acq On : 19 Apr 2019 23:38
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µl/5ml/MSVOA D/SOIL
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D041519S.M
 Title : SW846 8260
 Last Update : Thu Apr 18 13:49:04 2019

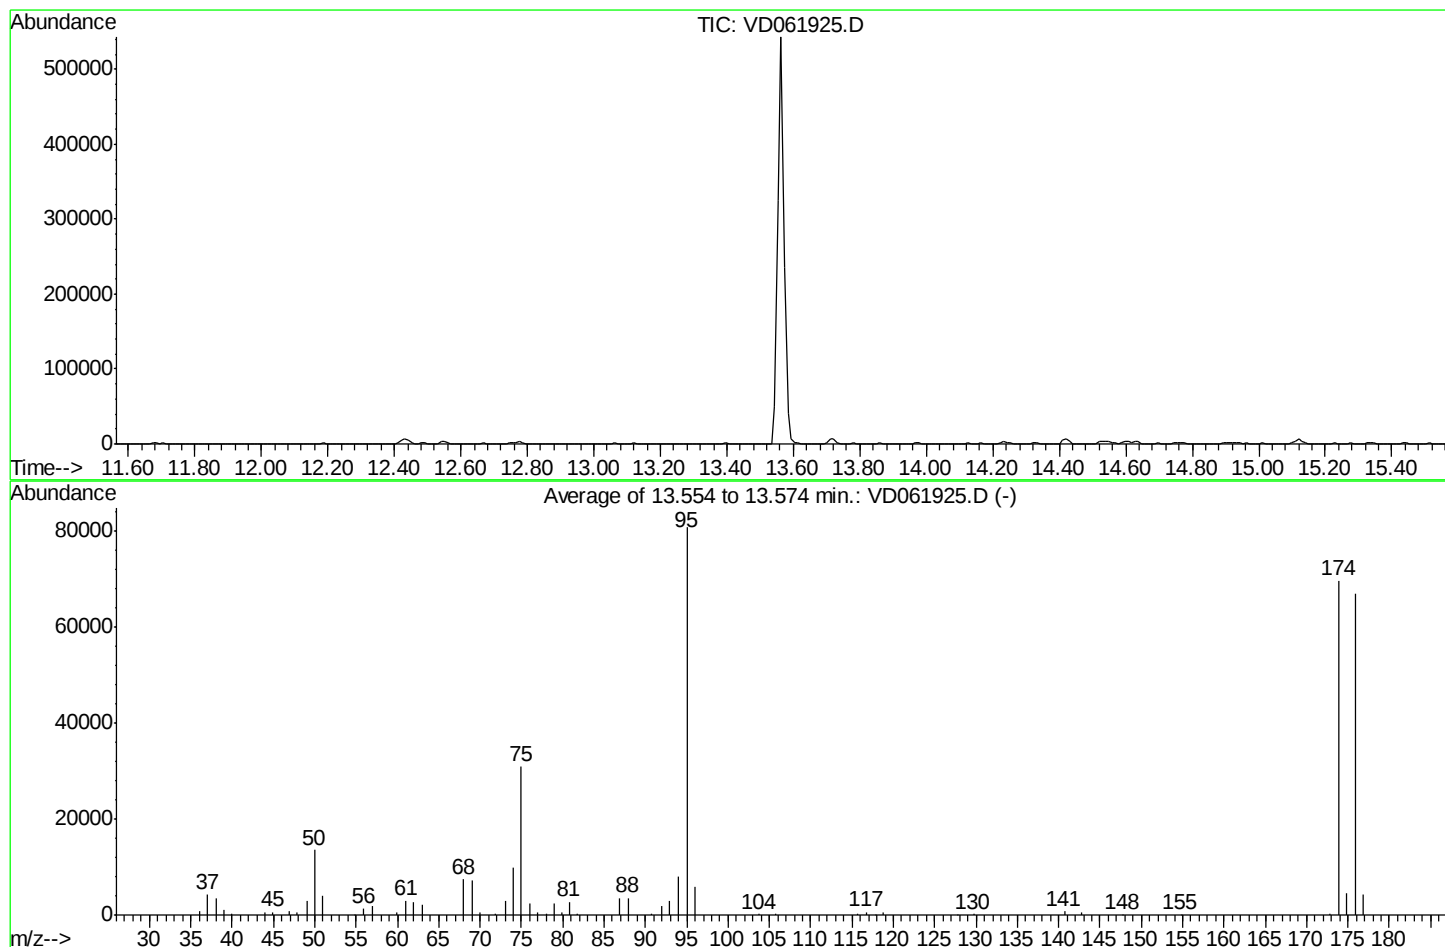

AutoFind: Scans 1232, 1233, 1234; Background Corrected with Scan 1227

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	13562	PASS
75	95	30	60	38.3	30878	PASS
95	95	100	100	100.0	80669	PASS
96	95	5	9	7.2	5773	PASS
173	174	0.00	2	0.2	147	PASS
174	95	50	100	86.3	69653	PASS
175	174	5	9	6.3	4410	PASS
176	174	95	101	96.1	66914	PASS
177	176	5	9	6.3	4201	PASS