
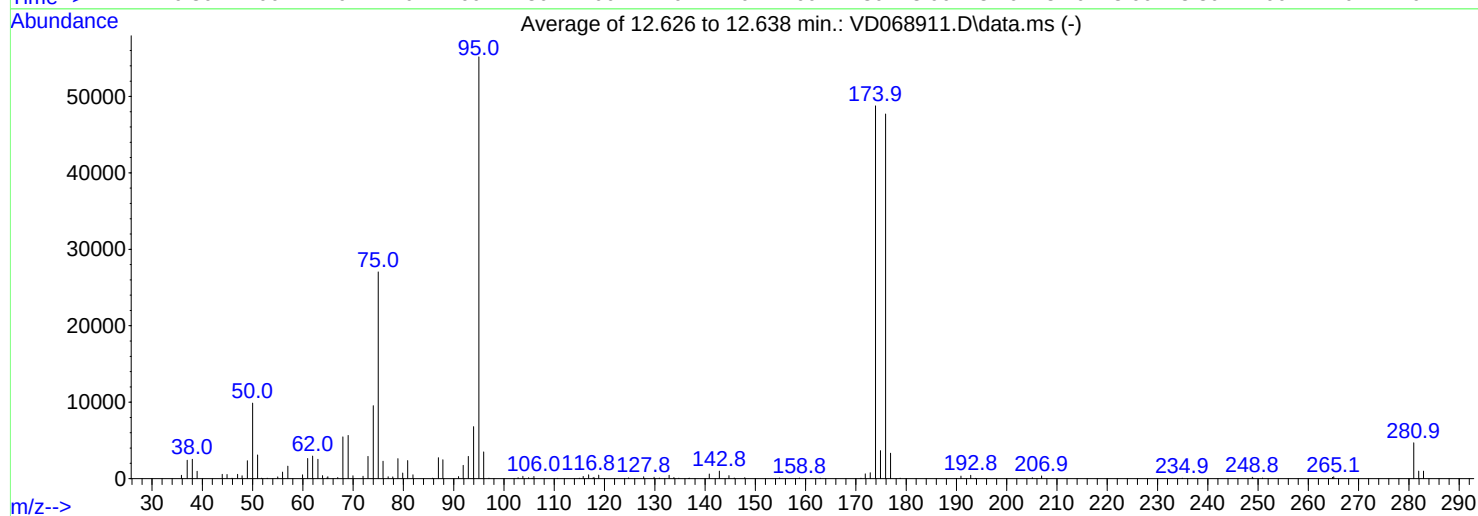


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042021\
Data File : VD068911.D
Acq On : 20 Apr 2021 08:17
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D040721S.M
Title : SW846 8260
Last Update : Thu Apr 08 03:50:31 2021

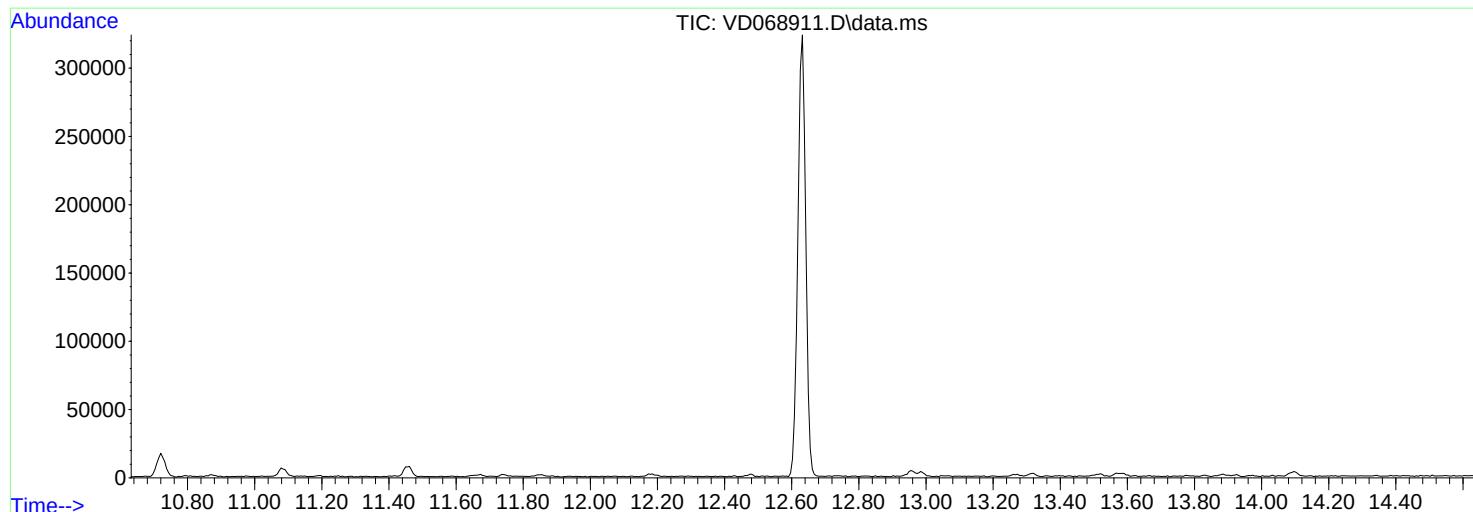

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1812

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.9	9876	PASS
75	95	30	60	49.0	27048	PASS
95	95	100	100	100.0	55176	PASS
96	95	5	9	6.4	3505	PASS
173	174	0.00	2	1.6	775	PASS
174	95	50	100	88.4	48773	PASS
175	174	5	9	7.5	3659	PASS
176	174	95	101	97.8	47696	PASS
177	176	5	9	7.0	3339	PASS