
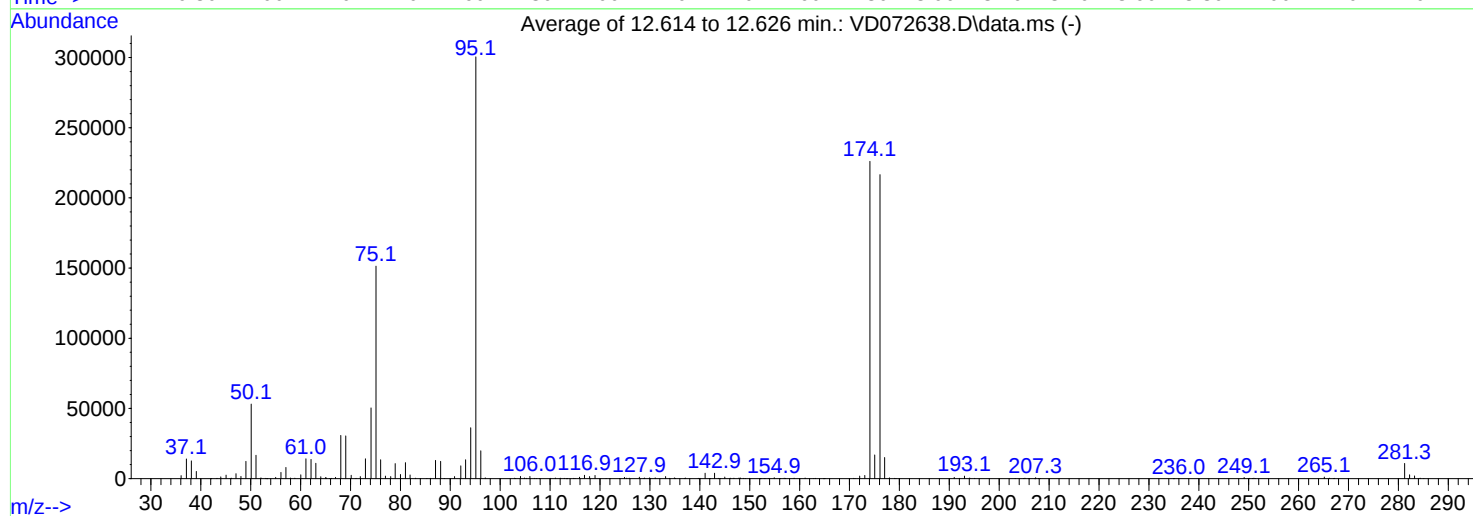


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042022\
 Data File : VD072638.D
 Acq On : 20 Apr 2022 09:07
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D032922S.M
 Title : SW846 8260
 Last Update : Wed Mar 30 02:44:36 2022

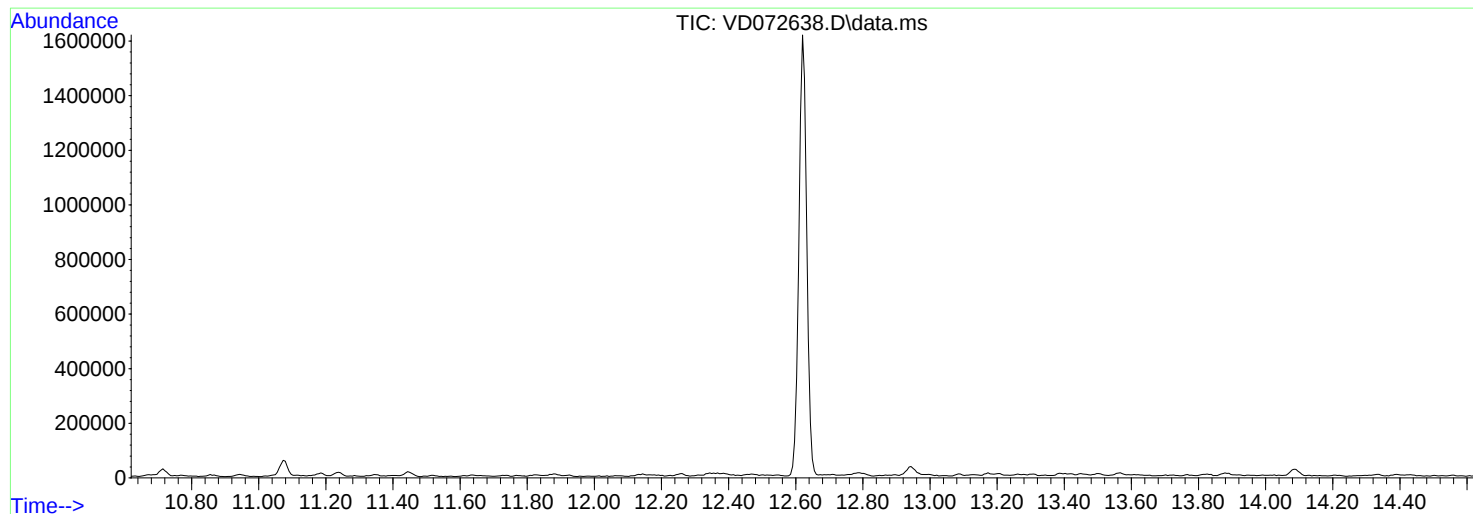

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1809

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	53139	PASS
75	95	30	60	50.4	151424	PASS
95	95	100	100	100.0	300498	PASS
96	95	5	9	6.6	19874	PASS
173	174	0.00	2	1.0	2276	PASS
174	95	50	100	75.2	226091	PASS
175	174	5	9	7.5	16894	PASS
176	174	95	101	95.8	216533	PASS
177	176	5	9	7.0	15057	PASS