

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042122\
 Data File : VD072662.D
 Acq On : 21 Apr 2022 11:07
 Operator : VA/SY
 Sample : VD0421SBL01
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VD0421SBL01

Quant Time: Apr 21 14:53:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D032922S.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 30 02:44:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.973	168	520011	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	927541	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.638	117	864860	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.561	152	388898	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	281367	44.729	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	89.460%
35) Dibromofluoromethane	7.914	113	299775	41.587	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	83.180%
50) Toluene-d8	10.332	98	1117605	44.603	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	89.200%
62) 4-Bromofluorobenzene	12.620	95	382959	39.135	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	78.260%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042122\
Data File : VD072662.D
Acq On : 21 Apr 2022 11:07
Operator : VA/SY
Sample : VD0421SBL01
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VD0421SBL01

Quant Time: Apr 21 14:53:28 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D032922S.M
Quant Title : SW846 8260
QLast Update : Wed Mar 30 02:44:36 2022
Response via : Initial Calibration




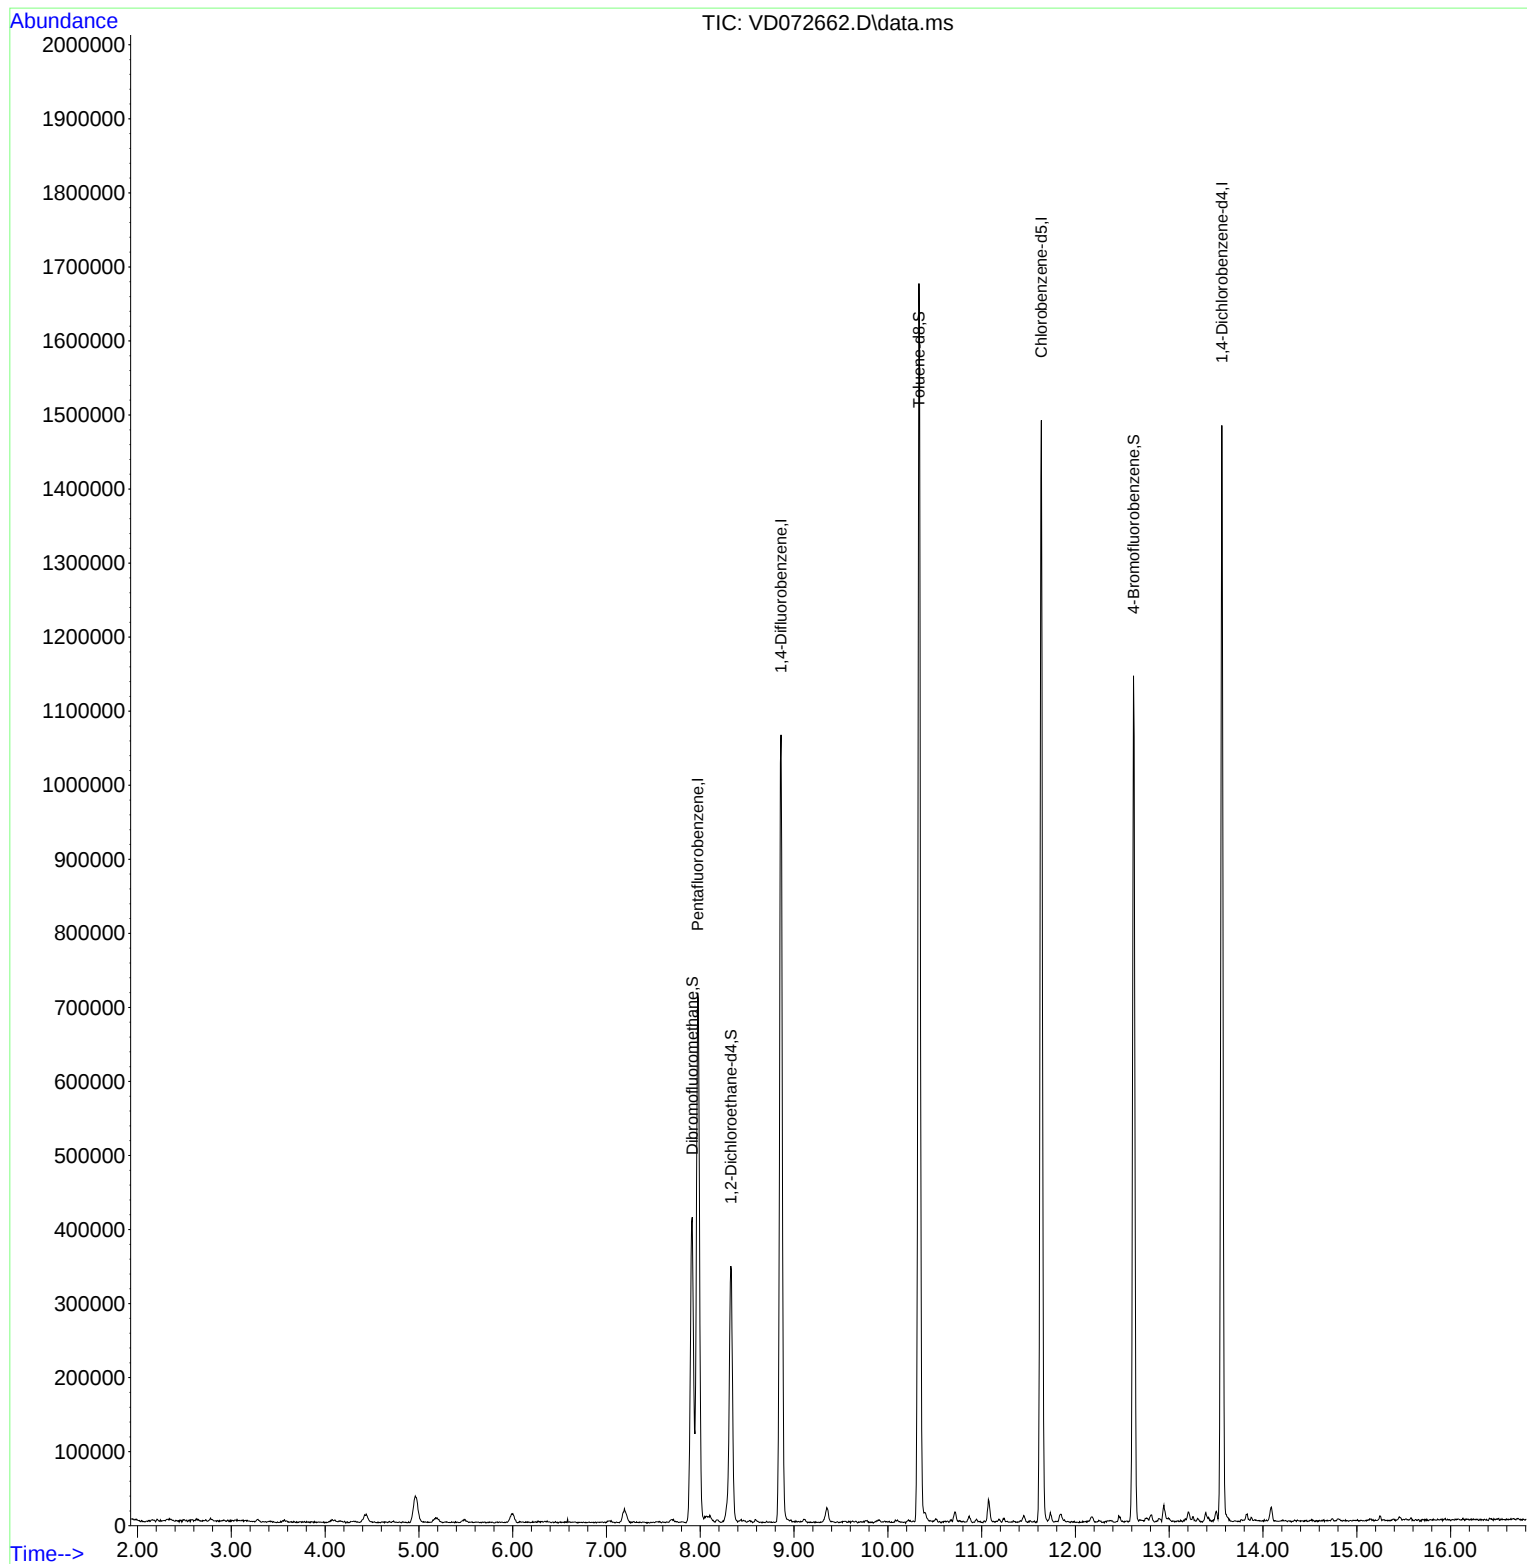


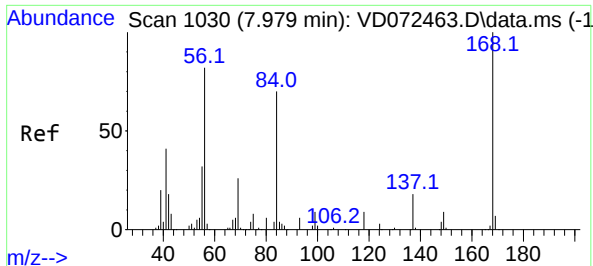

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.973 min Scan# 1030
Delta R.T. -0.006 min
Lab File: VD072662.D
Acq: 21 Apr 2022 11:07




Instrument :
MSVOA_D
ClientSampleId :
VD0421SBL01


Tgt Ion:168 Resp: 520011
Ion Ratio Lower Upper
168 100
99 58.4 49.8 74.6

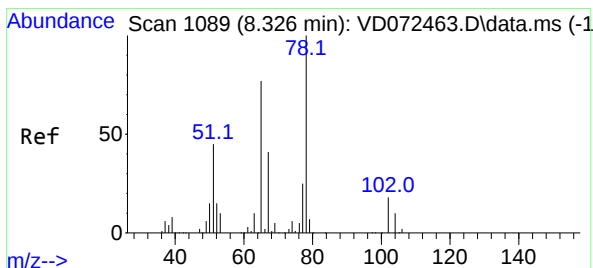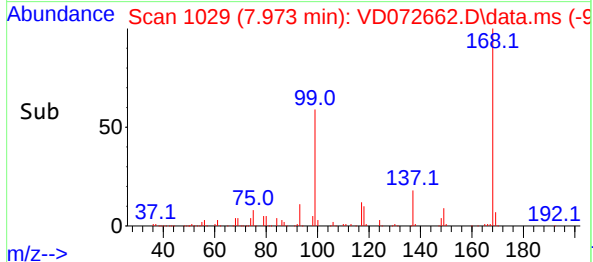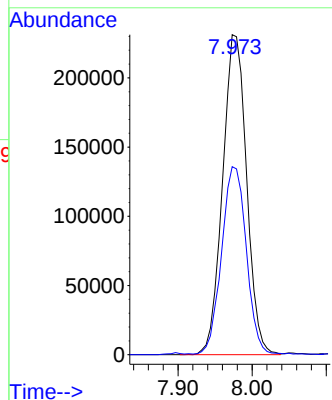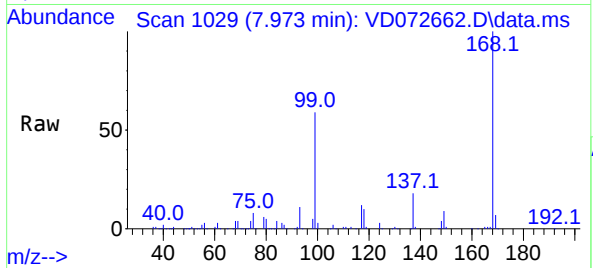

#33
1,2-Dichloroethane-d4
Concen: 44.729 ug/l
RT: 8.326 min Scan# 1089
Delta R.T. -0.000 min
Lab File: VD072662.D
Acq: 21 Apr 2022 11:07

Tgt Ion: 65 Resp: 281367
Ion Ratio Lower Upper
65 100
67 52.4 0.0 101.4


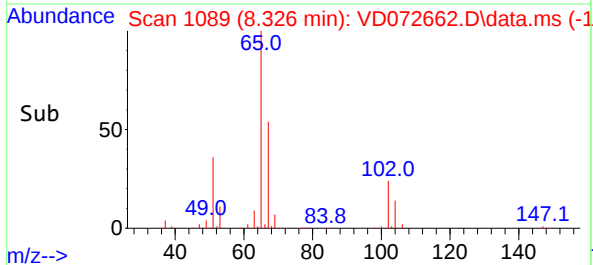
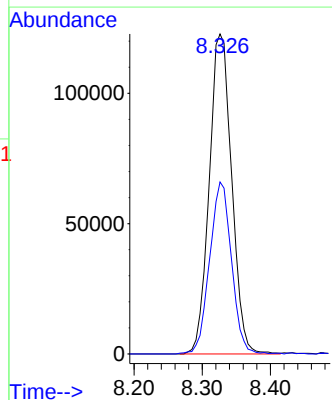
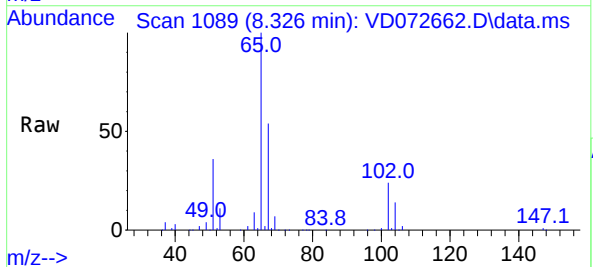


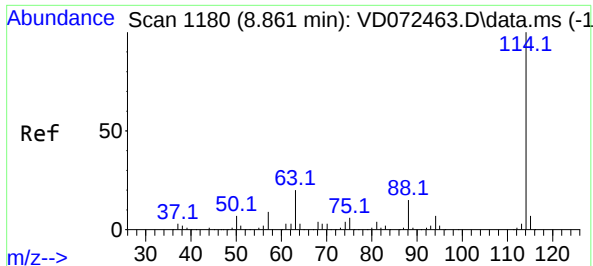

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.861 min Scan# 1180
Delta R.T. -0.000 min
Lab File: VD072662.D
Acq: 21 Apr 2022 11:07




Instrument :
MSVOA_D
ClientSampleId :
VD0421SBL01


Tgt Ion:114 Resp: 927541
Ion Ratio Lower Upper
114 100
63 19.6 0.0 46.6
88 15.3 0.0 33.2

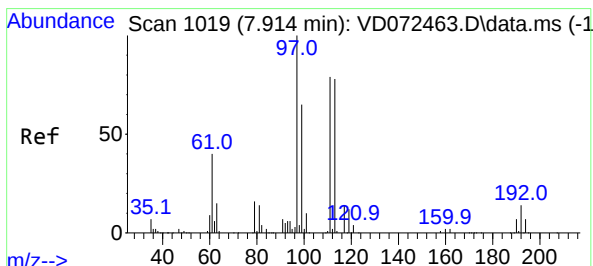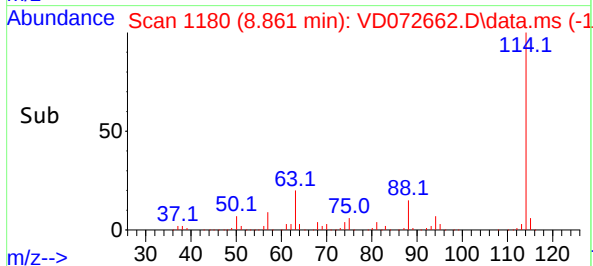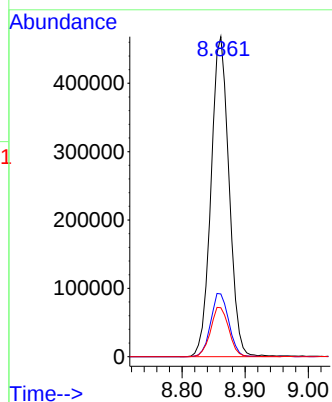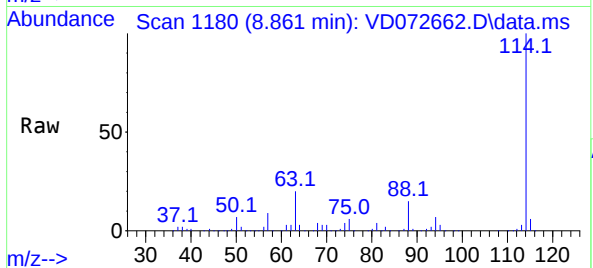

#35
Dibromofluoromethane
Concen: 41.587 ug/l
RT: 7.914 min Scan# 1019
Delta R.T. 0.000 min
Lab File: VD072662.D
Acq: 21 Apr 2022 11:07

Tgt Ion:113 Resp: 299775
Ion Ratio Lower Upper
113 100
111 101.9 83.8 125.6
192 17.4 14.6 21.8


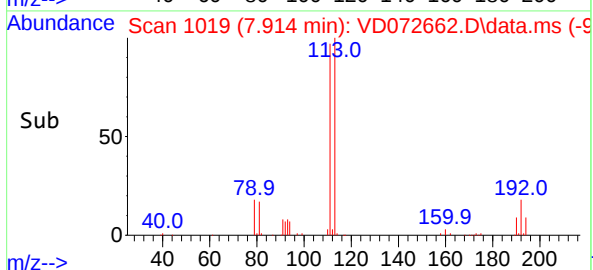
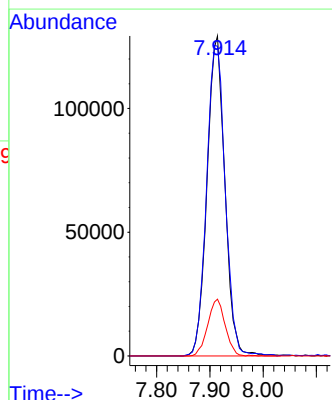
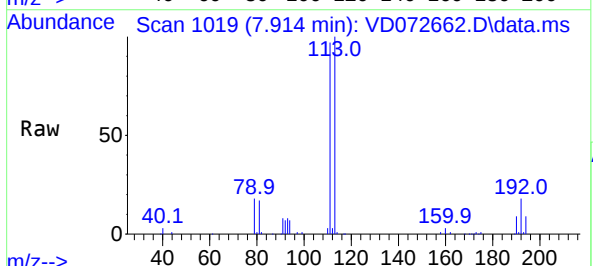


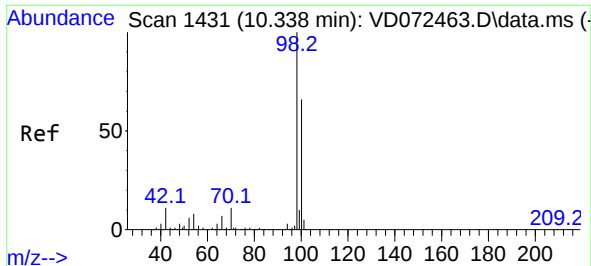

#50
Toluene-d8
Concen: 44.603 ug/l
RT: 10.332 min Scan# 1431
Delta R.T. -0.006 min
Lab File: VD072662.D
Acq: 21 Apr 2022 11:07




Instrument :
MSVOA_D
ClientSampleId :
VD0421SBL01


Tgt Ion: 98 Resp: 1117605
Ion Ratio Lower Upper
98 100
100 67.0 52.4 78.6

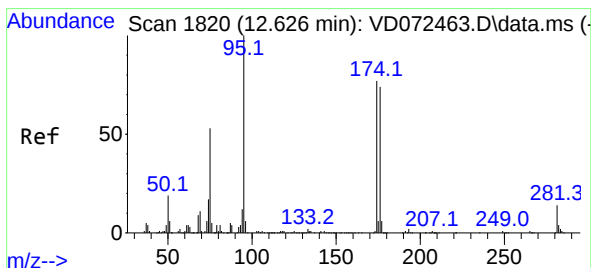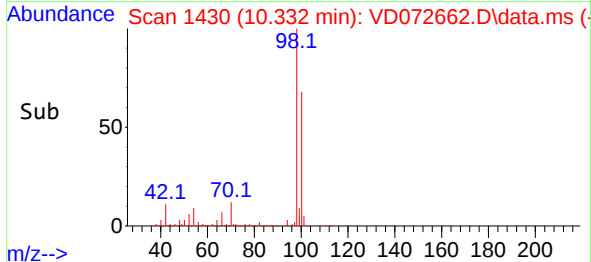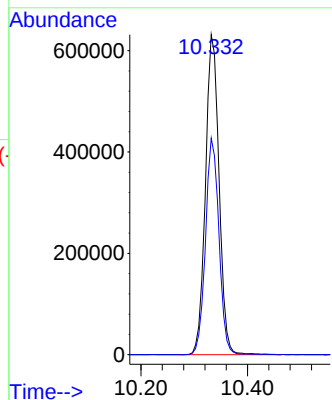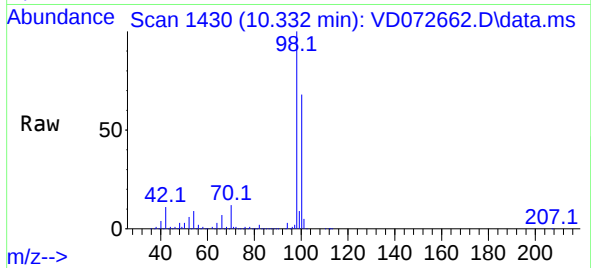

#62
4-Bromofluorobenzene
Concen: 39.135 ug/l
RT: 12.620 min Scan# 1819
Delta R.T. -0.006 min
Lab File: VD072662.D
Acq: 21 Apr 2022 11:07

Tgt Ion: 95 Resp: 382959
Ion Ratio Lower Upper
95 100
174 76.1 0.0 152.8
176 73.1 0.0 145.4


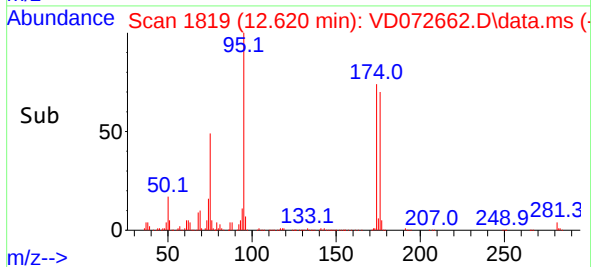
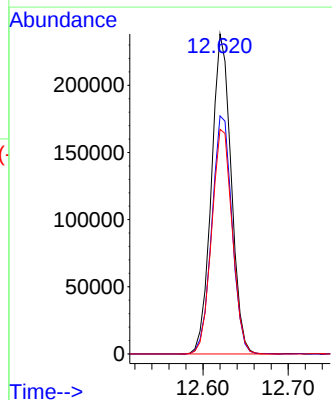
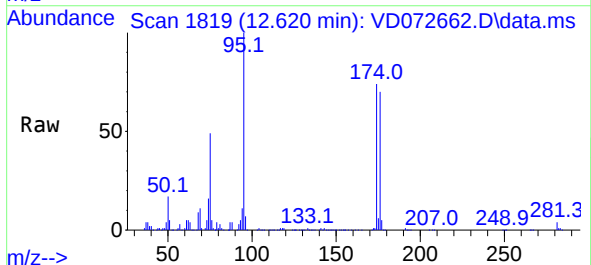


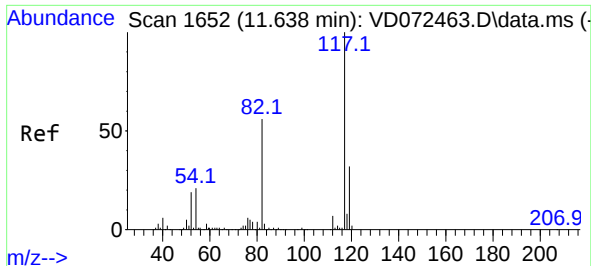

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.638 min Scan# 117
Delta R.T. 0.000 min
Lab File: VD072662.D
Acq: 21 Apr 2022 11:07

Instrument :
MSVOA_D
ClientSampleId :
VD0421SBL01

Tgt Ion:117 Resp: 864860
Ion Ratio Lower Upper
117 100
82 55.2 45.3 67.9
119 32.2 26.6 40.0

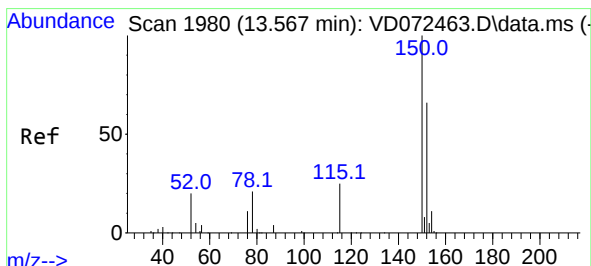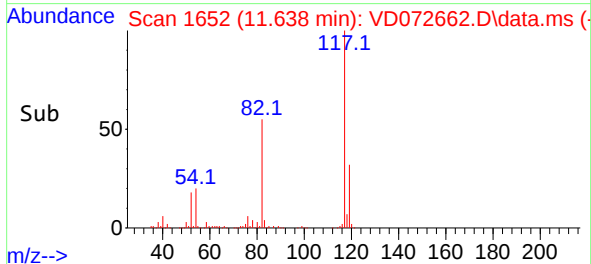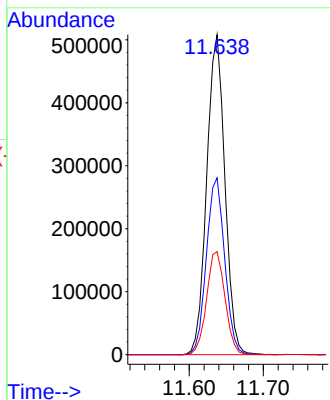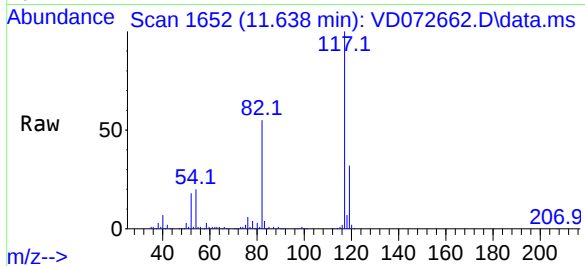

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.561 min Scan# 1979
Delta R.T. -0.006 min
Lab File: VD072662.D
Acq: 21 Apr 2022 11:07

Tgt Ion:152 Resp: 388898
Ion Ratio Lower Upper
152 100
115 61.4 31.3 93.8
150 160.6 0.0 348.6

