

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042221\
 Data File : VD068953.D
 Acq On : 22 Apr 2021 15:23
 Operator : VA/SY
 Sample : M2107-06
 Misc : 5.07G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 SB-30-9.5-10.0

Quant Time: Apr 23 08:46:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D040721S.M
 Quant Title : SW846 8260
 QLast Update : Thu Apr 08 03:50:31 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.985	168	95864	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.867	114	157632	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.644	117	204166	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.573	152	107330	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.338	65	57286	56.54	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 113.08%	
35) Dibromofluoromethane	7.920	113	59704	58.23	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 116.46%	
50) Toluene-d8	10.338	98	206381	53.36	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	= 106.72%	
62) 4-Bromofluorobenzene	12.632	95	82093	63.91	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	= 127.82%	


Target Compounds	Qvalue
-----	-----


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042221\
Data File : VD068953.D
Acq On : 22 Apr 2021 15:23
Operator : VA/SY
Sample : M2107-06
Misc : 5.07G/5.00ml/MSVOA_D/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
SB-30-9.5-10.0

Quant Time: Apr 23 08:46:11 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D040721S.M
Quant Title : SW846 8260
QLast Update : Thu Apr 08 03:50:31 2021
Response via : Initial Calibration




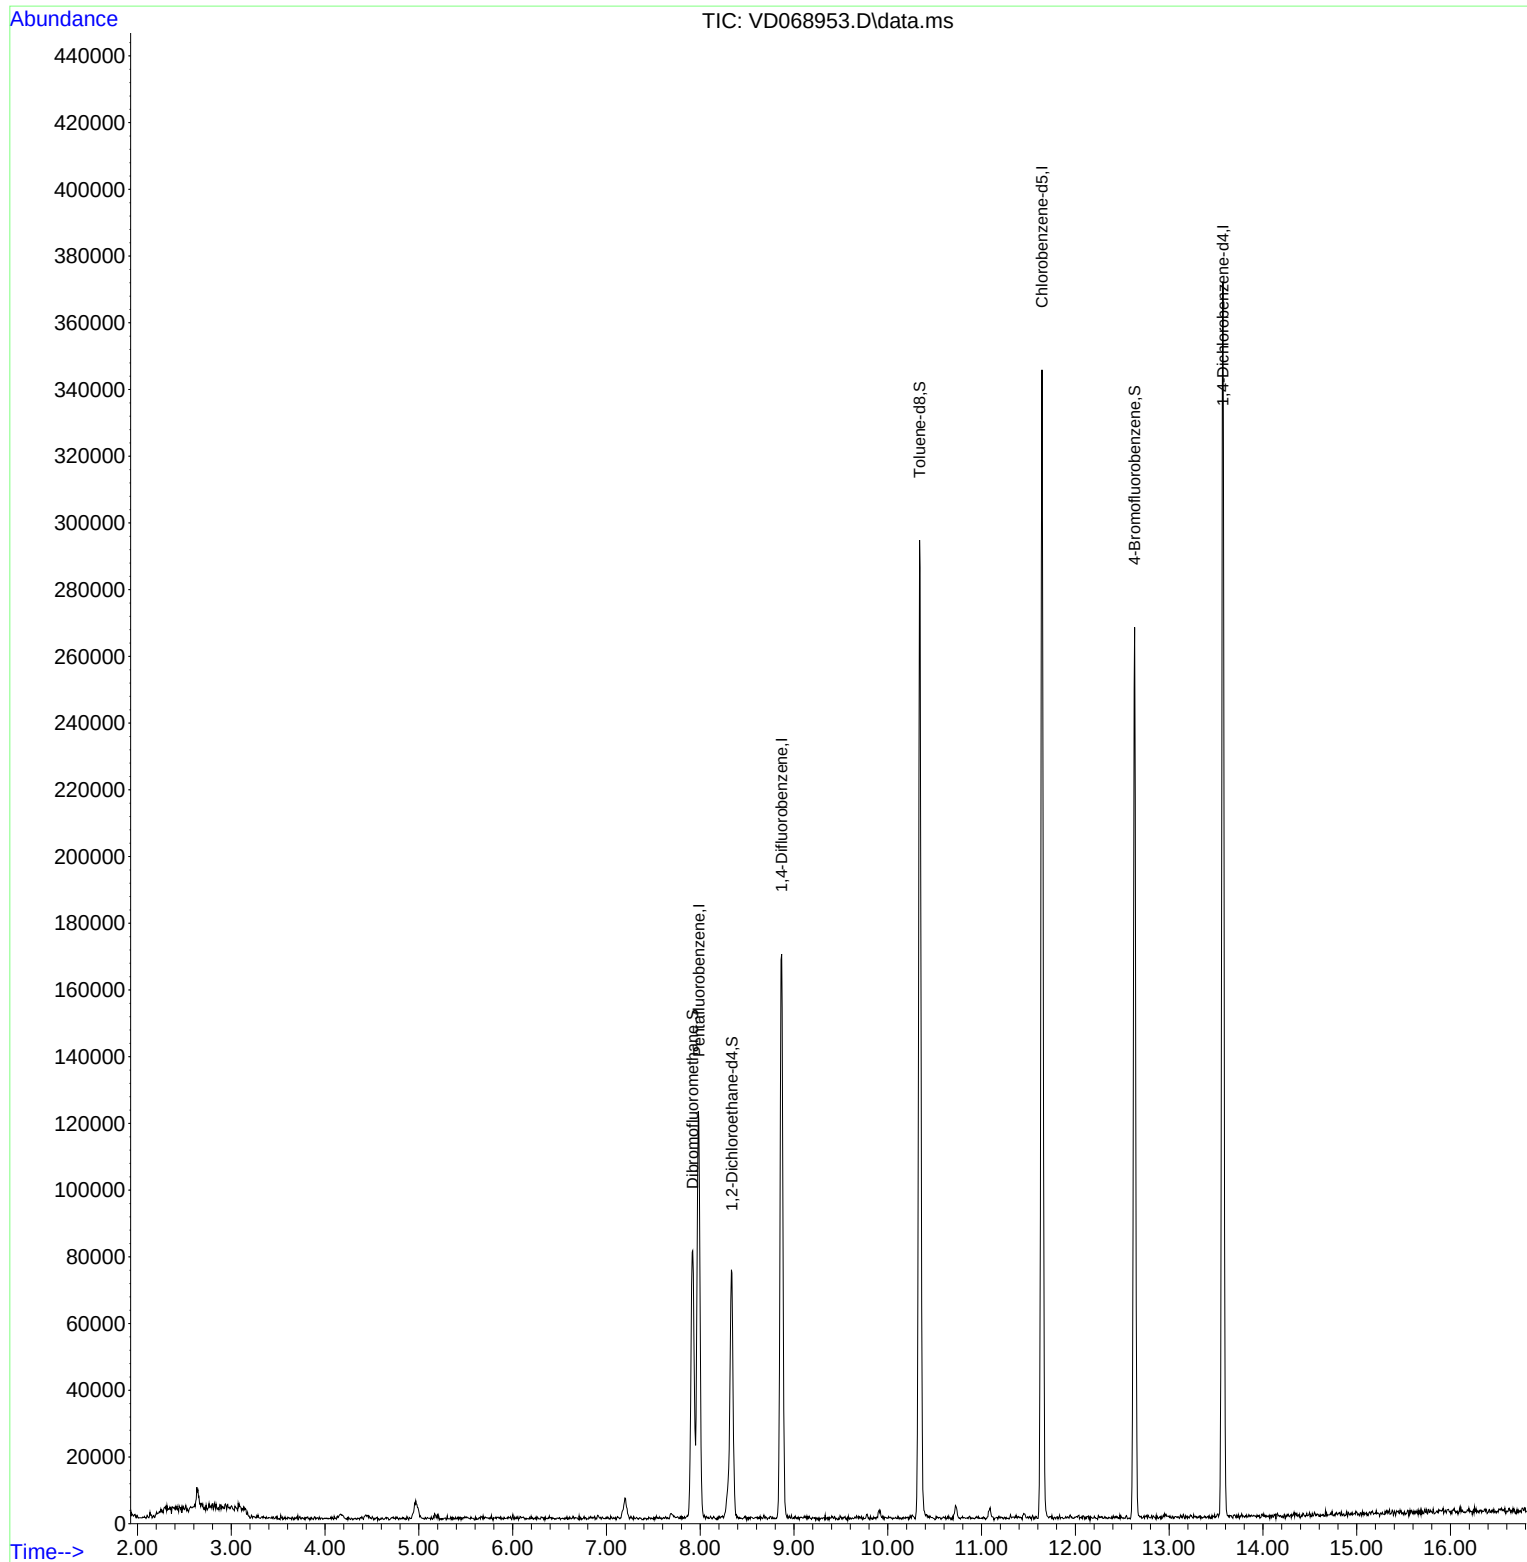


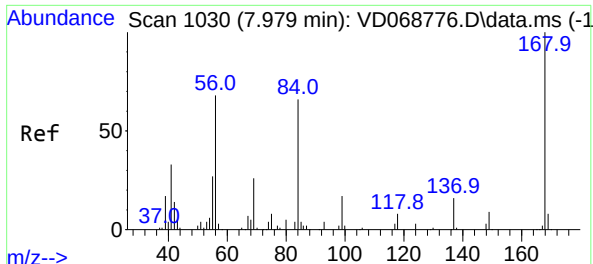

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.985 min Scan# 1031
Delta R.T. 0.006 min
Lab File: VD068953.D
Acq: 22 Apr 2021 15:23




Instrument :
MSVOA_D
ClientSampleId :
SB-30-9.5-10.0


Tgt Ion:168 Resp: 95864
Ion Ratio Lower Upper
168 100
99 49.1 46.2 69.2

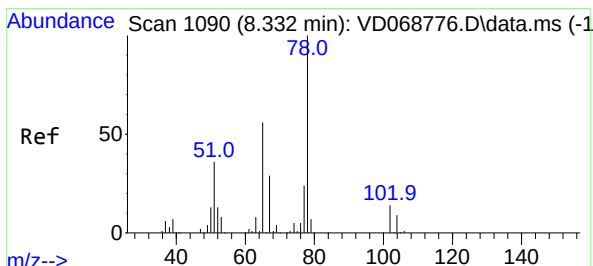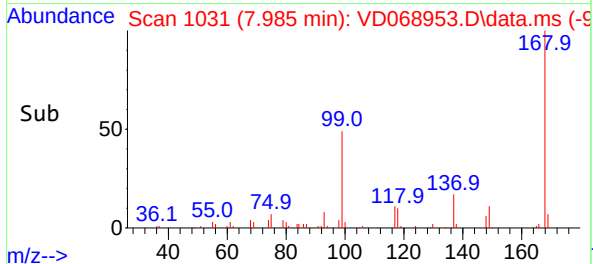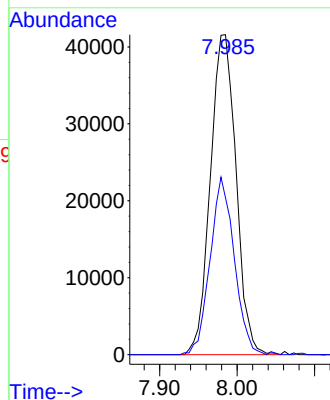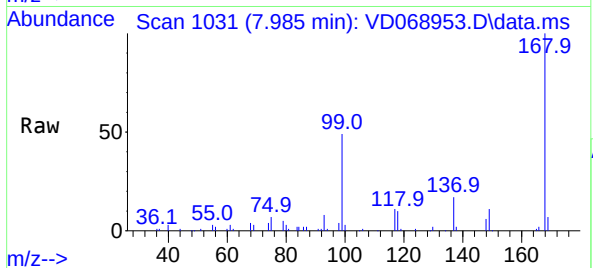

#33
1,2-Dichloroethane-d4
Concen: 56.54 ug/l
RT: 8.338 min Scan# 1091
Delta R.T. 0.006 min
Lab File: VD068953.D
Acq: 22 Apr 2021 15:23

Tgt Ion: 65 Resp: 57286
Ion Ratio Lower Upper
65 100
67 52.5 0.0 106.0


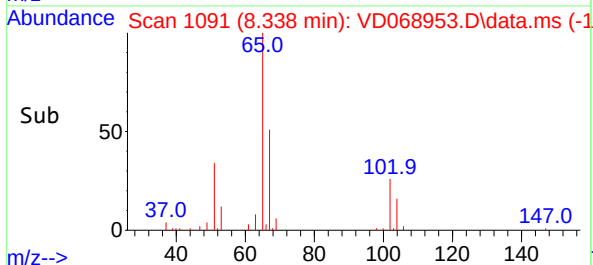
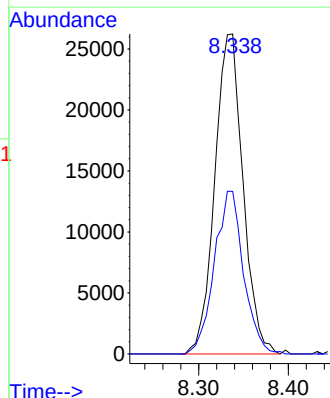
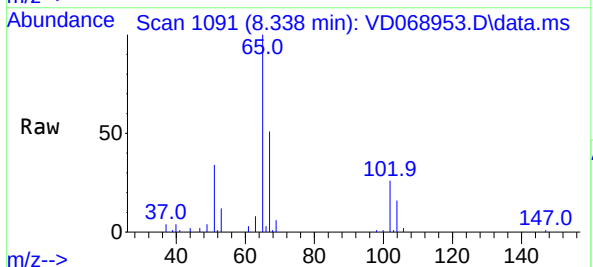


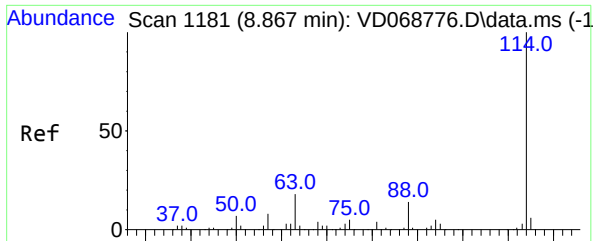

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.867 min Scan# 1181
Delta R.T. 0.000 min
Lab File: VD068953.D
Acq: 22 Apr 2021 15:23




Instrument :
MSVOA_D
ClientSampleId :
SB-30-9.5-10.0


Tgt Ion:114 Resp: 157632
Ion Ratio Lower Upper
114 100
63 17.5 0.0 38.2
88 15.3 0.0 29.4

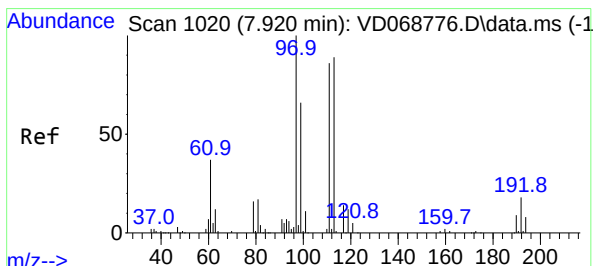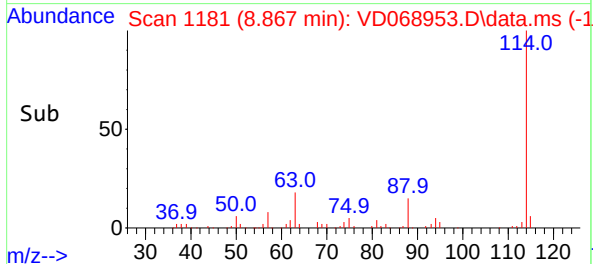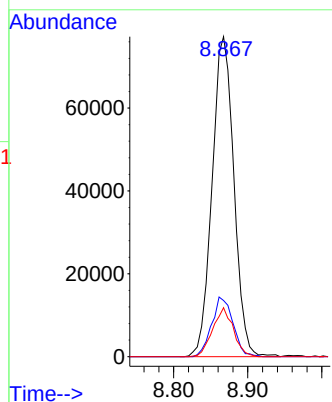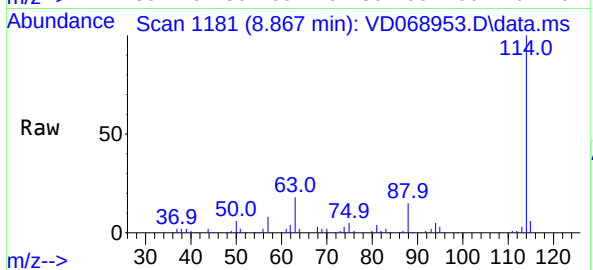

#35
Dibromofluoromethane
Concen: 58.23 ug/l
RT: 7.920 min Scan# 1020
Delta R.T. 0.000 min
Lab File: VD068953.D
Acq: 22 Apr 2021 15:23

Tgt Ion:113 Resp: 59704
Ion Ratio Lower Upper
113 100
111 103.1 82.5 123.7
192 20.4 15.1 22.7


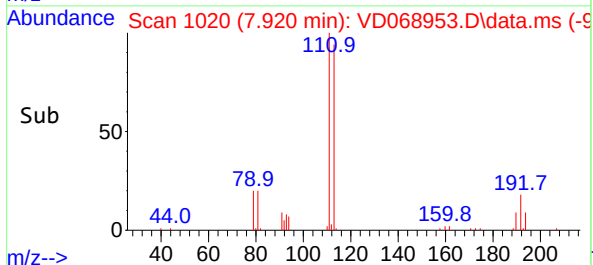
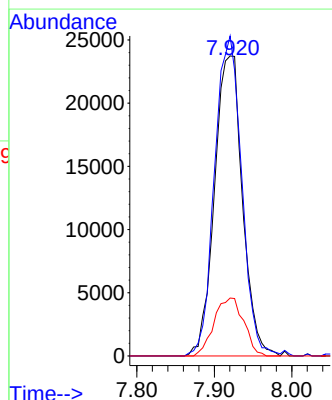
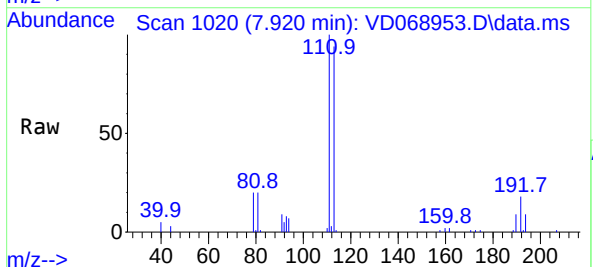


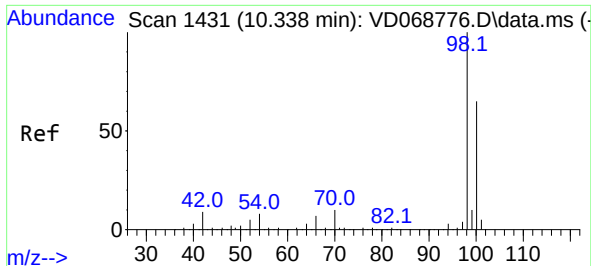

#50
Toluene-d8
Concen: 53.36 ug/l
RT: 10.338 min Scan# 1431
Delta R.T. -0.000 min
Lab File: VD068953.D
Acq: 22 Apr 2021 15:23




Instrument :
MSVOA_D
ClientSampleId :
SB-30-9.5-10.0


Tgt Ion: 98 Resp: 206381
Ion Ratio Lower Upper
98 100
100 64.8 51.8 77.6

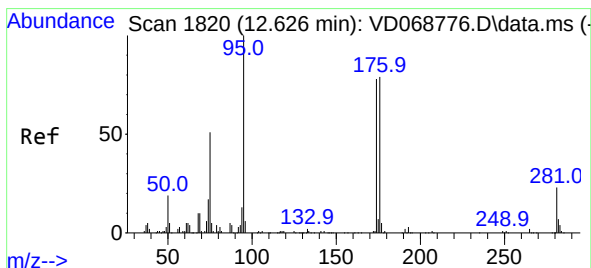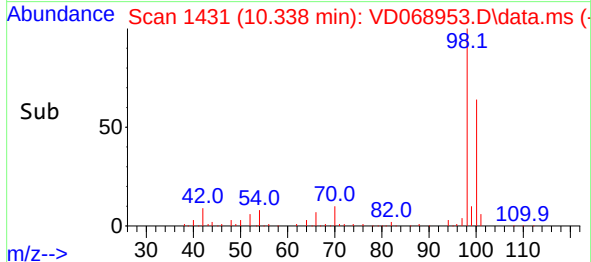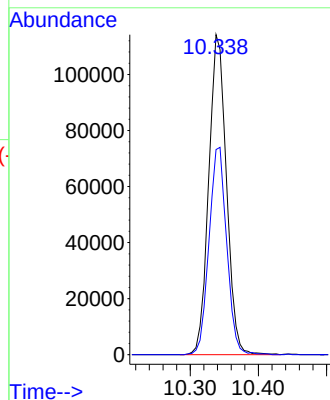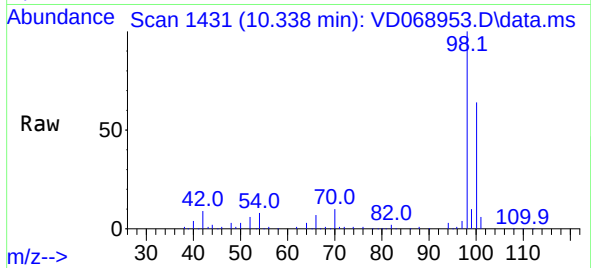

#62
4-Bromofluorobenzene
Concen: 63.91 ug/l
RT: 12.632 min Scan# 1821
Delta R.T. 0.006 min
Lab File: VD068953.D
Acq: 22 Apr 2021 15:23

Tgt Ion: 95 Resp: 82093
Ion Ratio Lower Upper
95 100
174 93.9 0.0 168.0
176 91.9 0.0 160.2


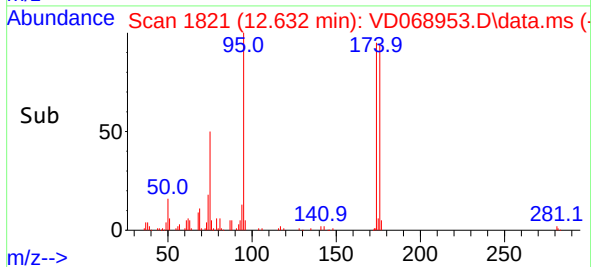
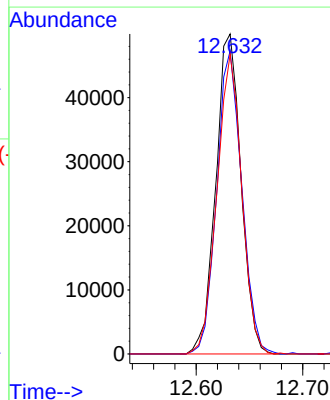
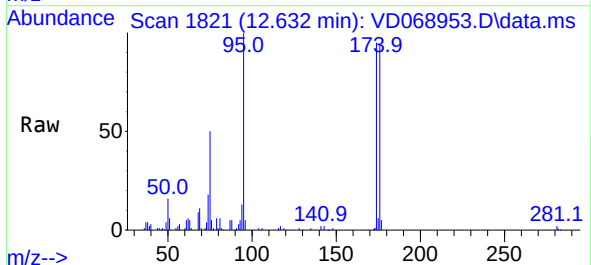


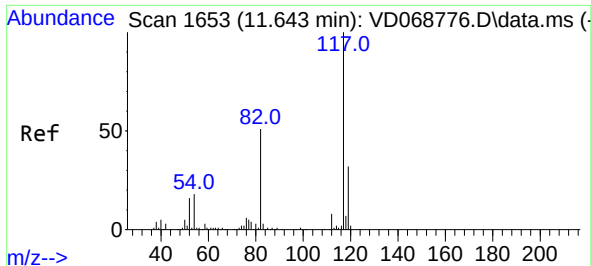

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.644 min Scan# 1653
Delta R.T. 0.001 min
Lab File: VD068953.D
Acq: 22 Apr 2021 15:23

Instrument :
MSVOA_D
ClientSampleId :
SB-30-9.5-10.0

Tgt Ion:	117	Resp:	204166
Ion	Ratio	Lower	Upper
117	100		
82	48.9	43.5	65.3
119	30.4	26.7	40.1

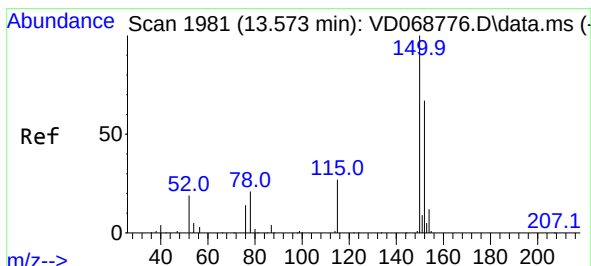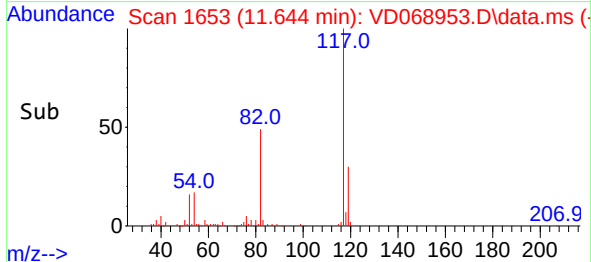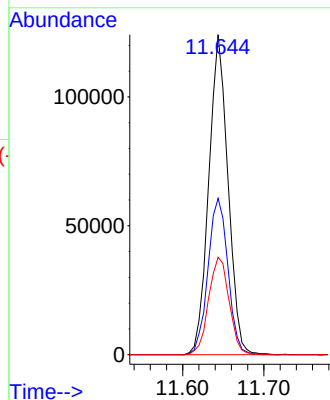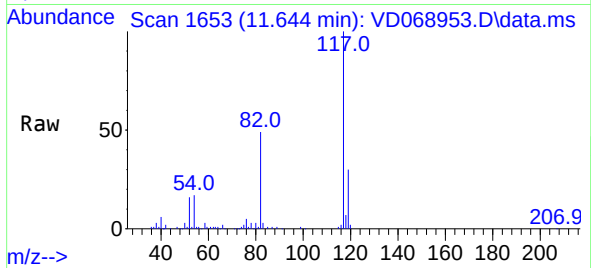

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.573 min Scan# 1981
Delta R.T. -0.000 min
Lab File: VD068953.D
Acq: 22 Apr 2021 15:23

Tgt Ion:	152	Resp:	107330
Ion	Ratio	Lower	Upper
152	100		
115	55.1	29.3	87.8
150	155.2	0.0	347.6

