
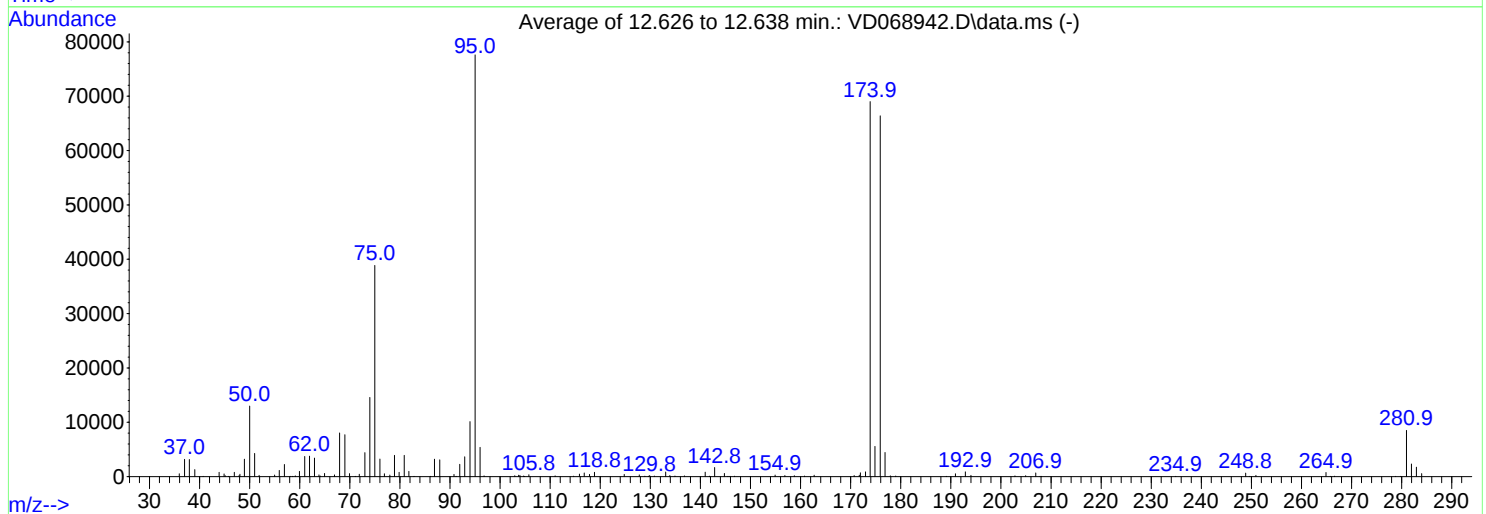


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042221\
Data File : VD068942.D
Acq On : 22 Apr 2021 09:05
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D040721S.M
Title : SW846 8260
Last Update : Thu Apr 08 03:50:31 2021

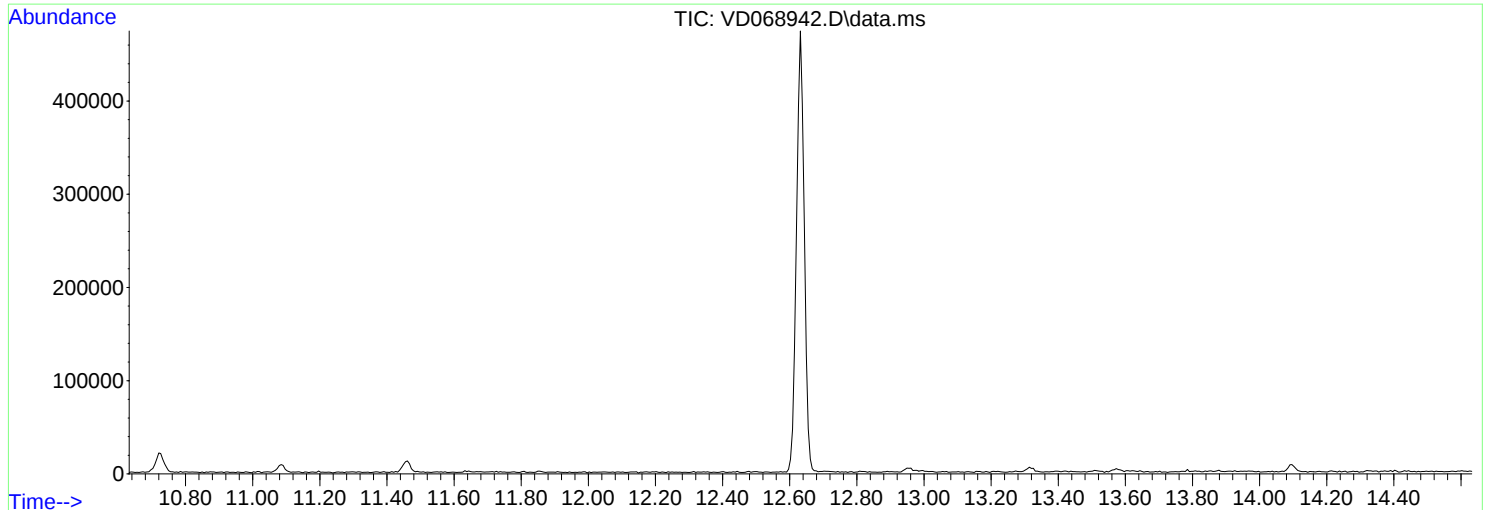

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	12989	PASS
75	95	30	60	50.1	38875	PASS
95	95	100	100	100.0	77608	PASS
96	95	5	9	7.0	5395	PASS
173	174	0.00	2	1.3	873	PASS
174	95	50	100	88.9	69008	PASS
175	174	5	9	8.0	5553	PASS
176	174	95	101	96.2	66403	PASS
177	176	5	9	6.7	4459	PASS