



Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D042319S.M
Calibration Table Last Updated: Tue Apr 23 14:52:55 2019

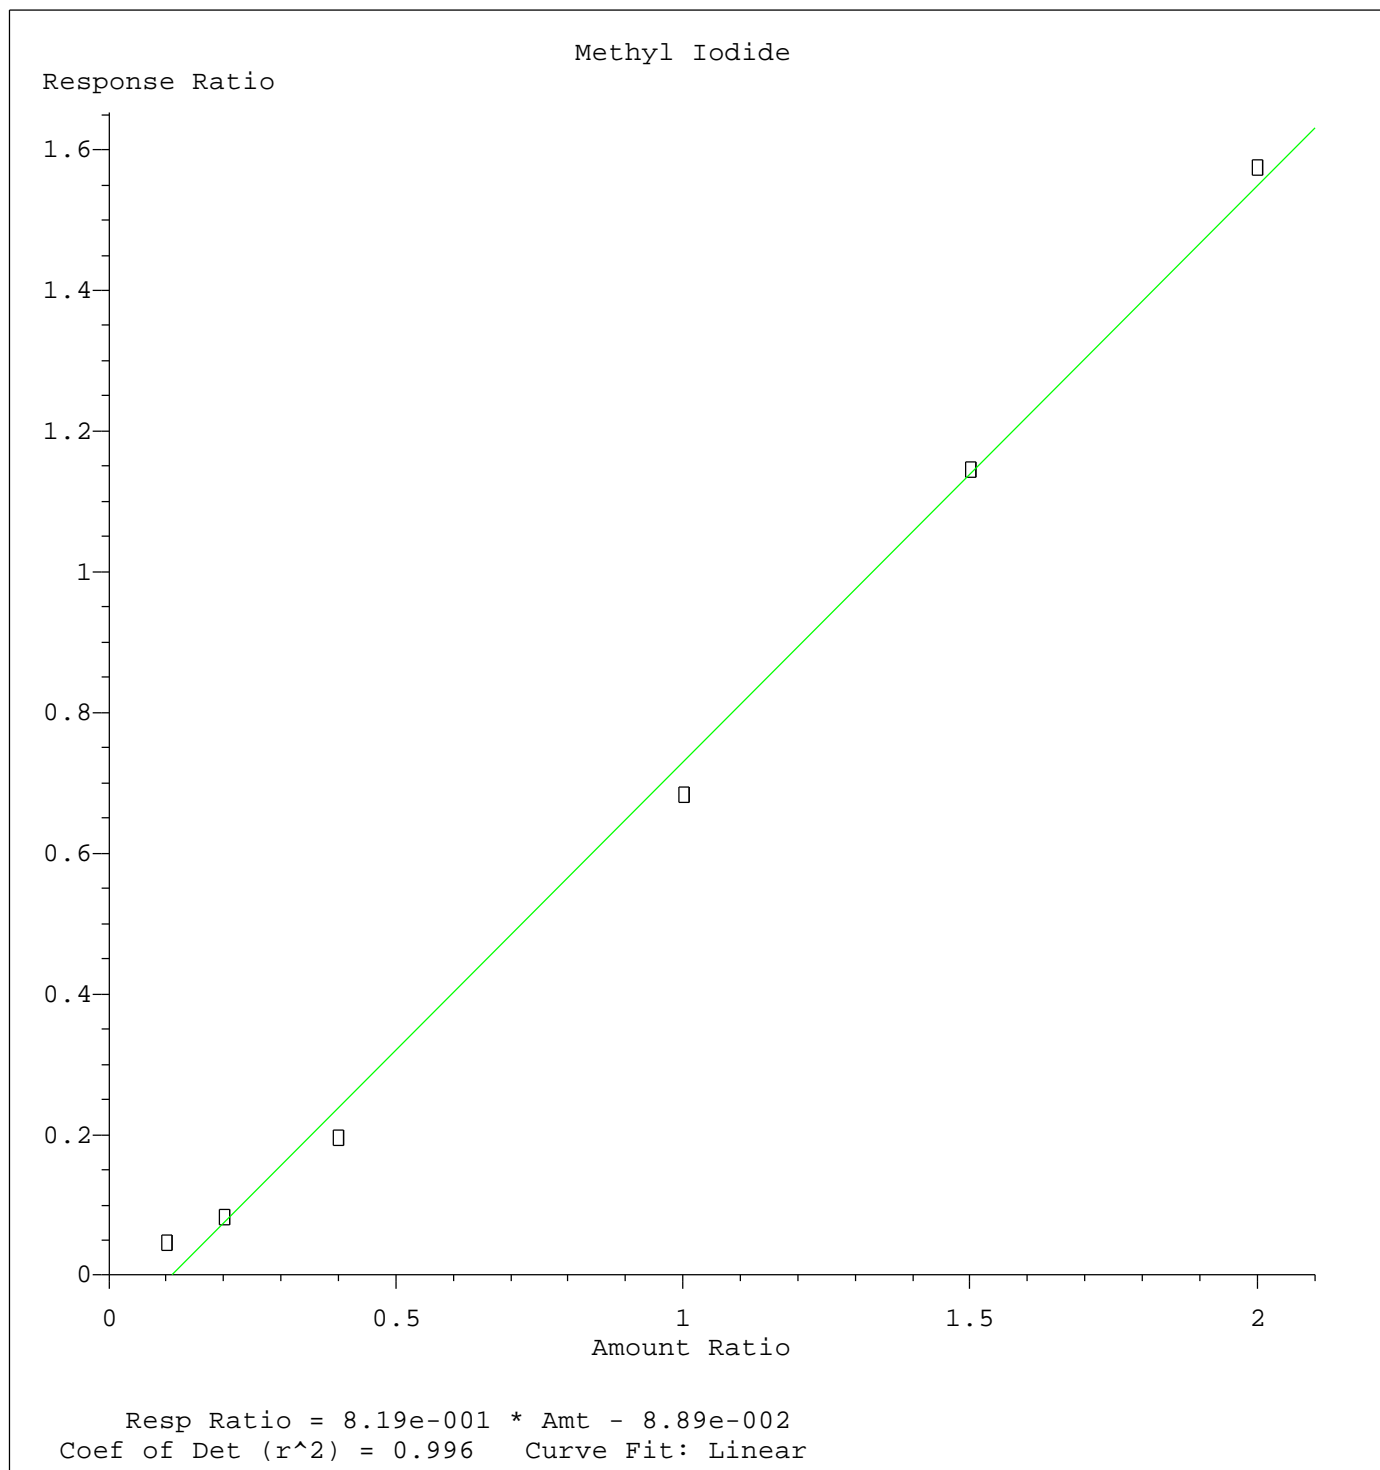


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D042319S.M
Calibration Table Last Updated: Tue Apr 23 14:52:55 2019

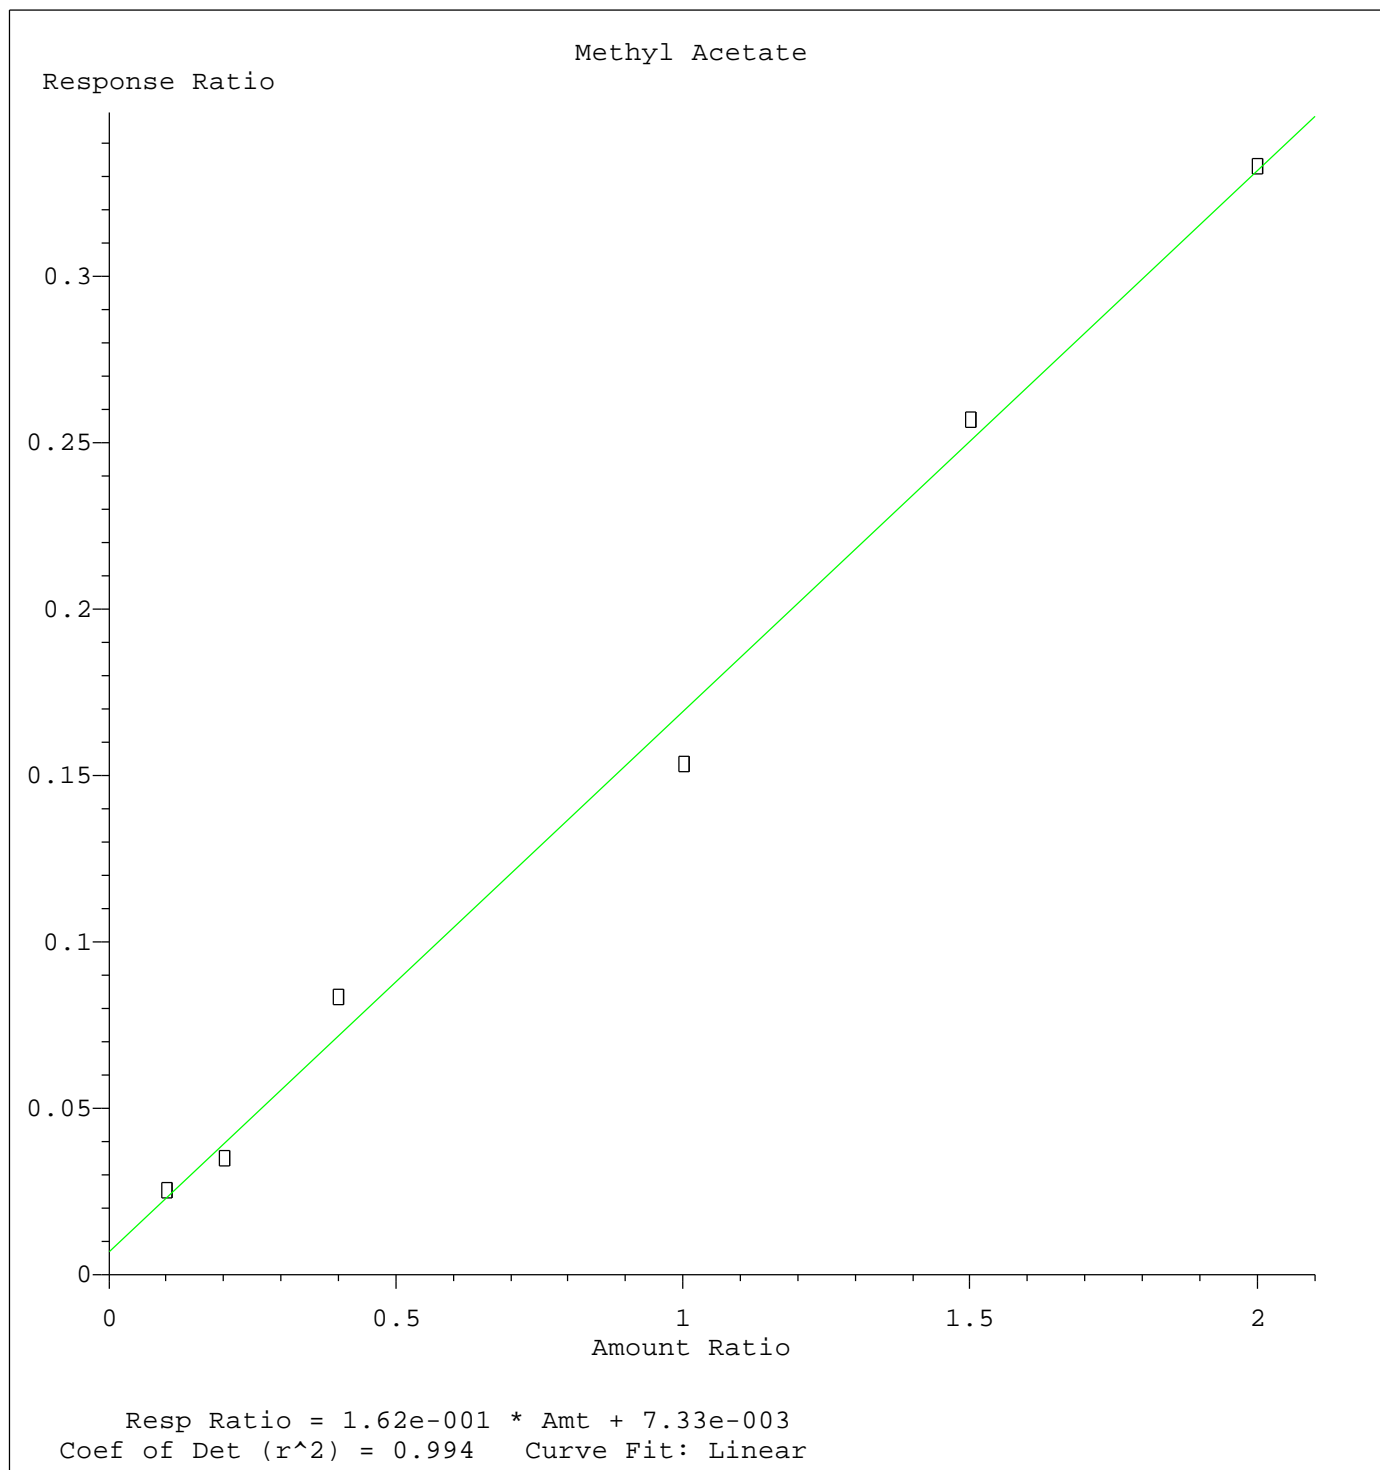

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D042319S.M
Calibration Table Last Updated: Tue Apr 23 14:52:55 2019

Methylene Chloride


Response Ratio

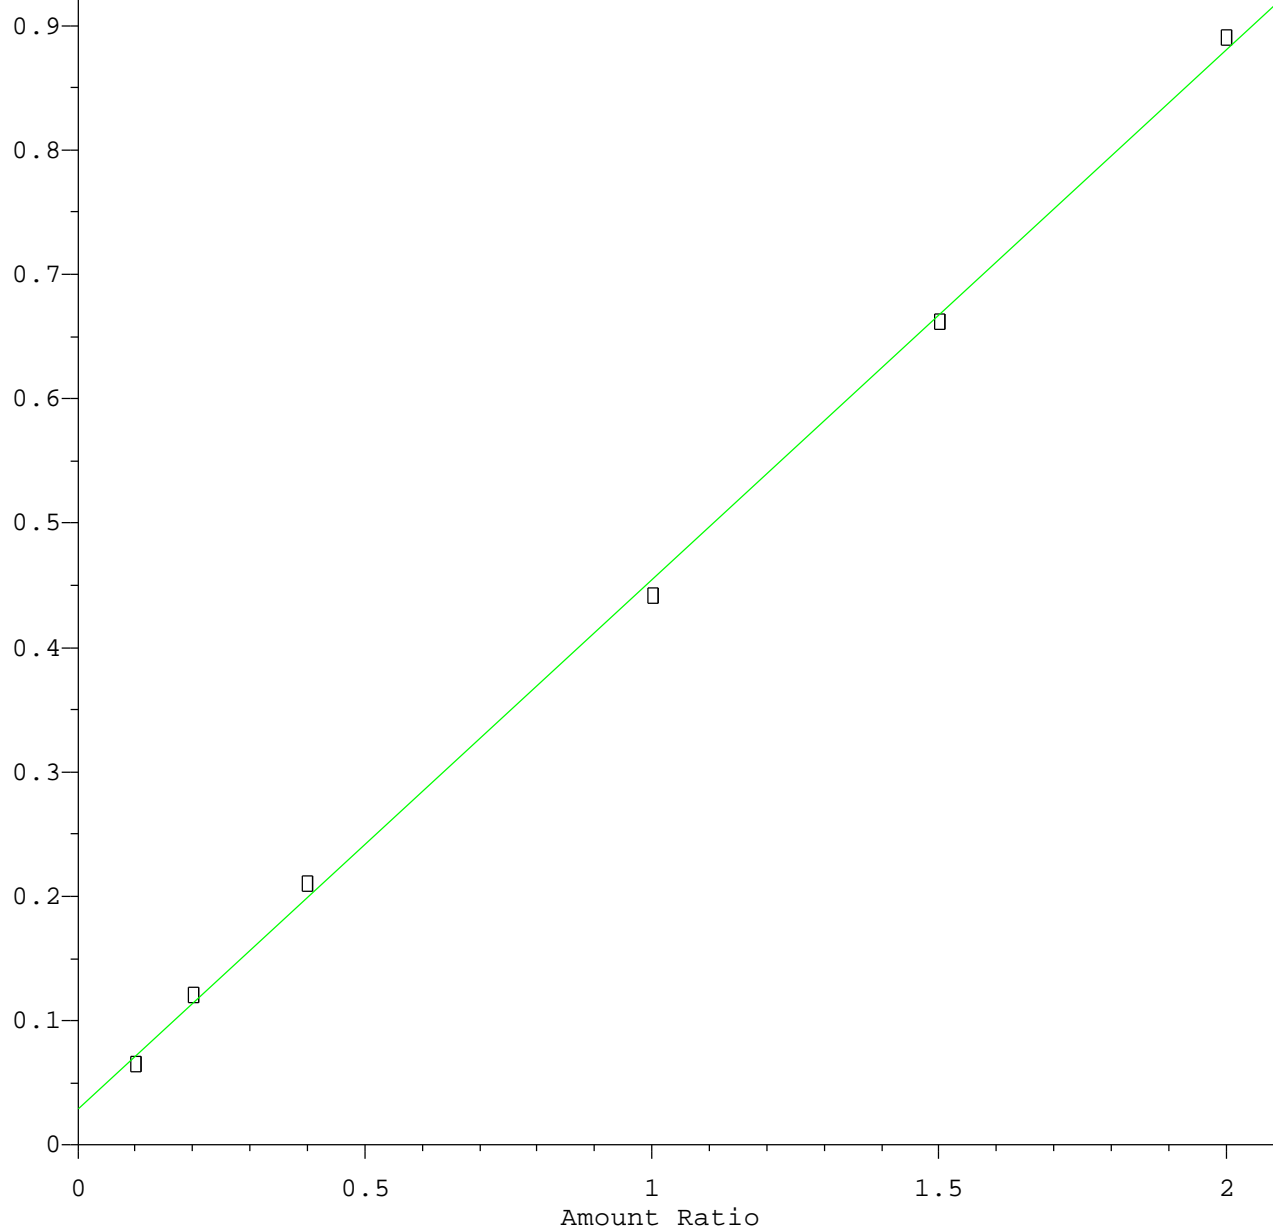

Resp Ratio = $4.26 \times 10^{-1} \times \text{Amt} + 2.90 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D042319S.M
Calibration Table Last Updated: Tue Apr 23 14:52:55 2019

1,2-Dibromo-3-Chloropropane

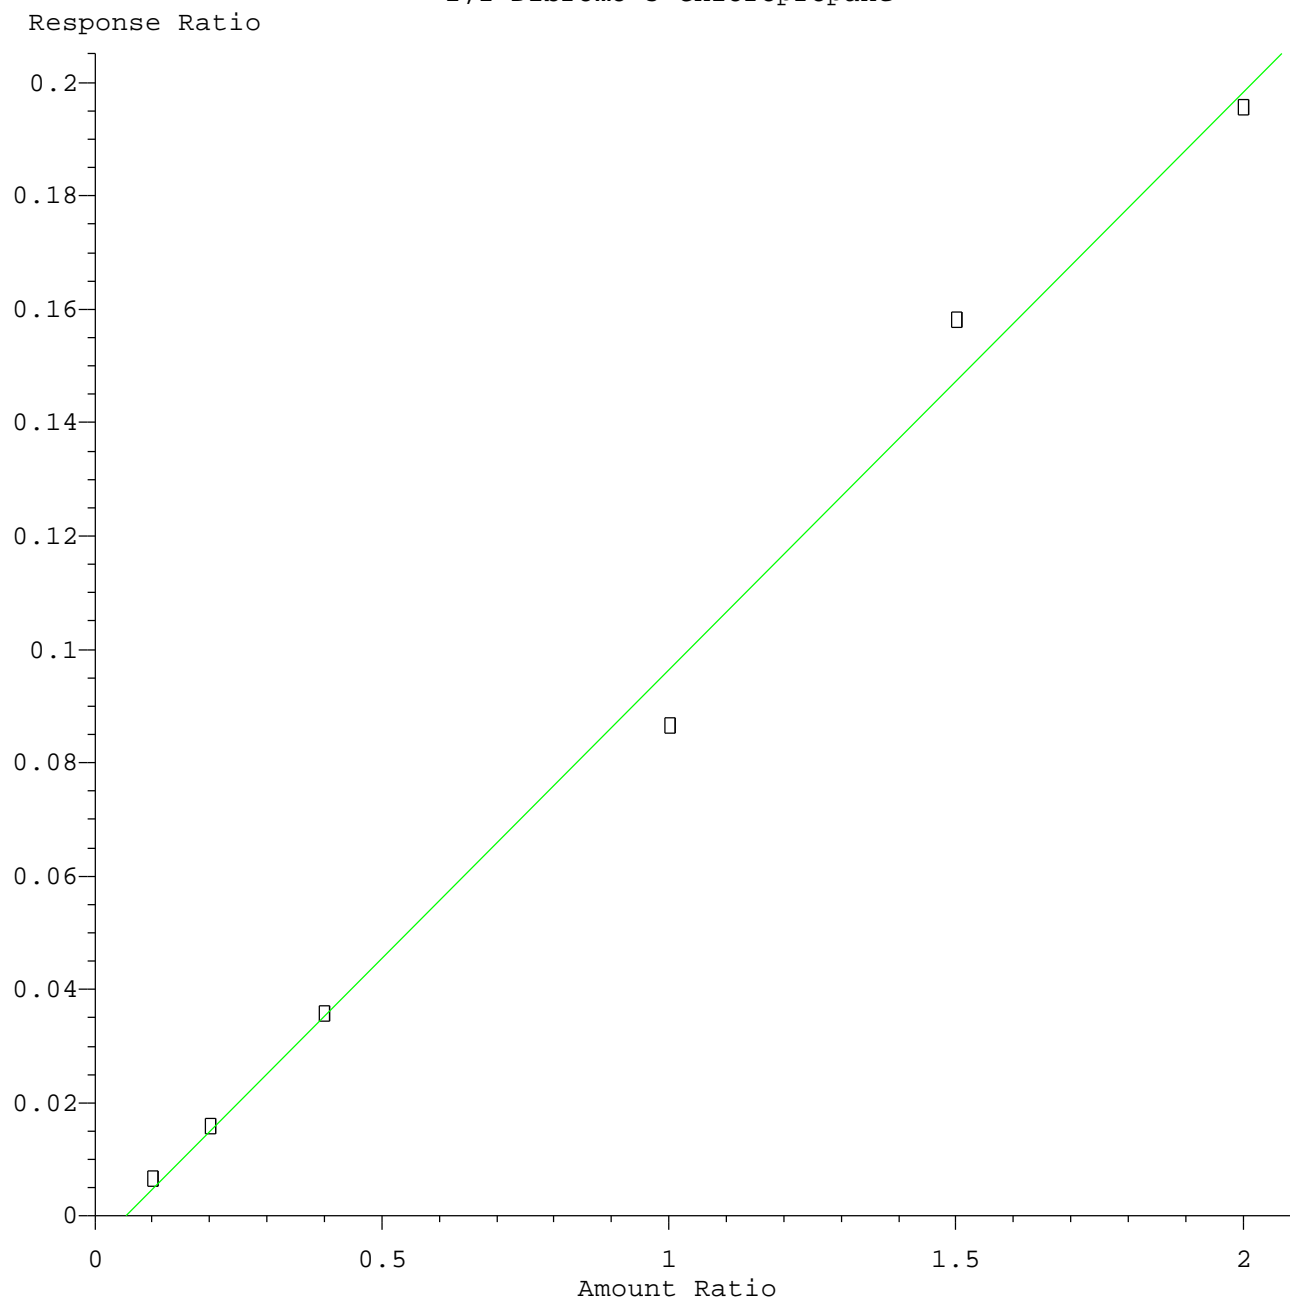

Resp Ratio = $1.02 \times 10^{-1} \times \text{Amt} - 5.38 \times 10^{-3}$
Coef of Det (r^2) = 0.993 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D042319S.M
Calibration Table Last Updated: Tue Apr 23 14:52:55 2019