


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD042319\
 Data File : VD061961.D
 Acq On : 23 Apr 2019 9:05
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µl/5ml/MSVOA D/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D042319S.M
 Title : SW846 8260
 Last Update : Tue Apr 23 14:52:55 2019

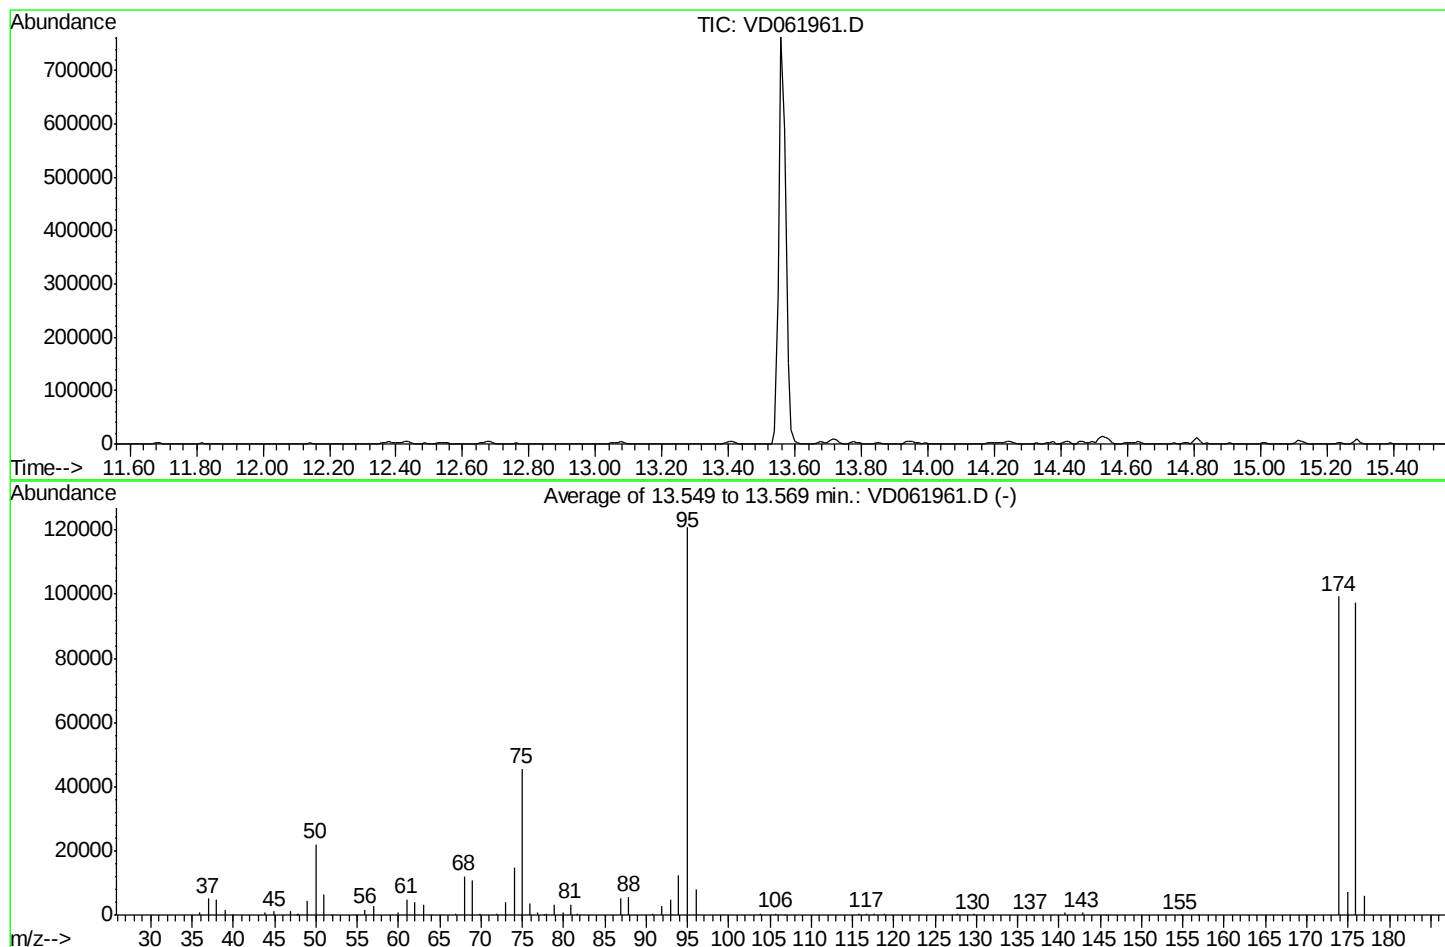

AutoFind: Scans 1232, 1233, 1234; Background Corrected with Scan 1228

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	22103	PASS
75	95	30	60	37.8	45666	PASS
95	95	100	100	100.0	120885	PASS
96	95	5	9	6.5	7892	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	82.1	99250	PASS
175	174	5	9	7.2	7195	PASS
176	174	95	101	98.2	97437	PASS
177	176	5	9	6.1	5983	PASS