


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD042319\
Data File : VD061982.D
Acq On : 23 Apr 2019 22:07
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D042319S.M
Title : SW846 8260
Last Update : Tue Apr 23 14:52:55 2019

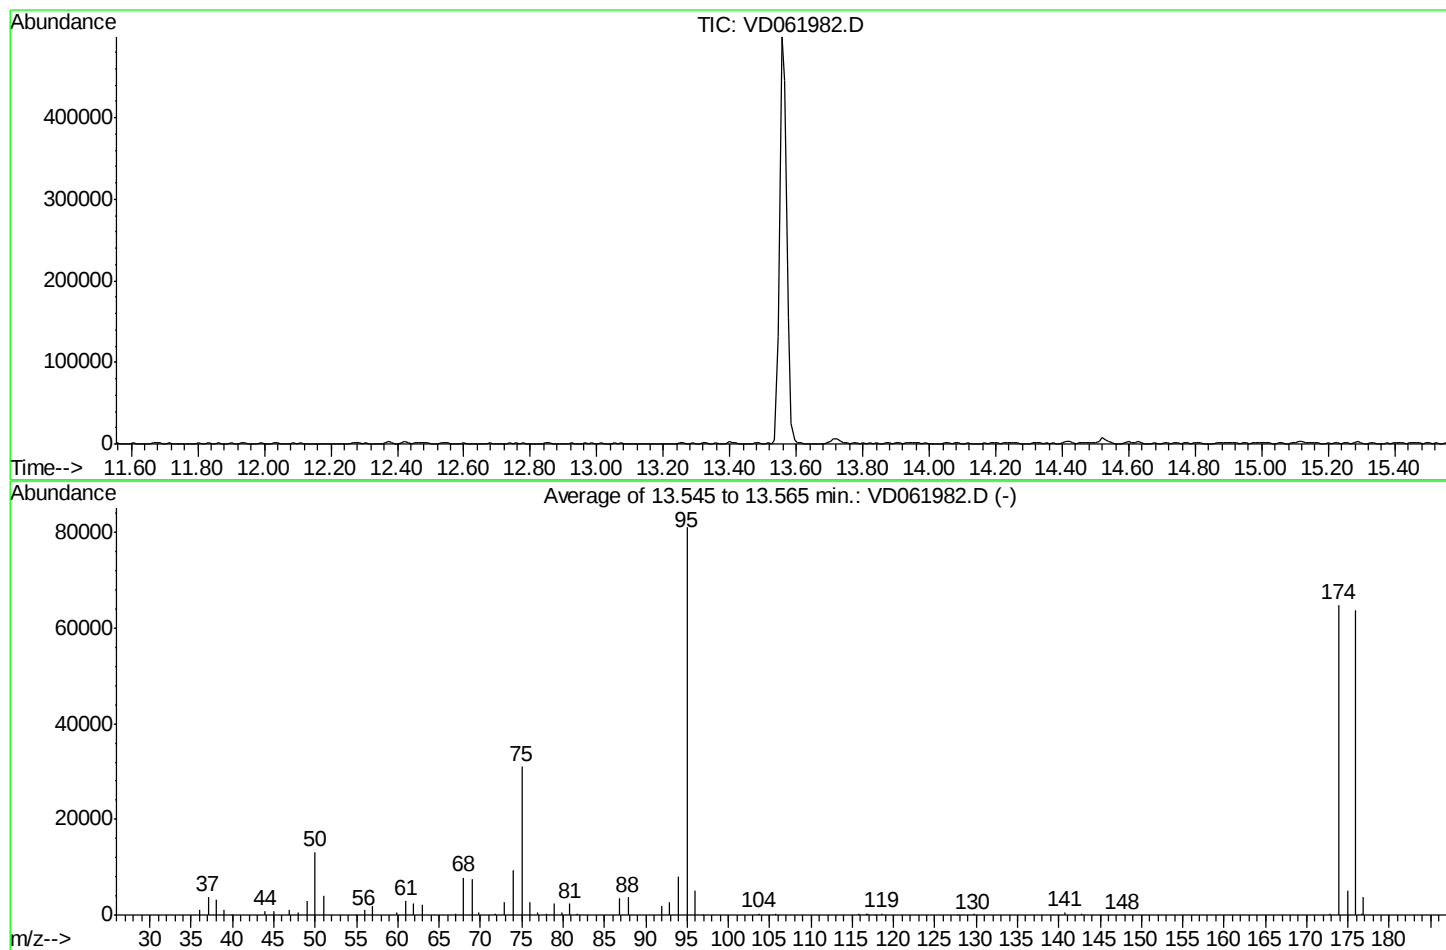

AutoFind: Scans 1231, 1232, 1233; Background Corrected with Scan 1227

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	13187	PASS
75	95	30	60	38.2	30945	PASS
95	95	100	100	100.0	81104	PASS
96	95	5	9	6.1	4967	PASS
173	174	0.00	2	0.2	158	PASS
174	95	50	100	80.0	64895	PASS
175	174	5	9	8.0	5160	PASS
176	174	95	101	98.3	63769	PASS
177	176	5	9	5.7	3633	PASS