

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042321\
 Data File : VD068962.D
 Acq On : 23 Apr 2021 12:44
 Operator : VA/SY
 Sample : M2107-14
 Misc : 5.06G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 SB-33-0-2.0

Quant Time: Apr 26 07:54:37 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D040721S.M
 Quant Title : SW846 8260
 QLast Update : Thu Apr 08 03:50:31 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.985	168	330115	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.867	114	562607	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.643	117	621439	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.573	152	291542	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.338	65	132206	37.89	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	75.78%
35) Dibromofluoromethane	7.920	113	166366	45.46	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	90.92%
50) Toluene-d8	10.344	98	703430	50.96	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	101.92%
62) 4-Bromofluorobenzene	12.632	95	268086	58.47	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	116.94%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042321\
Data File : VD068962.D
Acq On : 23 Apr 2021 12:44
Operator : VA/SY
Sample : M2107-14
Misc : 5.06G/5.00ml/MSVOA_D/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
SB-33-0-2.0

Quant Time: Apr 26 07:54:37 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D040721S.M
Quant Title : SW846 8260
QLast Update : Thu Apr 08 03:50:31 2021
Response via : Initial Calibration




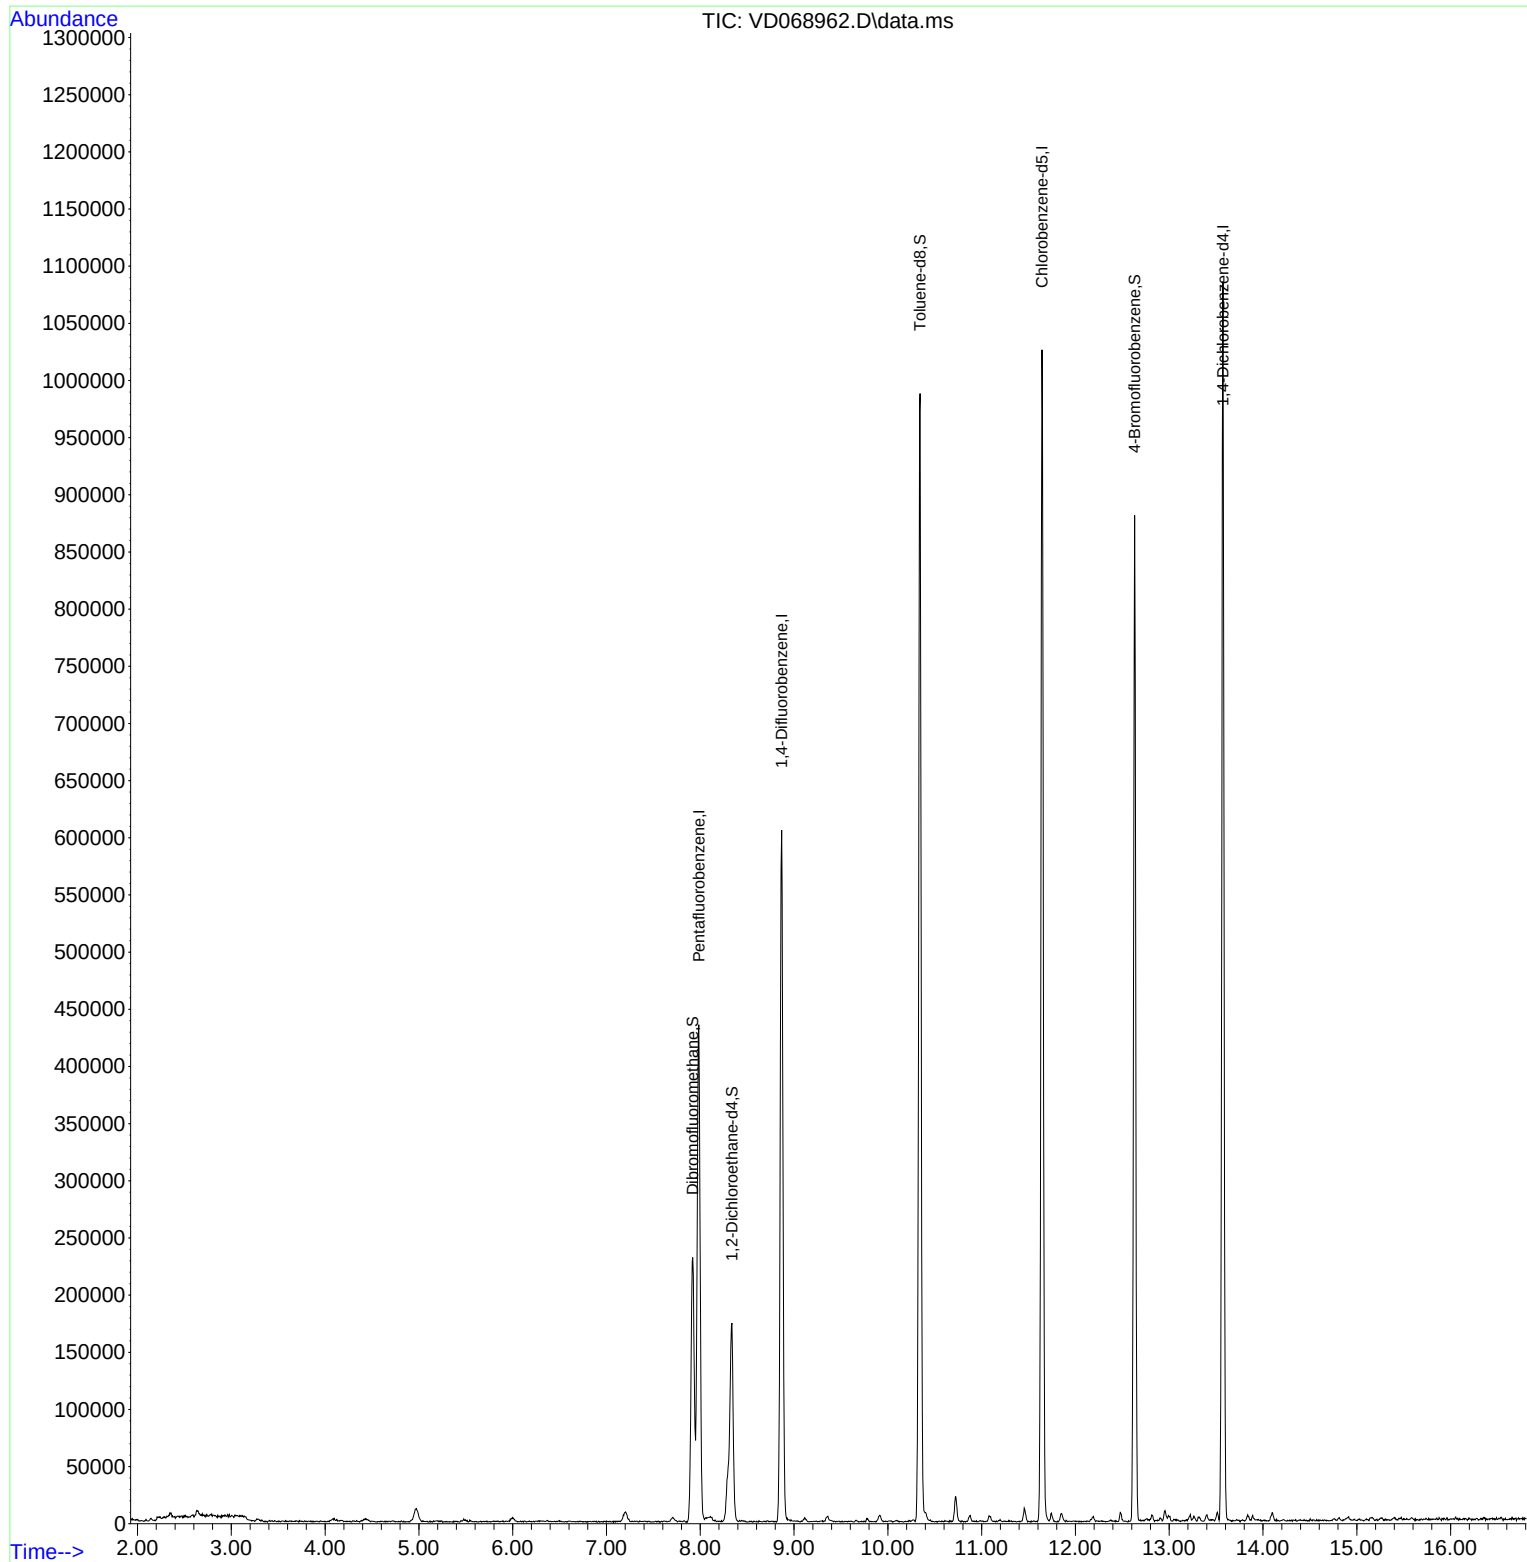


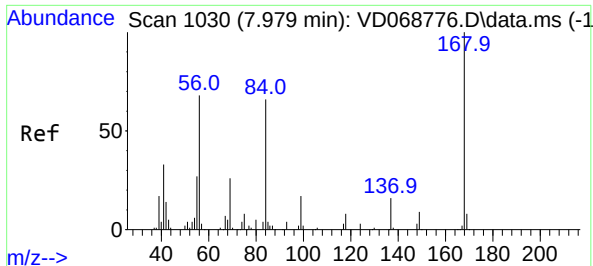

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.985 min Scan# 1031
Delta R.T. 0.006 min
Lab File: VD068962.D
Acq: 23 Apr 2021 12:44




Instrument :
MSVOA_D
ClientSampleId :
SB-33-0-2.0


Tgt Ion:168 Resp: 330115
Ion Ratio Lower Upper
168 100
99 52.7 46.2 69.2

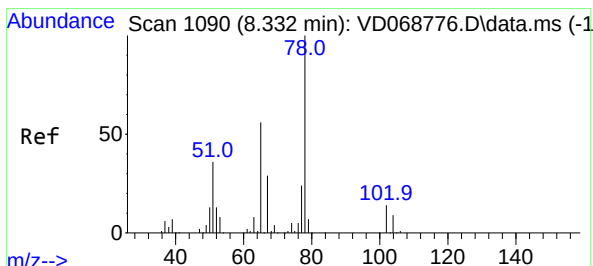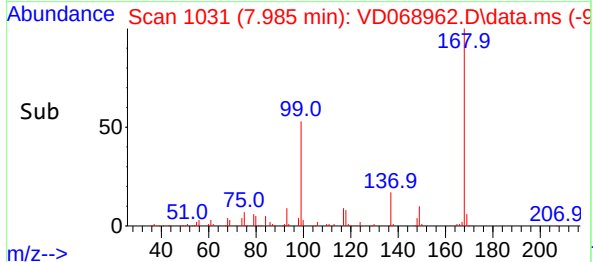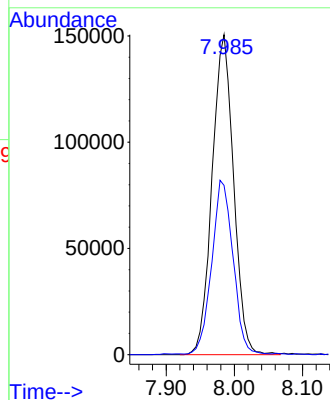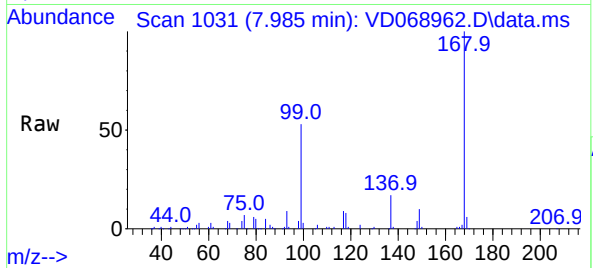

#33
1,2-Dichloroethane-d4
Concen: 37.89 ug/l
RT: 8.338 min Scan# 1091
Delta R.T. 0.006 min
Lab File: VD068962.D
Acq: 23 Apr 2021 12:44

Tgt Ion: 65 Resp: 132206
Ion Ratio Lower Upper
65 100
67 54.2 0.0 106.0


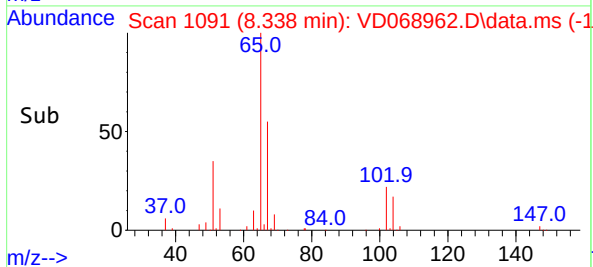
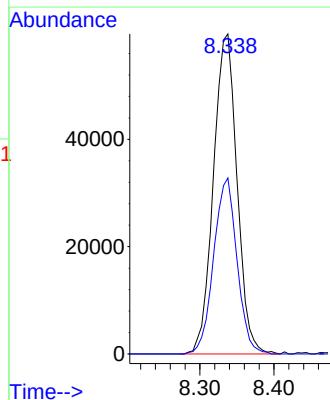
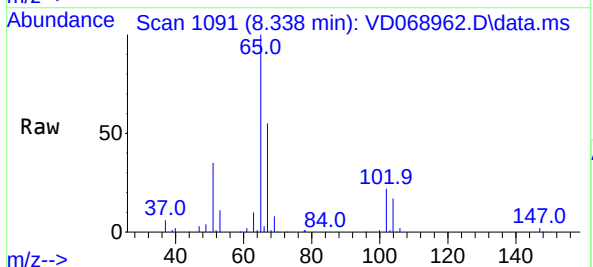


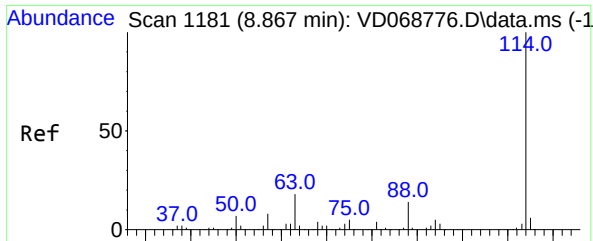

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.867 min Scan# 1181
Delta R.T. 0.000 min
Lab File: VD068962.D
Acq: 23 Apr 2021 12:44




Instrument :
MSVOA_D
ClientSampleId :
SB-33-0-2.0


Tgt Ion:114 Resp: 562607
Ion Ratio Lower Upper
114 100
63 17.6 0.0 38.2
88 14.5 0.0 29.4

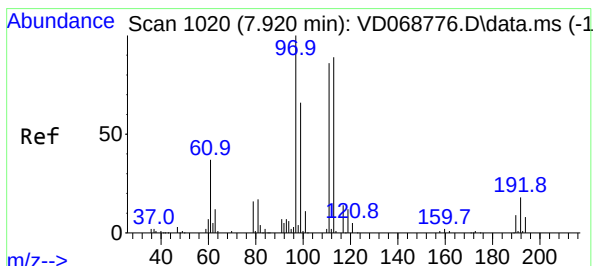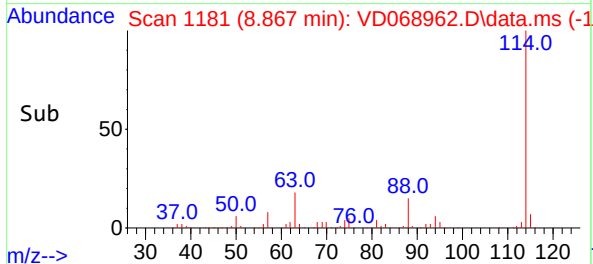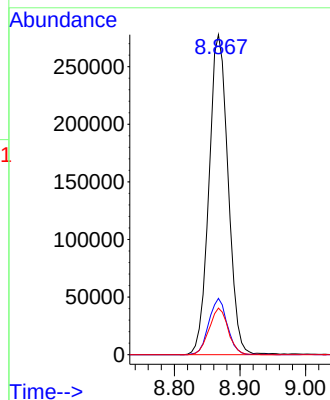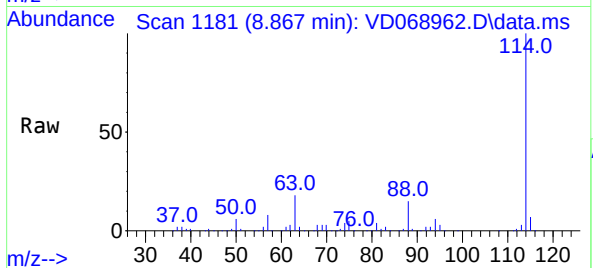

#35
Dibromofluoromethane
Concen: 45.46 ug/l
RT: 7.920 min Scan# 1020
Delta R.T. 0.000 min
Lab File: VD068962.D
Acq: 23 Apr 2021 12:44

Tgt Ion:113 Resp: 166366
Ion Ratio Lower Upper
113 100
111 104.7 82.5 123.7
192 20.4 15.1 22.7


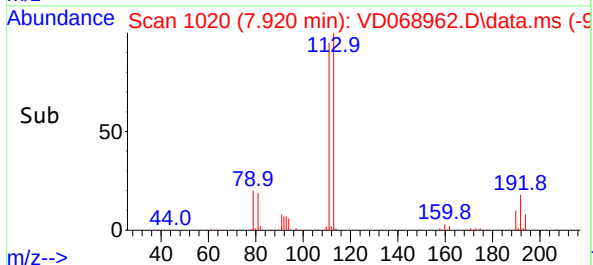
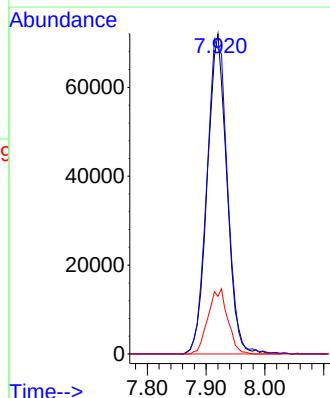
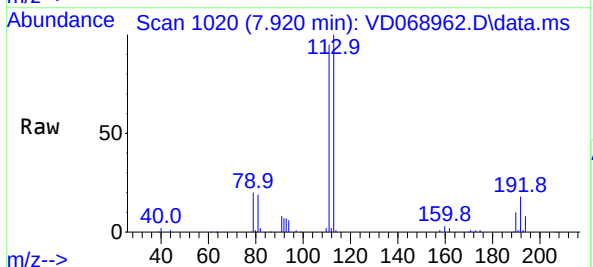


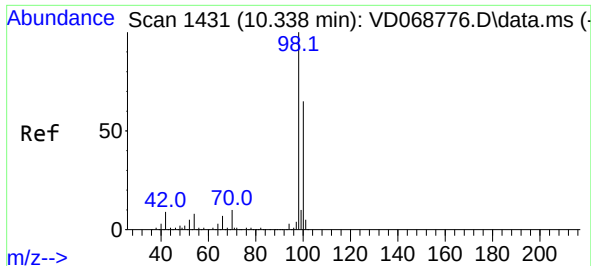

#50
Toluene-d8
Concen: 50.96 ug/l
RT: 10.344 min Scan# 1432
Delta R.T. 0.006 min
Lab File: VD068962.D
Acq: 23 Apr 2021 12:44




Instrument :
MSVOA_D
ClientSampleId :
SB-33-0-2.0


Tgt Ion: 98 Resp: 703430
Ion Ratio Lower Upper
98 100
100 65.0 51.8 77.6

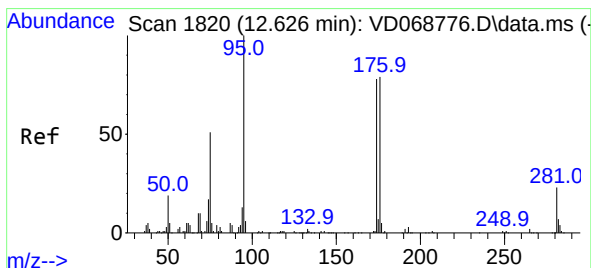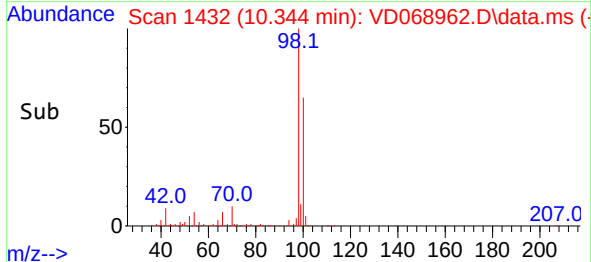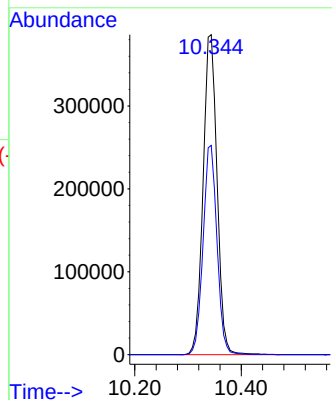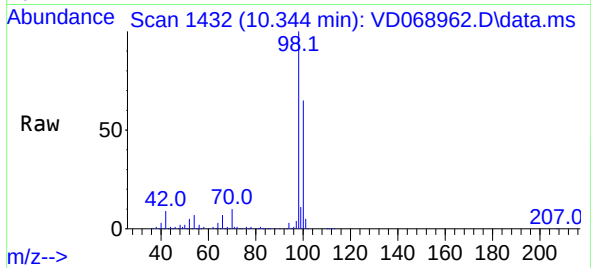

#62
4-Bromofluorobenzene
Concen: 58.47 ug/l
RT: 12.632 min Scan# 1821
Delta R.T. 0.006 min
Lab File: VD068962.D
Acq: 23 Apr 2021 12:44

Tgt Ion: 95 Resp: 268086
Ion Ratio Lower Upper
95 100
174 89.5 0.0 168.0
176 83.6 0.0 160.2


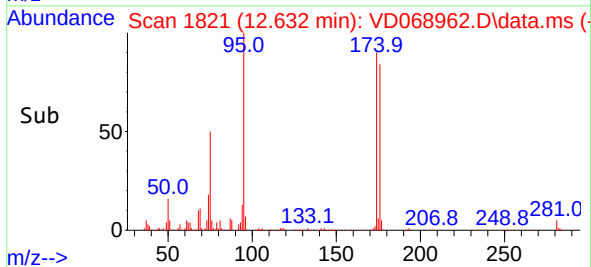
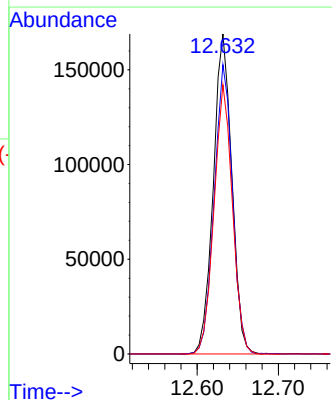
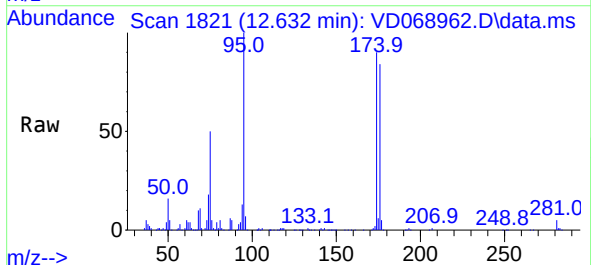


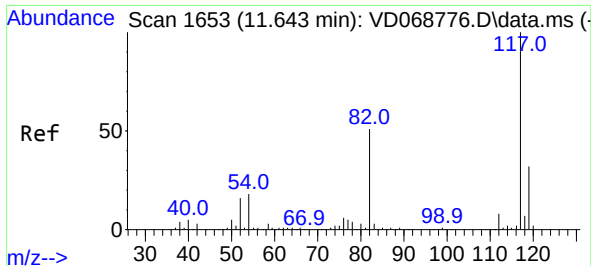

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.643 min Scan# 1653
Delta R.T. 0.000 min
Lab File: VD068962.D
Acq: 23 Apr 2021 12:44

Instrument :
MSVOA_D
ClientSampleId :
SB-33-0-2.0

Tgt Ion:117 Resp: 621439
Ion Ratio Lower Upper
117 100
82 51.7 43.5 65.3
119 32.7 26.7 40.1

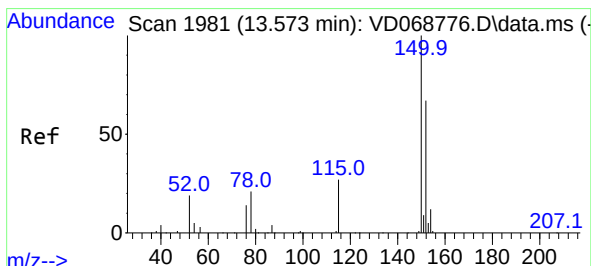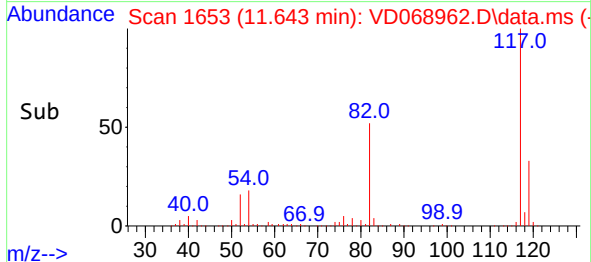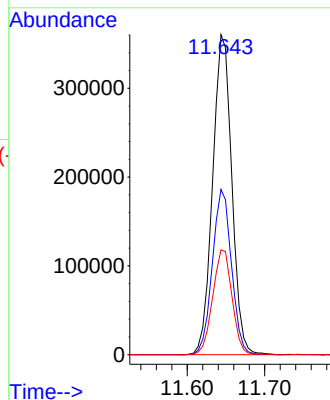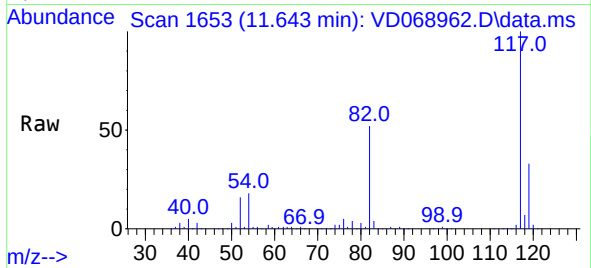

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.573 min Scan# 1981
Delta R.T. -0.000 min
Lab File: VD068962.D
Acq: 23 Apr 2021 12:44

Tgt Ion:152 Resp: 291542
Ion Ratio Lower Upper
152 100
115 55.7 29.3 87.8
150 158.0 0.0 347.6

