

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD042419\
 Data File : VD061995.D
 Acq On : 24 Apr 2019 13:57
 Operator : VA/AP
 Sample : K2522-07
 Misc : 6.25g/5ml/MSVOA D/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 SP-WOODBURY

Quant Time: Apr 26 11:04:27 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D042319S.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 23 14:52:55 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.05	168	23812	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.23	114	52073	50.00	ug/l	0.00
63) Chlorobenzene-d5	12.37	117	55465	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	14.52	152	23188	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.47	65	23352	125.30	ug/l	0.00
Spiked Amount	50.000		Recovery	=	250.60%	
35) Dibromofluoromethane	6.93	113	25575	71.02	ug/l	0.00
Spiked Amount	50.000		Recovery	=	142.04%	
50) Toluene-d8	10.42	98	44146	51.52	ug/l	0.00
Spiked Amount	50.000		Recovery	=	103.04%	
62) 4-Bromofluorobenzene	13.56	95	21540	62.67	ug/l	0.00
Spiked Amount	50.000		Recovery	=	125.34%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD042419\
Data File : VD061995.D
Acq On : 24 Apr 2019 13:57
Operator : VA/AP
Sample : K2522-07
Misc : 6.25g/5ml/MSVOA D/SOIL
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
SP-WOODBURY

Quant Time: Apr 26 11:04:27 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D042319S.M
Quant Title : SW846 8260
QLast Update : Tue Apr 23 14:52:55 2019
Response via : Initial Calibration

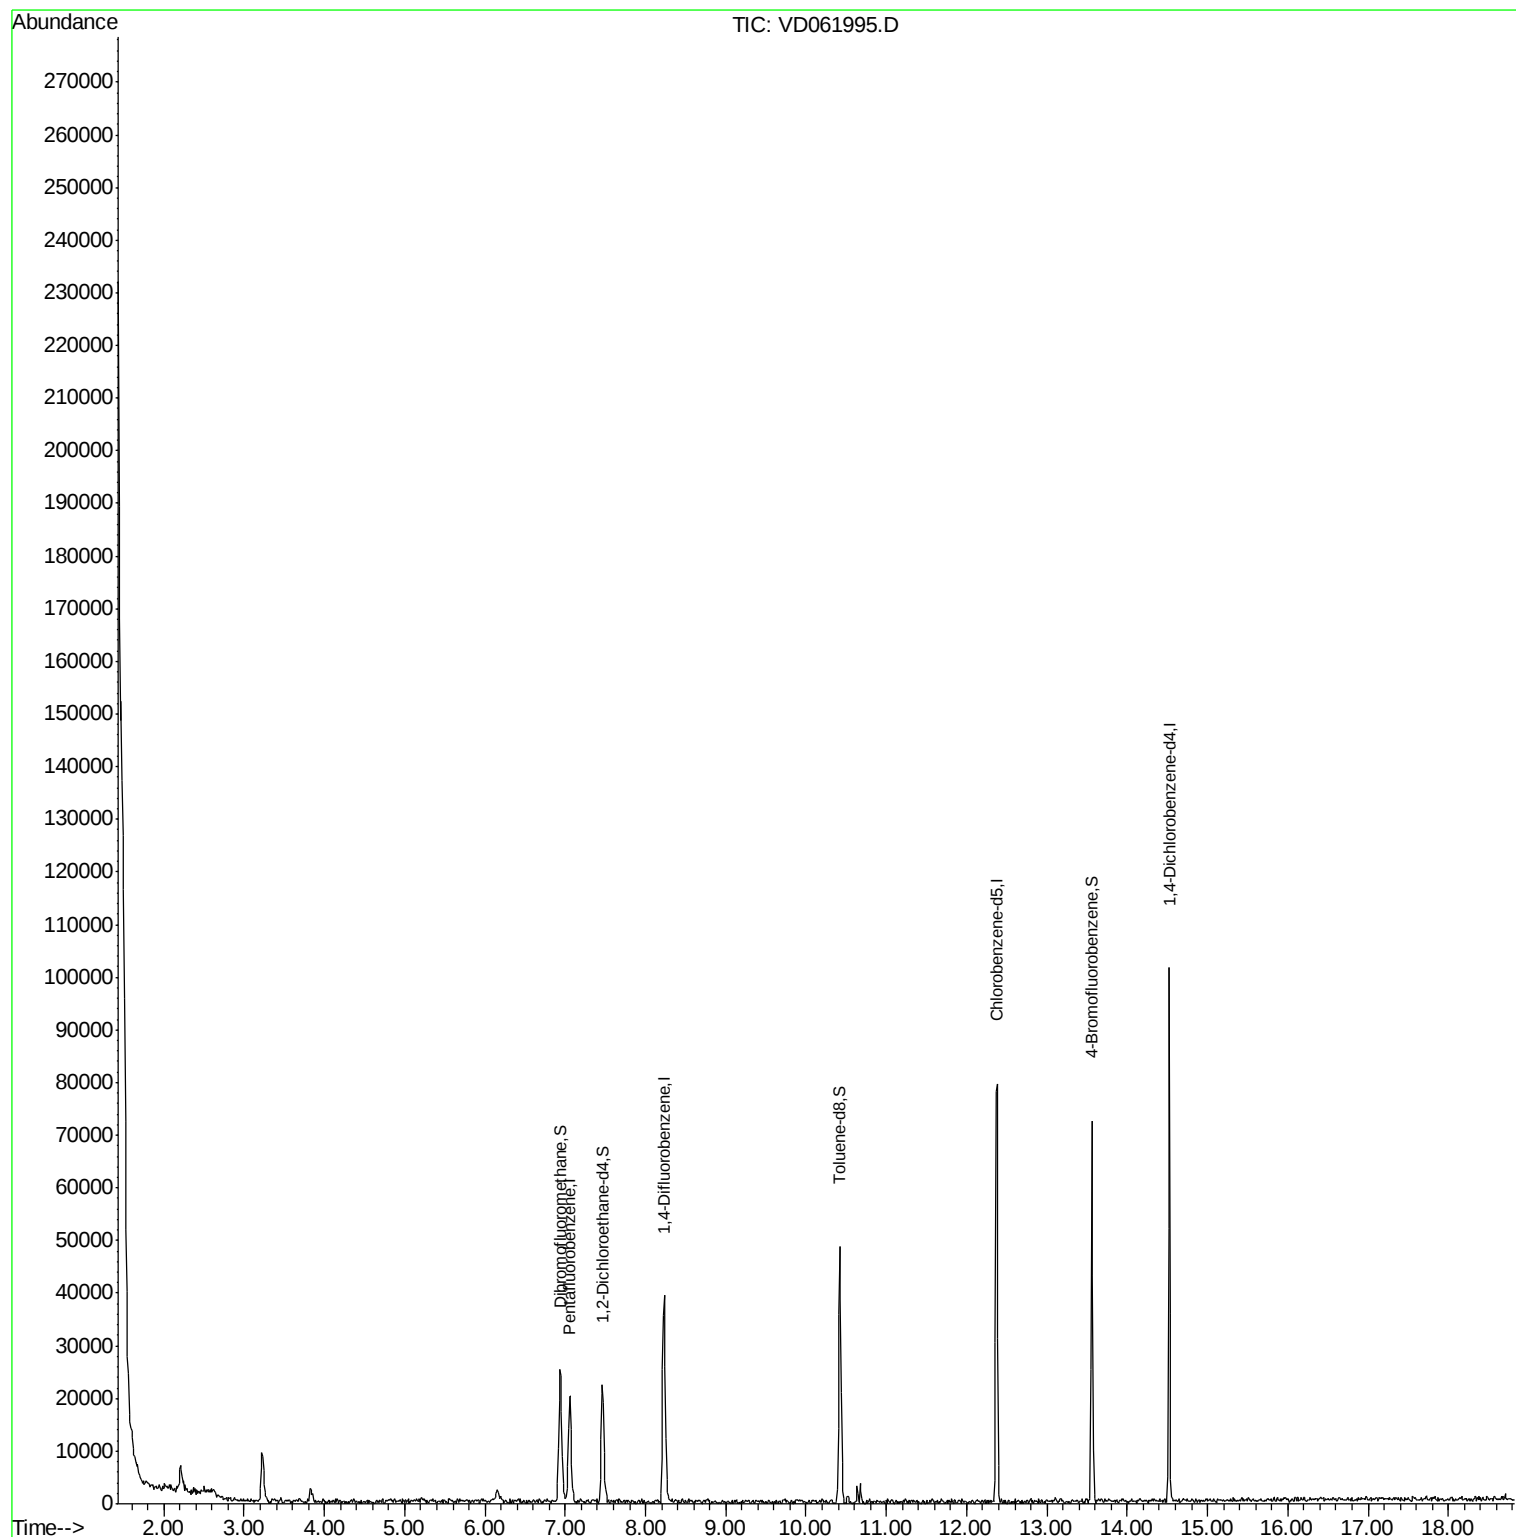

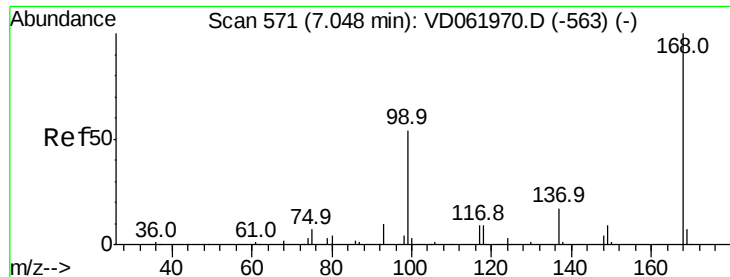

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.05 min Scan# 572

Delta R.T. -0.00 min

Lab File: VD061995.D

Acq: 24 Apr 2019 13:57

Instrument :

MSVOA_D

ClientSampleId :


SP-WOODBURY

Tot Ion:168 Resp: 23812

Ion Ratio Lower Upper




168 100

99 52.4 46.5 69.7

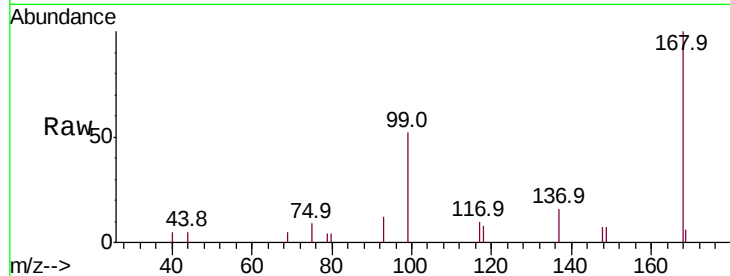

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.95 (98.65 to 99.65): VDC

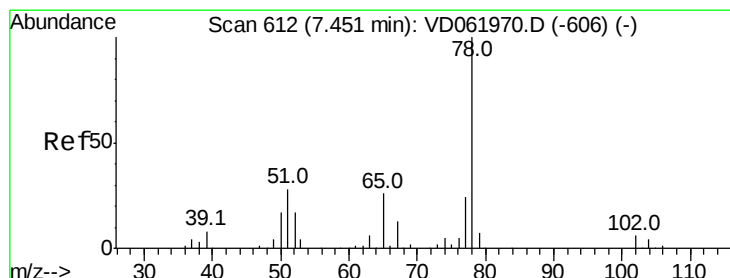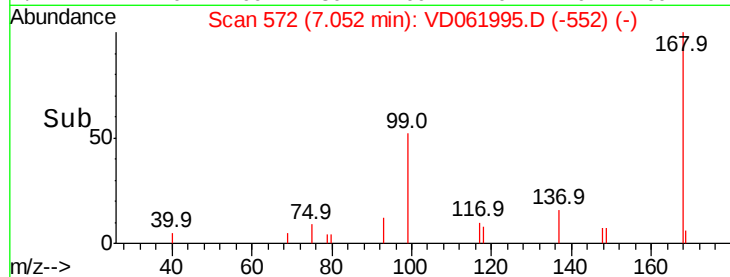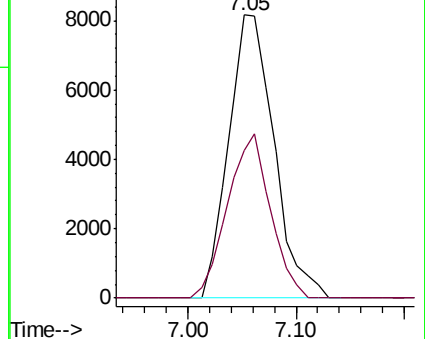

#33

1,2-Dichloroethane-d4

Concen: 125.302 ug/l

RT: 7.47 min Scan# 614

Delta R.T. 0.01 min

Lab File: VD061995.D


Acq: 24 Apr 2019 13:57

Tgt Ion: 65 Resp: 23352

Ion Ratio Lower Upper



65 100


67 57.5 0.0 98.0

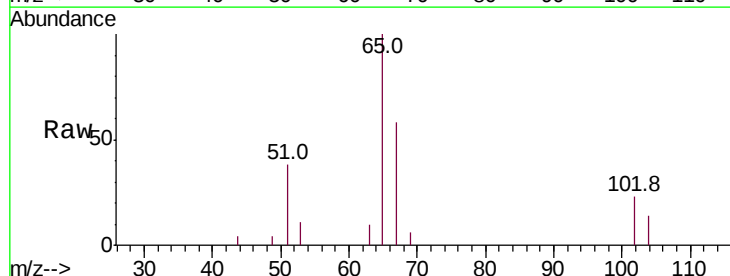

Abundance Ion 64.95 (64.65 to 65.65): VDC

Ion 66.90 (66.60 to 67.60): VDC

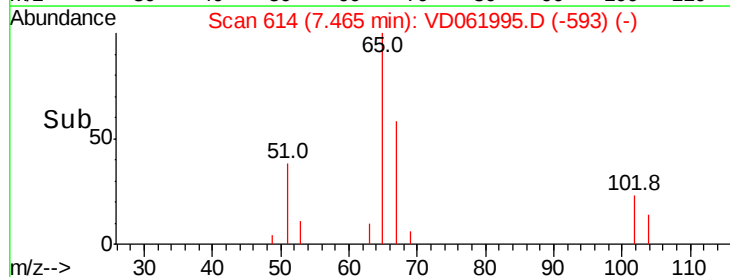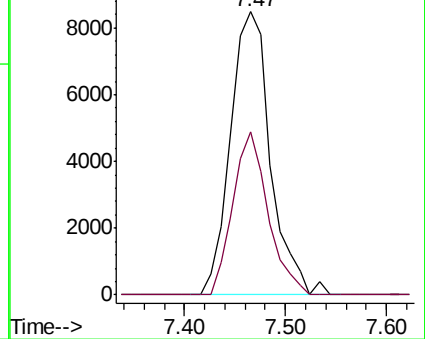


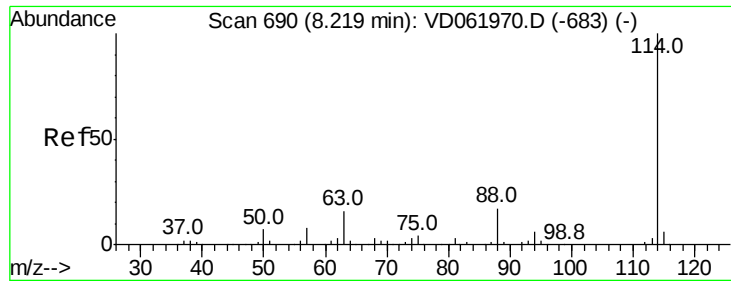




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.23 min Scan# 692
 Delta R.T. 0.01 min
 Lab File: VD061995.D
 Acq: 24 Apr 2019 13:57

Instrument :
 MSVOA_D
 ClientSampleId :
 SP-WOODBURY

Tot Ion:114 Resp: 52073
 Ion Ratio Lower Upper
 114 100
 63 17.1 0.0 32.4
 88 19.9 0.0 33.6

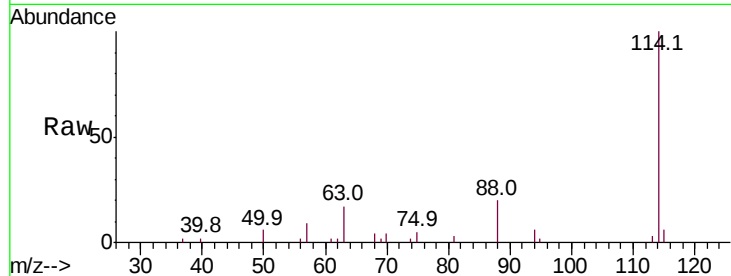


Abundance Ion 114.00 (113.70 to 114.70): V
 Ion 62.95 (62.65 to 63.65): V
 Ion 87.90 (87.60 to 88.60): V

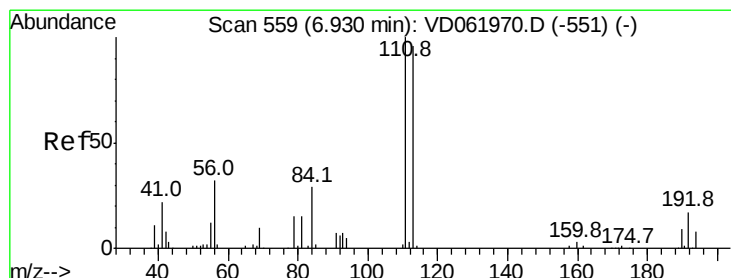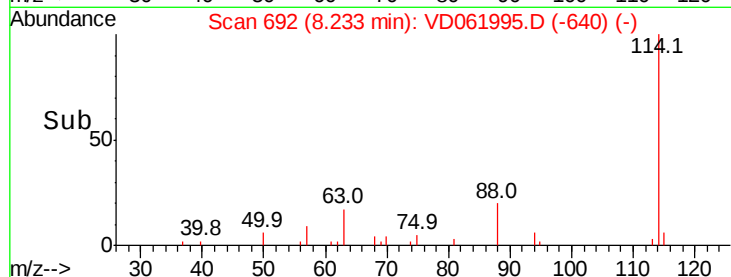
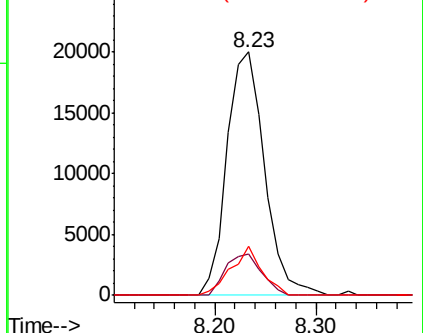



#35
 Dibromofluoromethane
 Concen: 71.015 ug/l
 RT: 6.93 min Scan# 560
 Delta R.T. -0.00 min
 Lab File: VD061995.D
 Acq: 24 Apr 2019 13:57

Tgt Ion:113 Resp: 25575
 Ion Ratio Lower Upper
 113 100
 111 93.8 78.5 117.7
 192 17.9 13.0 19.4

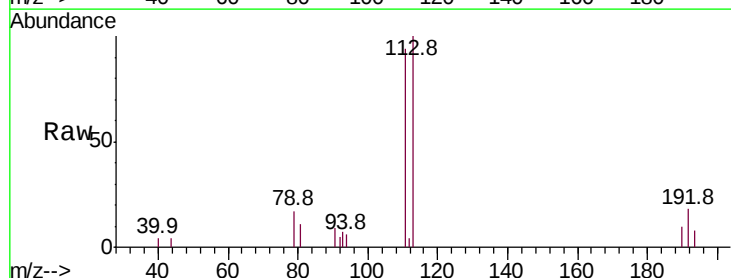

Abundance Ion 112.90 (112.60 to 113.60): V
 Ion 110.90 (110.60 to 111.60): V
 Ion 191.80 (191.50 to 192.50): V

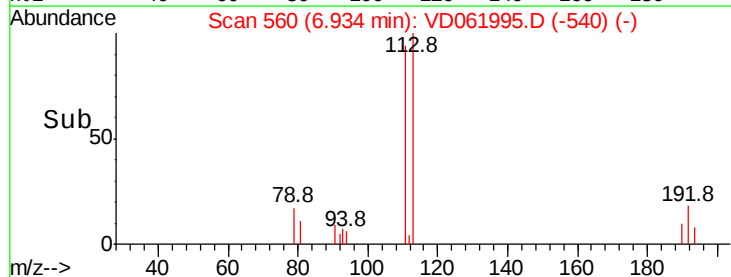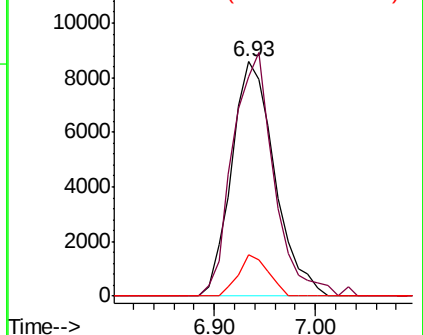

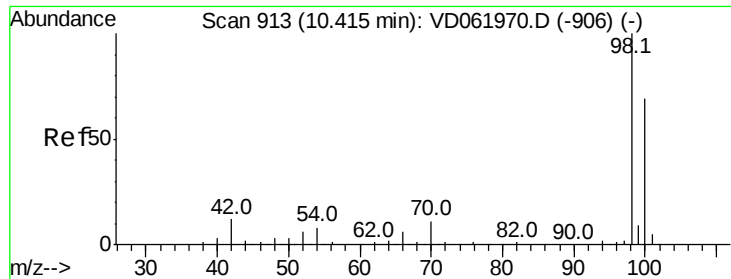

#50

Toluene-d8

Concen: 51.516 ug/l

RT: 10.42 min Scan# 914

Delta R.T. -0.00 min

Lab File: VD061995.D

Acq: 24 Apr 2019 13:57

Instrument :

MSVOA_D

ClientSampleId :


SP-WOODBURY

Tot Ion: 98 Resp: 44146

Ion Ratio Lower Upper

98 100

100 71.0 53.8 80.8

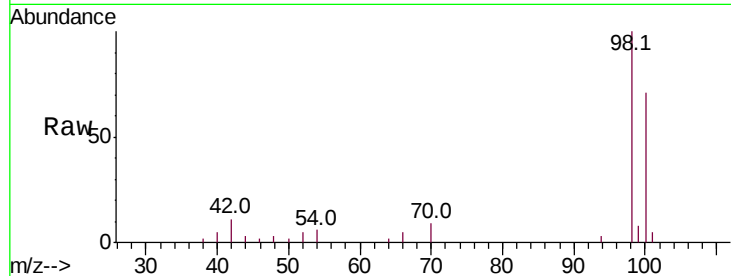

Abundance Ion 98.05 (97.75 to 98.75): VD061970.D (-906) (-)

Ion 100.05 (99.75 to 100.75): VD061970.D (-906) (-)

10.42

20000



15000

10000

5000

0

Time--> 10.30 10.40 10.50

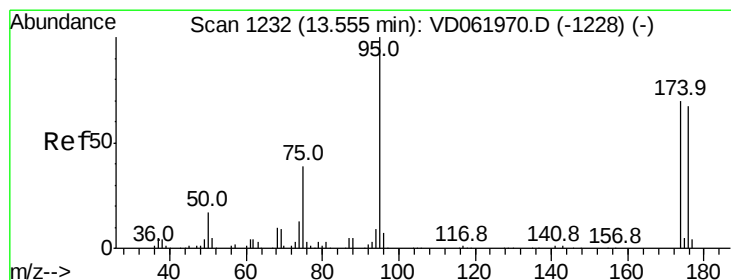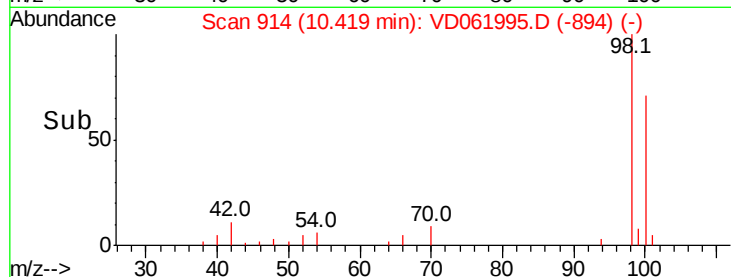

#62

4-Bromofluorobenzene

Concen: 62.669 ug/l

RT: 13.56 min Scan# 1233

Delta R.T. -0.00 min

Lab File: VD061995.D

Acq: 24 Apr 2019 13:57


Tgt Ion: 95 Resp: 21540

Ion Ratio Lower Upper

95 100

174 72.6 0.0 181.8

176 70.6 0.0 174.4

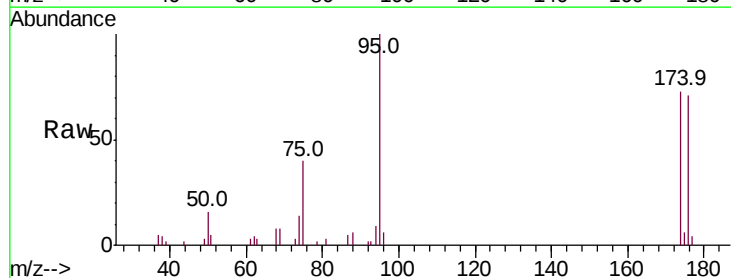

Abundance Ion 95.00 (94.70 to 95.70): VD061970.D (-1228) (-)

Ion 173.90 (173.60 to 174.60): VD061970.D (-1228) (-)

Ion 175.90 (175.60 to 176.60): VD061970.D (-1228) (-)

25000

20000


15000


10000

5000

0

Time--> 13.50 13.55 13.60




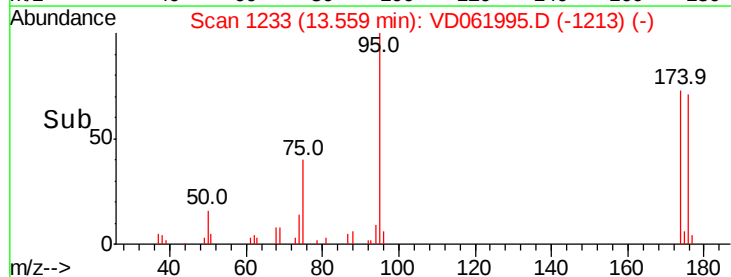


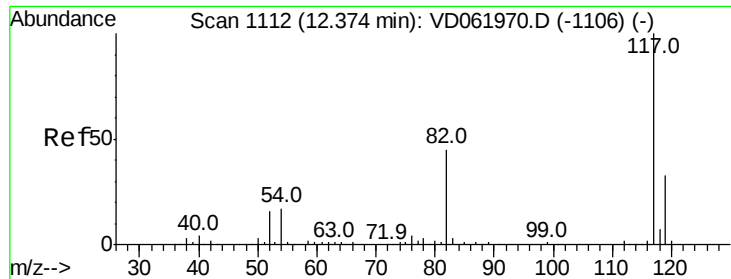

#63
 Chlorobenzene-d5
 Concen: 50.000 ug/l
 RT: 12.37 min Scan# 1112
 Delta R.T. -0.00 min
 Lab File: VD061995.D
 Acq: 24 Apr 2019 13:57

Instrument :
 MSVOA_D
 ClientSampleId :
 SP-WOODBURY

Tot Ion:117 Resp: 55465
 Ion Ratio Lower Upper
 117 100
 82 44.0 36.2 54.2
 119 26.4 26.2 39.4

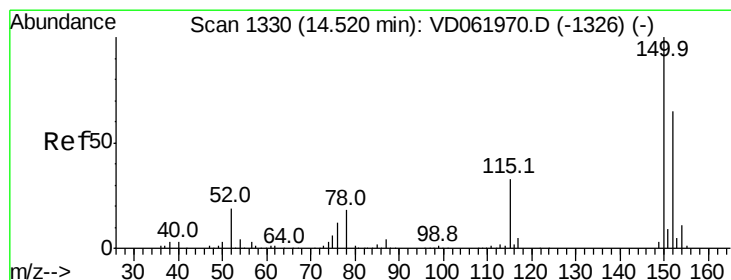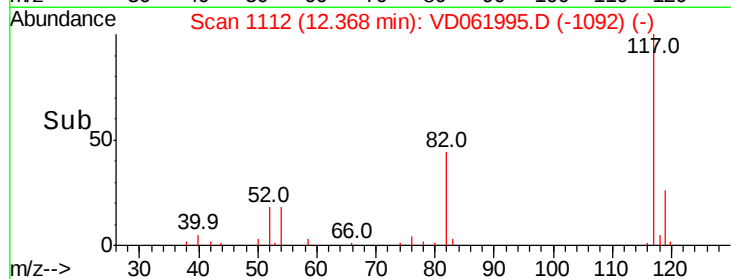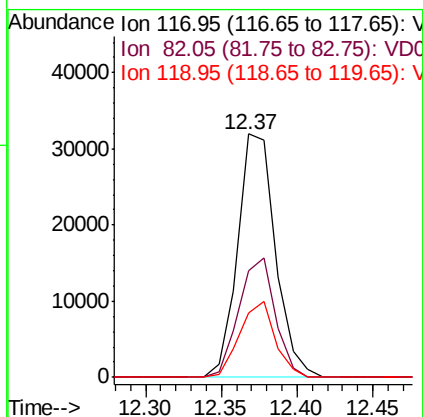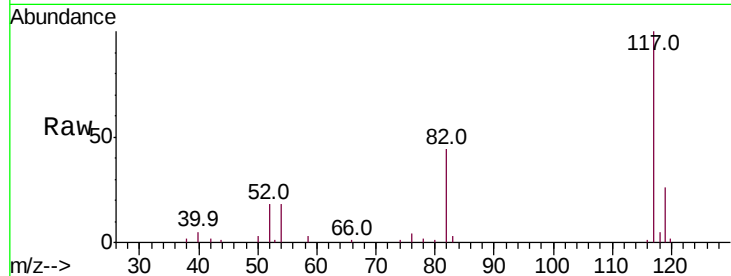

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 14.52 min Scan# 1331
 Delta R.T. -0.00 min
 Lab File: VD061995.D
 Acq: 24 Apr 2019 13:57

Tgt Ion:152 Resp: 23188
 Ion Ratio Lower Upper
 152 100
 115 47.6 30.9 92.7
 150 155.4 0.0 314.8

