

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD042419\
 Data File : VD062000.D
 Acq On : 24 Apr 2019 16:22
 Operator : VA/AP
 Sample : K2526-01
 Misc : 6.17g/5ml/MSVOA D/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 SOIL-ROLLOFFS

Quant Time: Apr 25 01:34:50 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D042319S.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 23 14:52:55 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	0.00	168	0	0.00	ug/l	-7.05
34) 1,4-Difluorobenzene	0.00	114	0	0.00	ug/l	-8.22
63) Chlorobenzene-d5	0.00	117	0	0.00	ug/l	-12.37
72) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ug/l	-14.52
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	0.00	65	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
35) Dibromofluoromethane	0.00	113	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
50) Toluene-d8	0.00	98	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
62) 4-Bromofluorobenzene	0.00	95	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD042419\
Data File : VD062000.D
Acq On : 24 Apr 2019 16:22
Operator : VA/AP
Sample : K2526-01
Misc : 6.17g/5ml/MSVOA D/SOIL
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
SOIL-ROLLOFFS

Quant Time: Apr 25 01:34:50 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D042319S.M
Quant Title : SW846 8260
QLast Update : Tue Apr 23 14:52:55 2019
Response via : Initial Calibration

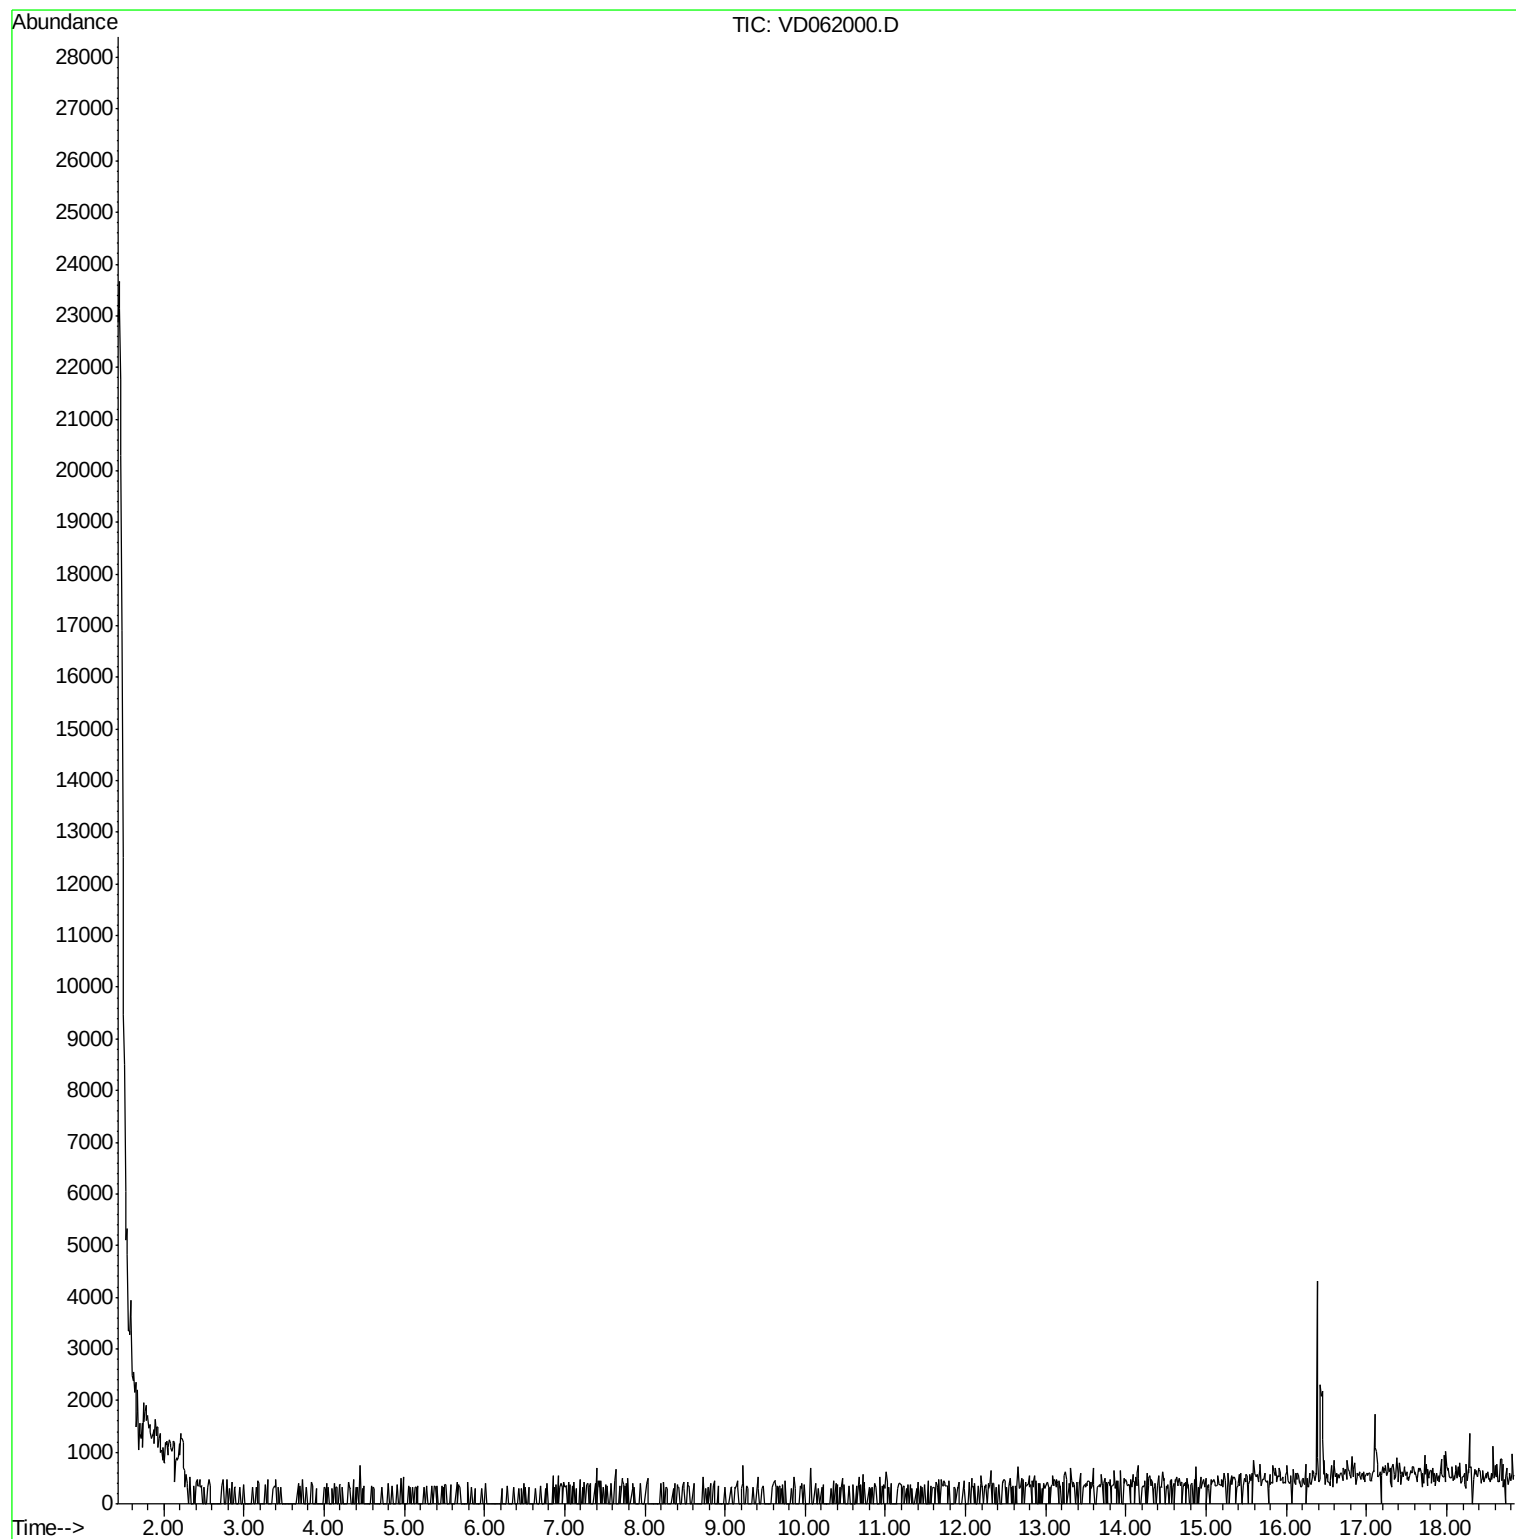

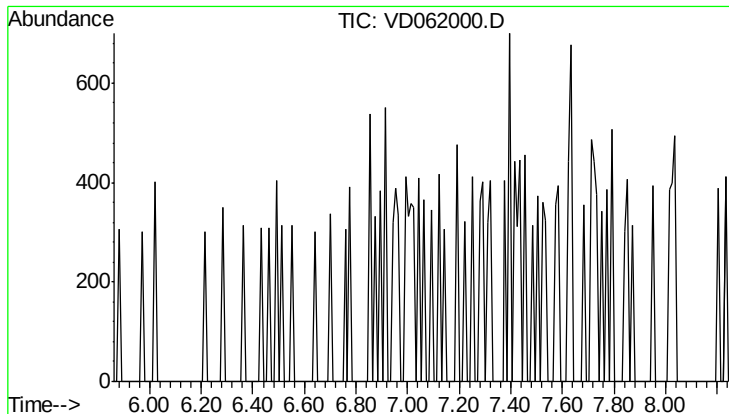

#1

Pentafluorobenzene

Concen: 0.000 ug/l

Expected RT: 7.05 min

Lab File: VD062000.D

Acq: 24 Apr 2019 16:22

Tot Ion: 168

Sig Exp Ratio

168 100



99 58.1

Instrument :

MSVOA_D

ClientSampleId :

SOIL-ROLLOFFS

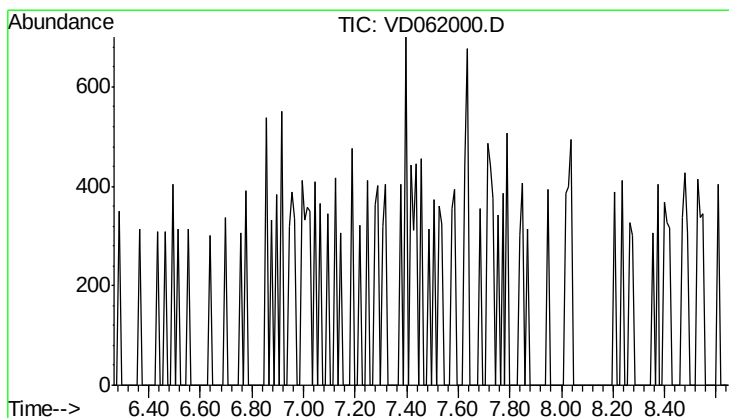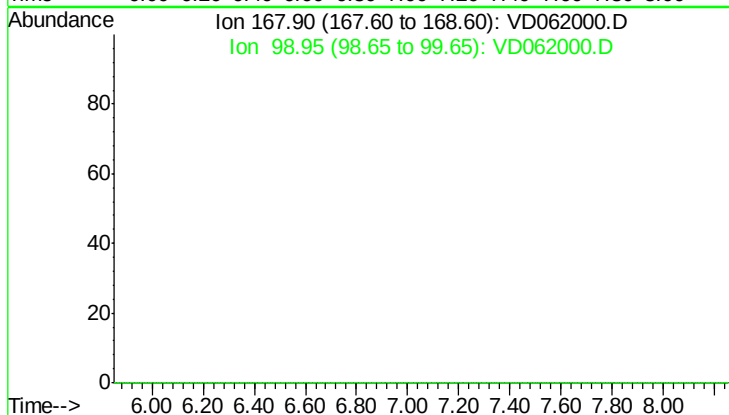

#33

1,2-Dichloroethane-d4

Concen: 0.000 ug/l

Expected RT: 7.46 min

Lab File: VD062000.D


Acq: 24 Apr 2019 16:22


Tgt Ion: 65

Sig Exp Ratio

65 100

67 49.0


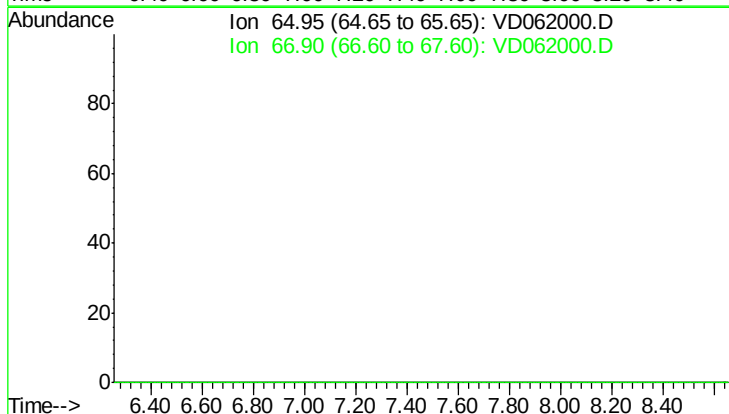


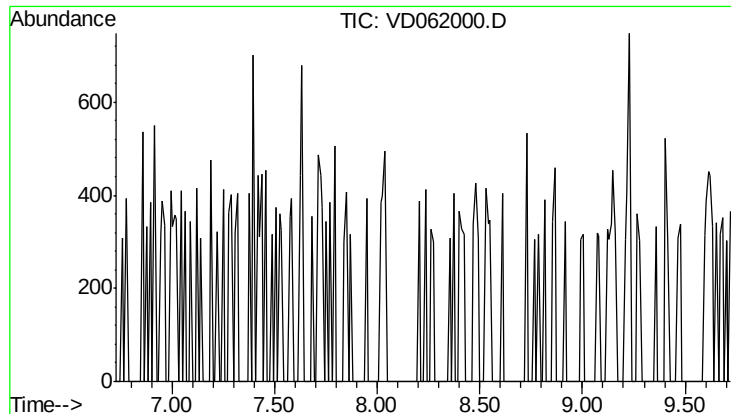

#34
 1,4-Difluorobenzene
 Concen: 0.000 ug/l
 Expected RT: 8.22 min
 Lab File: VD062000.D
 Acq: 24 Apr 2019 16:22


Instrument :
 MSVOA_D
 ClientSampleId :
 SOIL-ROLLOFFS


Tot Ion	114
Sig	Exp Ratio
114	100
63	16.2
88	16.8

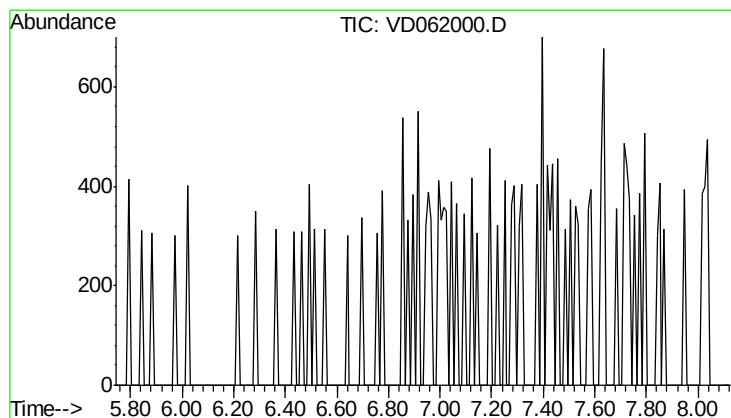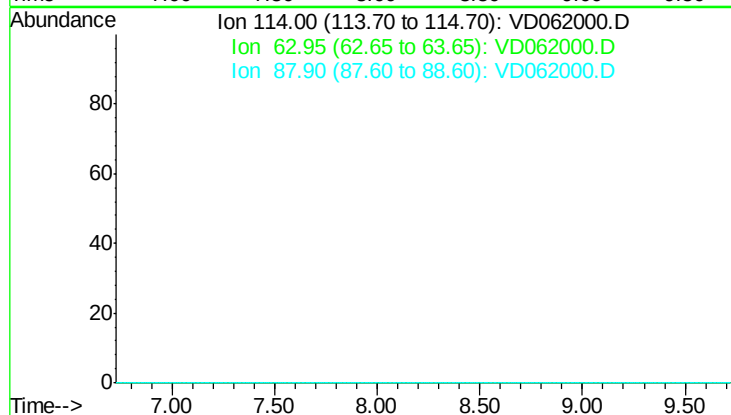

#35
 Dibromofluoromethane
 Concen: 0.000 ug/l
 Expected RT: 6.93 min
 Lab File: VD062000.D
 Acq: 24 Apr 2019 16:22

Tgt Ion	113
Sig	Exp Ratio
113	100
111	98.1
192	16.2

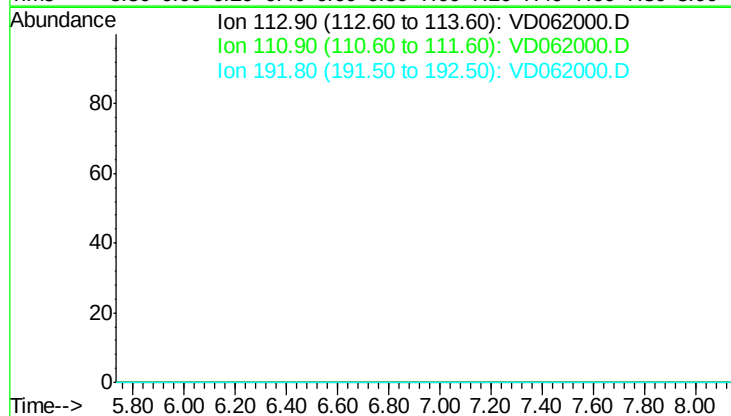


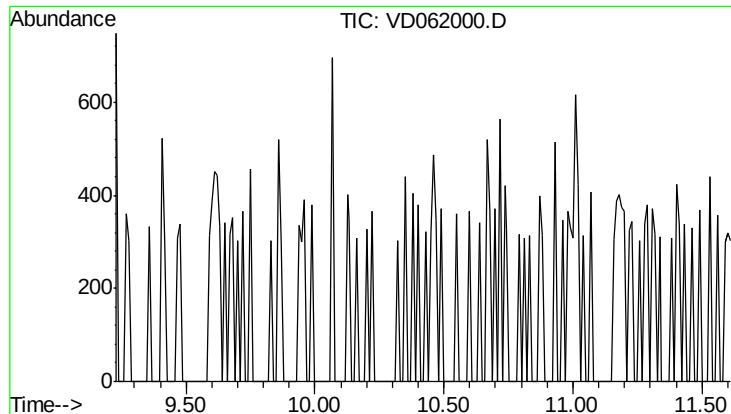


#50
Toluene-d8
Concen: 0.000 ug/l
Expected RT: 10.42 min

Lab File: VD062000.D
Acq: 24 Apr 2019 16:22

Instrument :
MSVOA_D
ClientSampleId :
SOIL-ROLLOFFS


Tot Ion	98
Sig	Exp Ratio
98	100
100	67.3

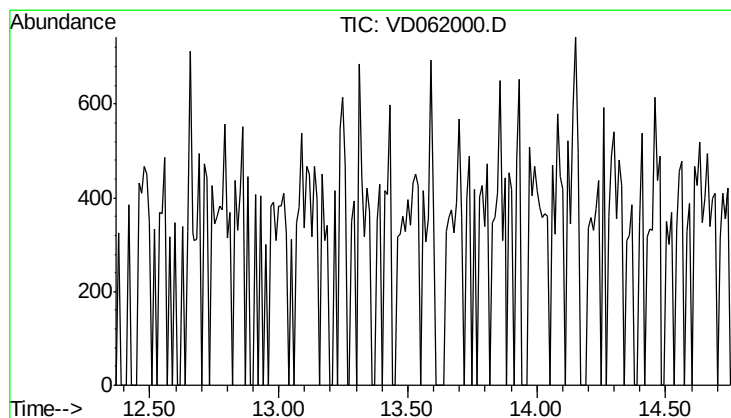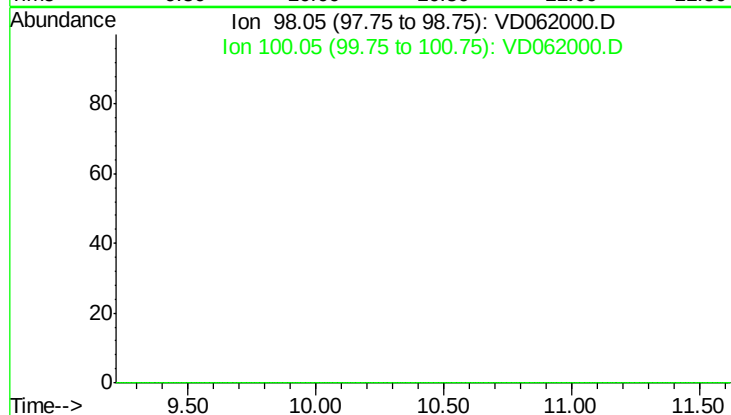


#62
4-Bromofluorobenzene
Concen: 0.000 ug/l
Expected RT: 13.56 min

Lab File: VD062000.D
Acq: 24 Apr 2019 16:22

Tgt Ion	95
Sig	Exp Ratio
95	100
174	90.9
176	87.2

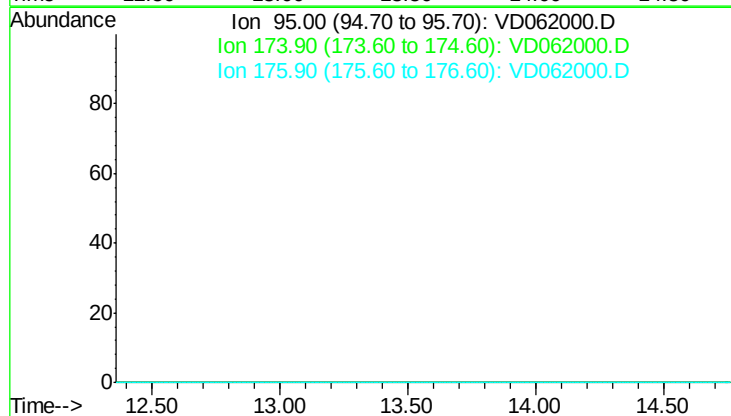


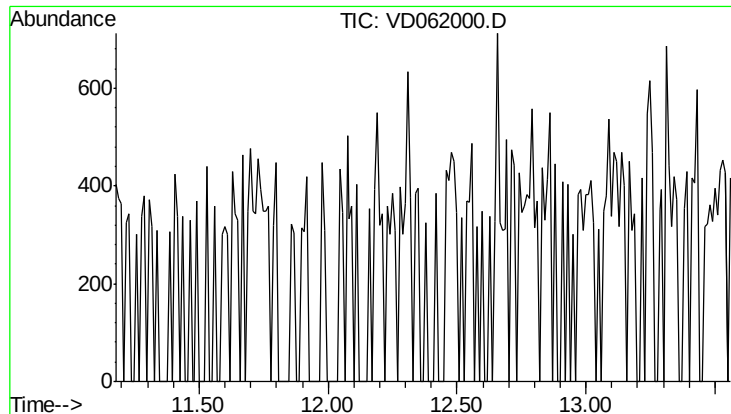


#63
 Chlorobenzene-d5
 Concen: 0.000 ug/l
 Expected RT: 12.37 min

Lab File: VD062000.D
 Acq: 24 Apr 2019 16:22

Instrument :
 MSVOA_D
 ClientSampleId :
 SOIL-ROLLOFFS

Tot Ion	117
Sig	Exp Ratio
117	100
82	45.2
119	32.8

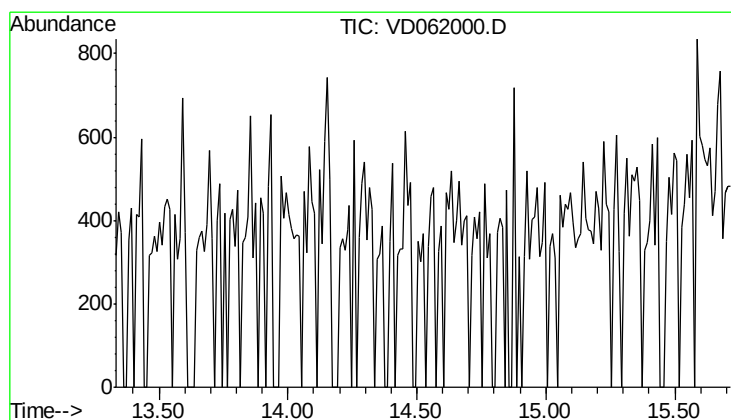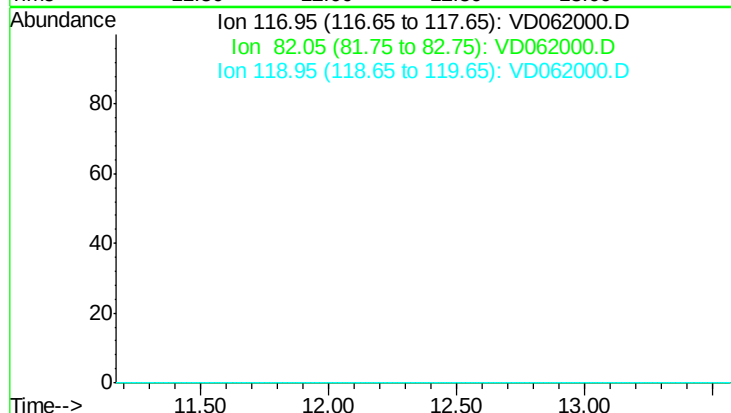

#72
 1,4-Dichlorobenzene-d4
 Concen: 0.000 ug/l
 Expected RT: 14.52 min

Lab File: VD062000.D
 Acq: 24 Apr 2019 16:22

Tgt Ion	152
Sig	Exp Ratio
152	100
115	61.8
150	157.4

