


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD042419\
Data File : VD061988.D
Acq On : 24 Apr 2019 10:07
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D042319S.M
Title : SW846 8260
Last Update : Tue Apr 23 14:52:55 2019

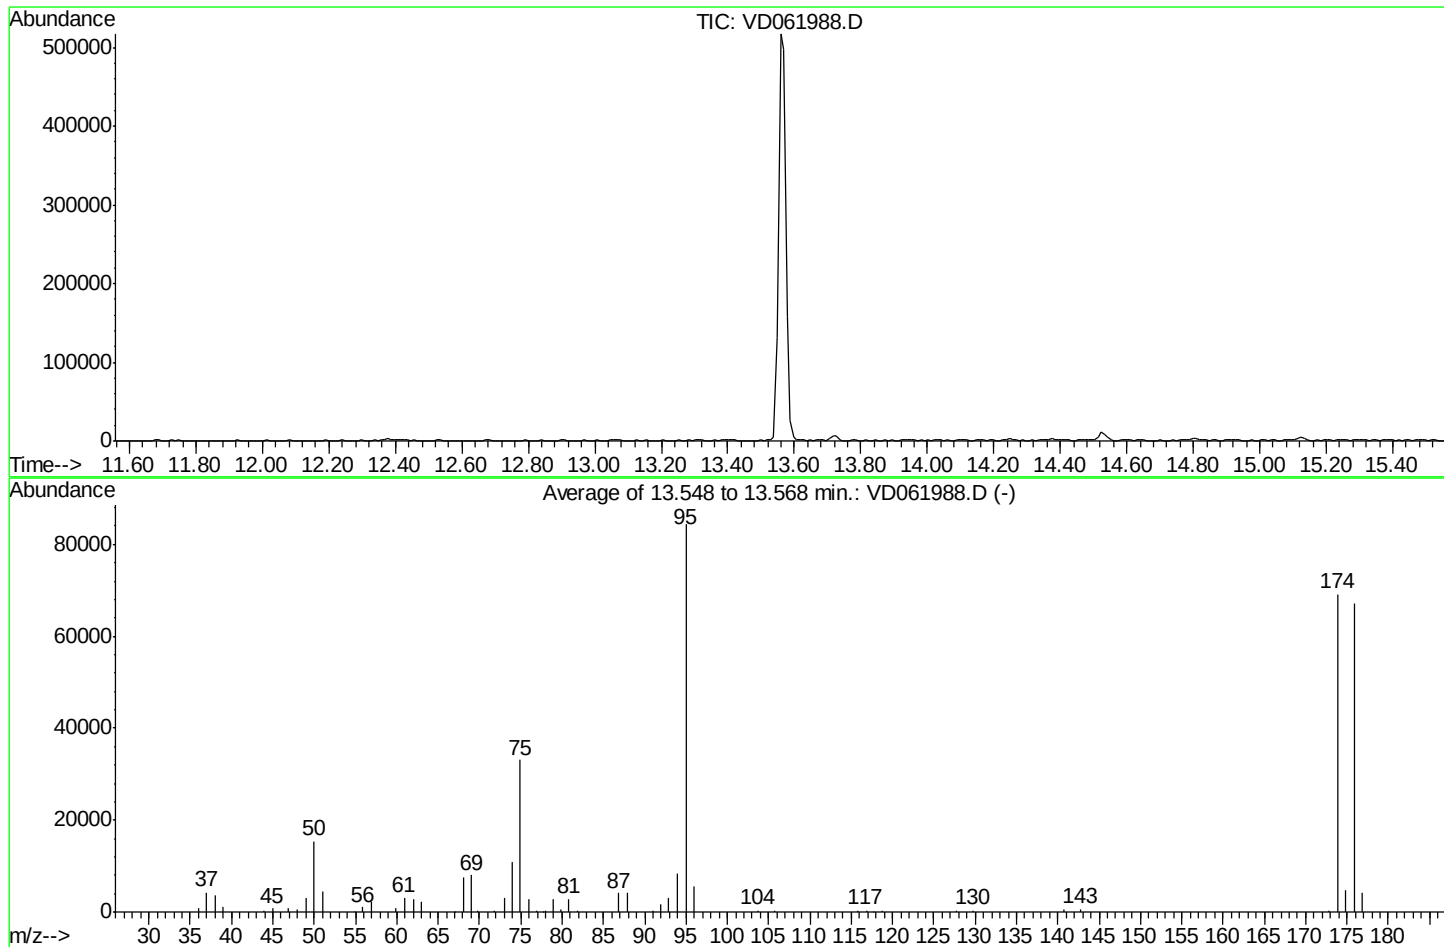

AutoFind: Scans 1232, 1233, 1234; Background Corrected with Scan 1228

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	15429	PASS
75	95	30	60	39.2	33072	PASS
95	95	100	100	100.0	84357	PASS
96	95	5	9	6.7	5650	PASS
173	174	0.00	2	0.3	204	PASS
174	95	50	100	82.0	69135	PASS
175	174	5	9	7.0	4842	PASS
176	174	95	101	97.1	67125	PASS
177	176	5	9	6.4	4287	PASS