


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD042419\
 Data File : VD062012.D
 Acq On : 24 Apr 2019 23:17
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µl/5ml/MSVOA D/SOIL
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D042319S.M
 Title : SW846 8260
 Last Update : Tue Apr 23 14:52:55 2019

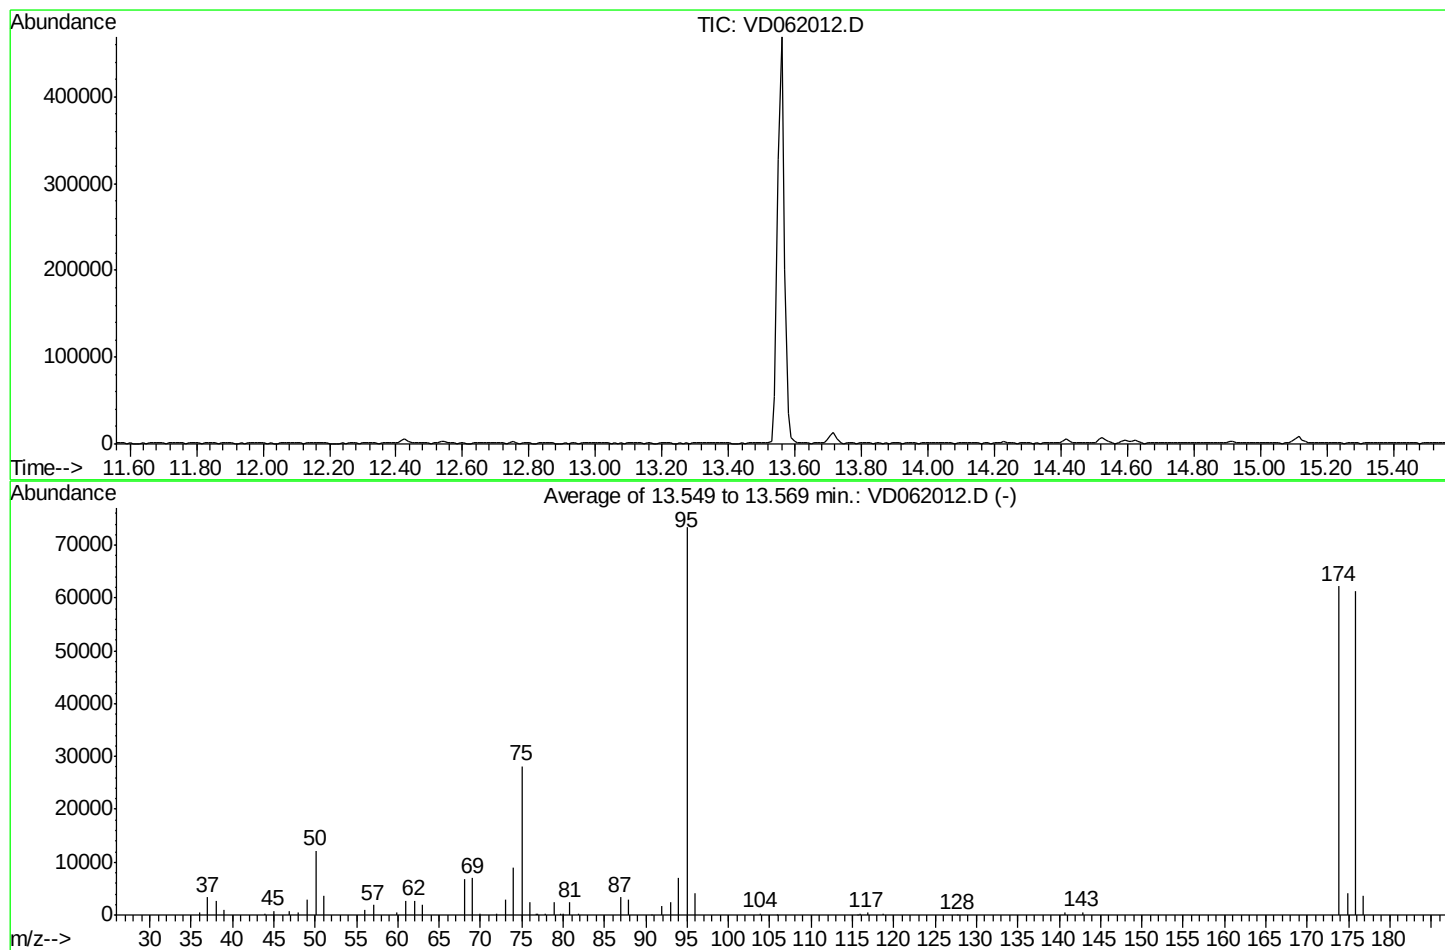

AutoFind: Scans 1232, 1233, 1234; Background Corrected with Scan 1227

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	12169	PASS
75	95	30	60	38.3	28121	PASS
95	95	100	100	100.0	73389	PASS
96	95	5	9	5.8	4250	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	84.7	62184	PASS
175	174	5	9	6.8	4206	PASS
176	174	95	101	98.7	61376	PASS
177	176	5	9	6.1	3720	PASS