




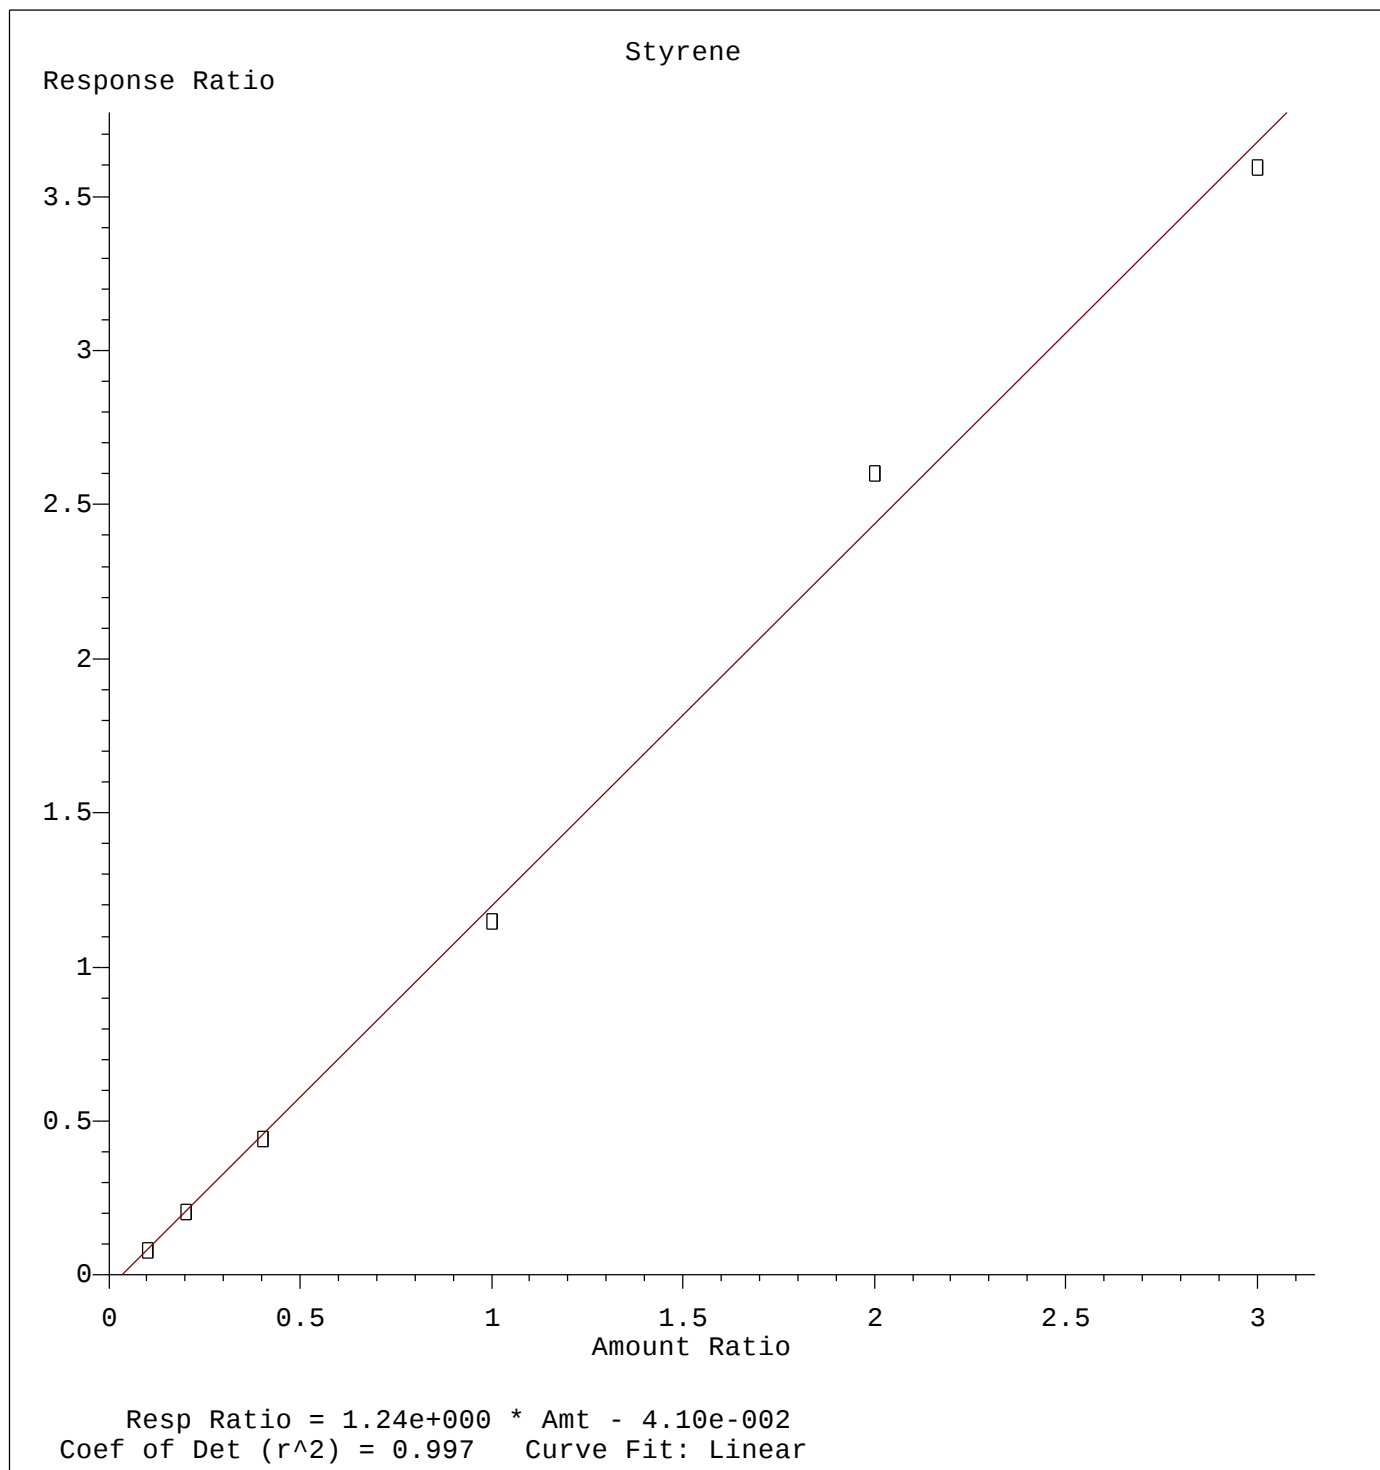


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D042420S.M
Calibration Table Last Updated: Fri Apr 24 14:44:29 2020

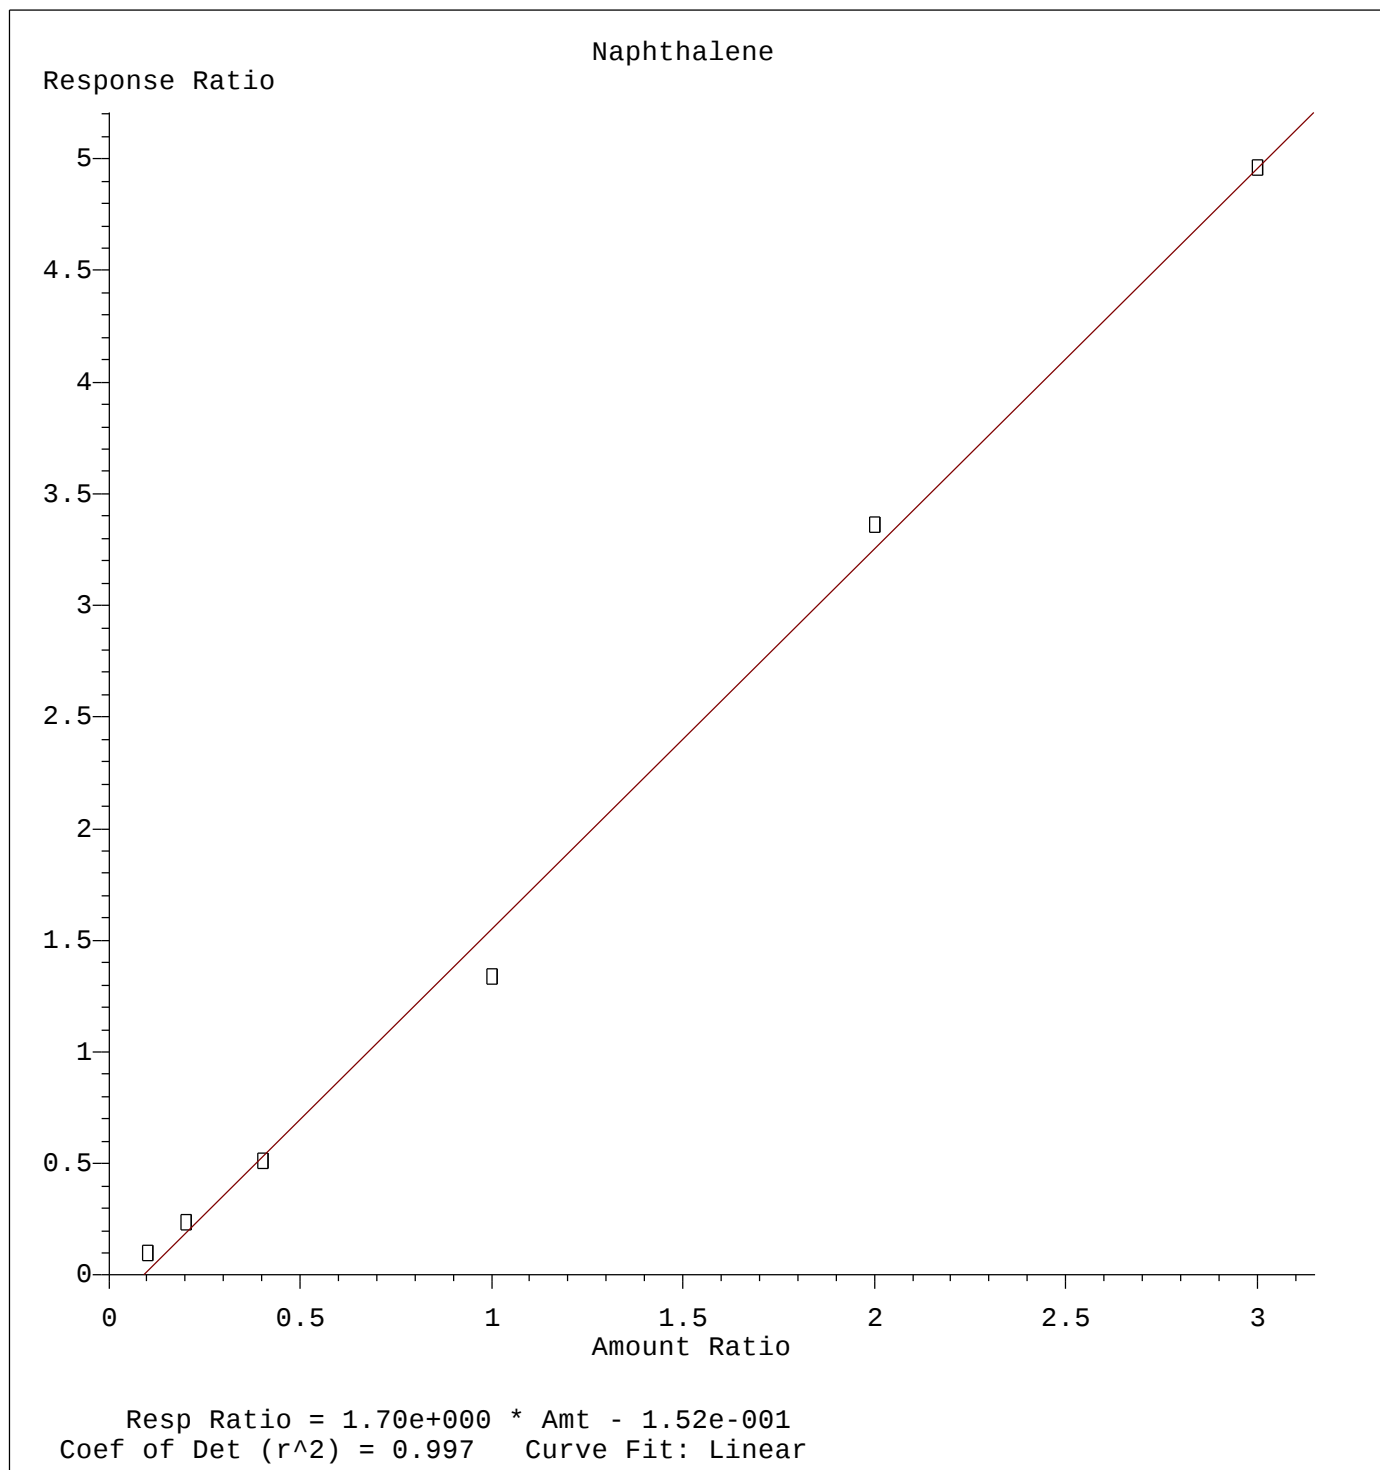


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D042420S.M
Calibration Table Last Updated: Fri Apr 24 14:44:29 2020

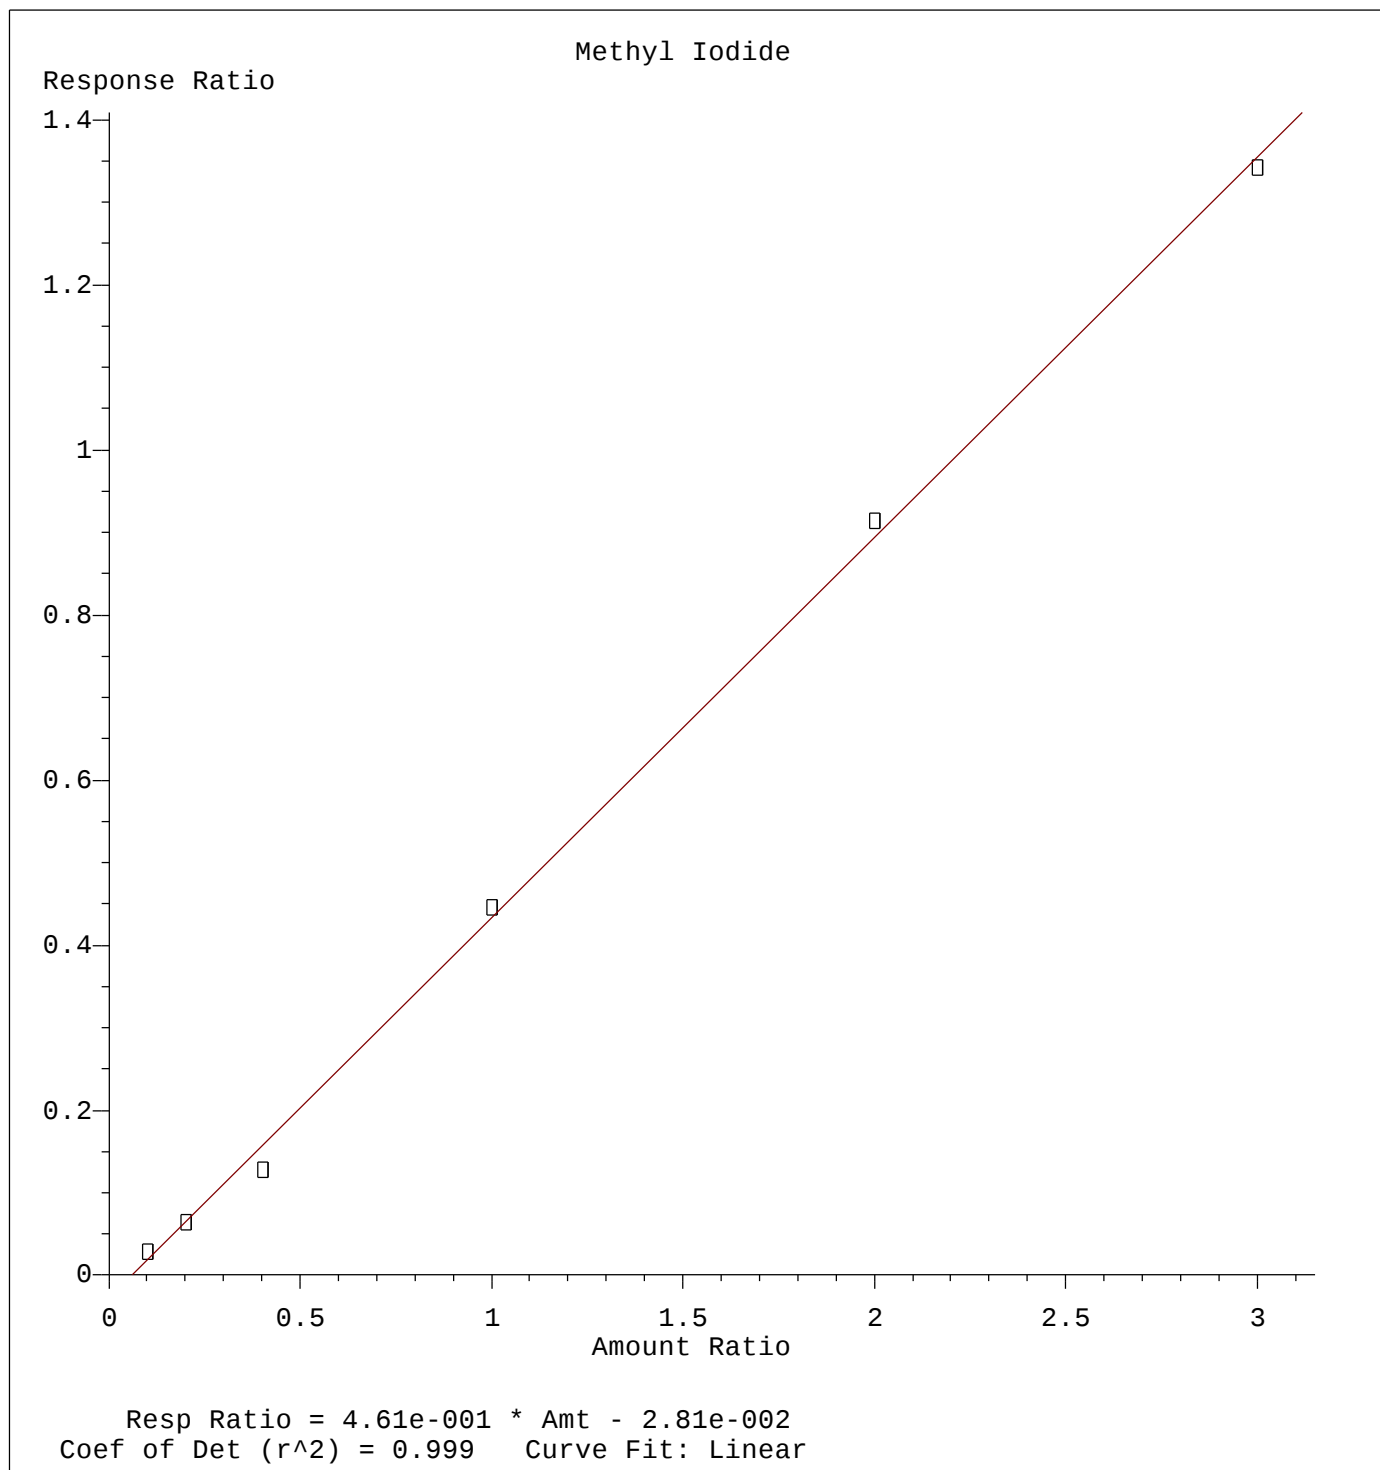


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D042420S.M
Calibration Table Last Updated: Fri Apr 24 14:44:29 2020

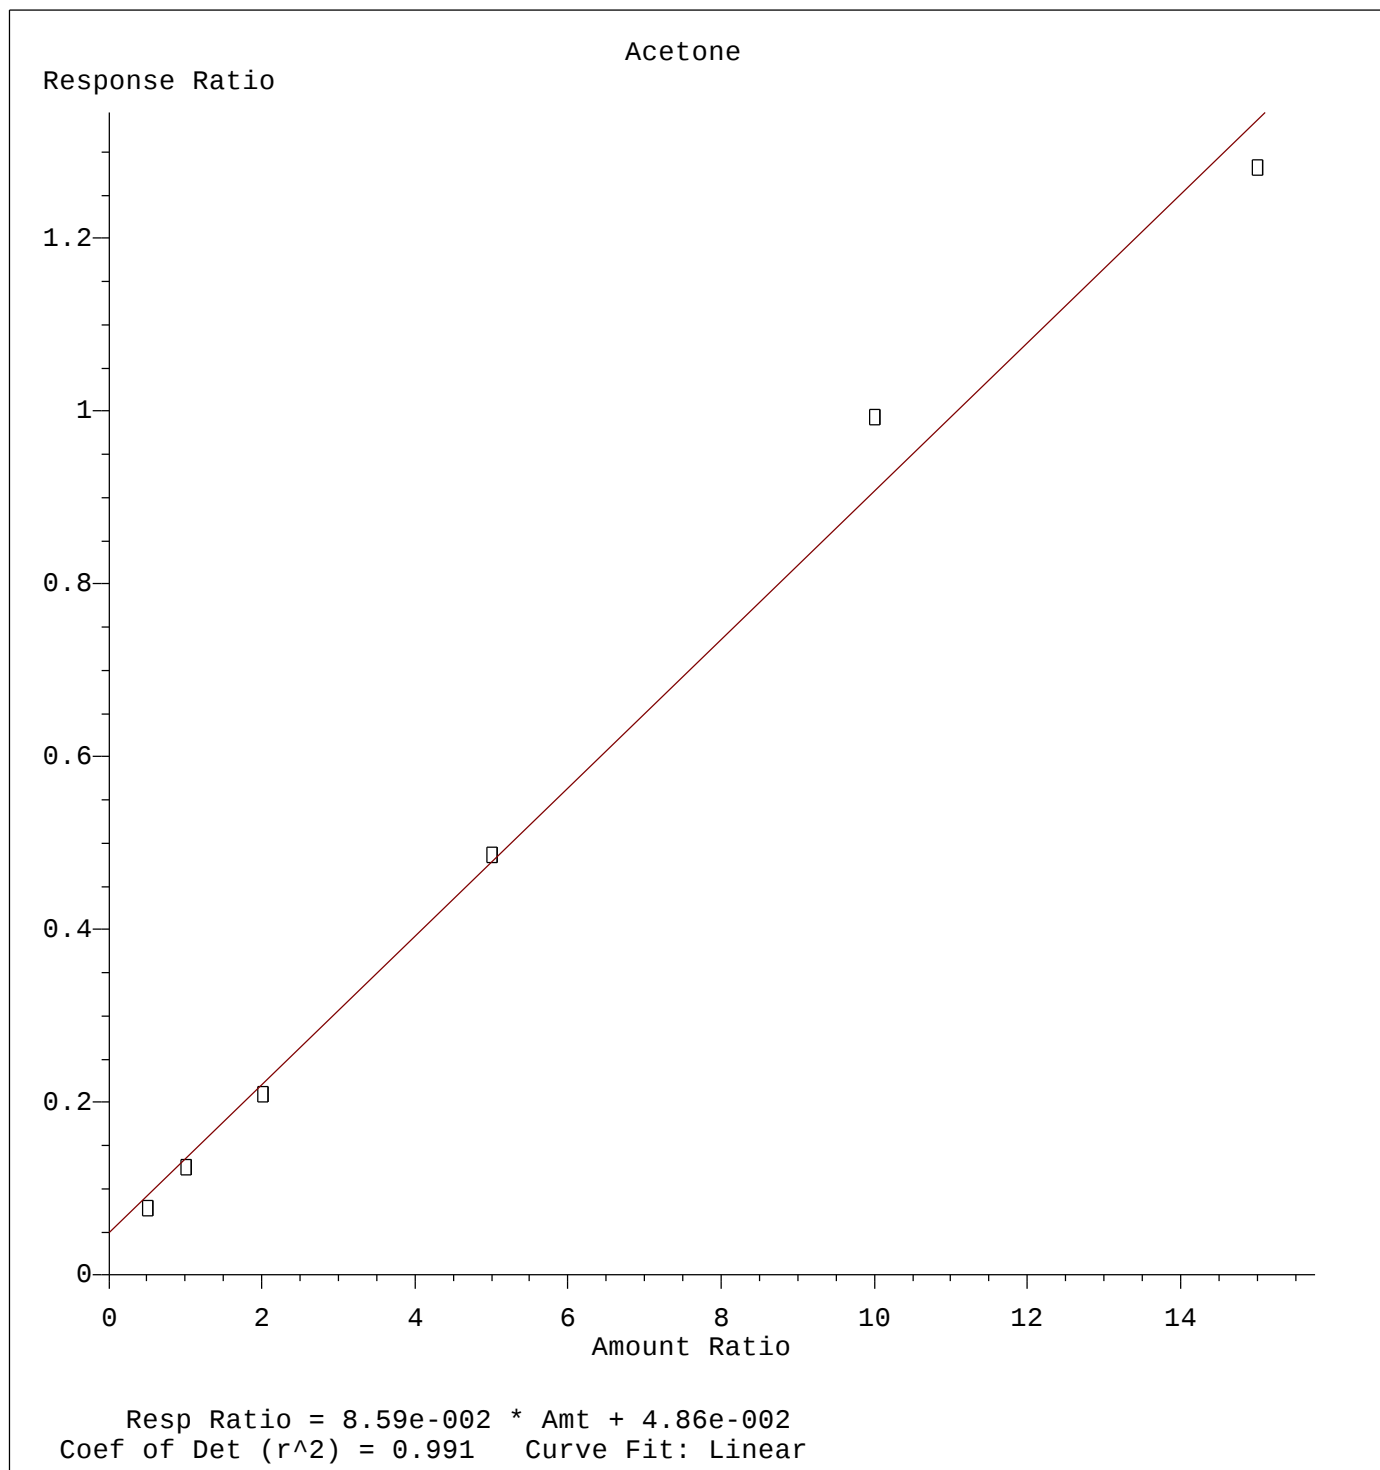

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D042420S.M
Calibration Table Last Updated: Fri Apr 24 14:44:29 2020

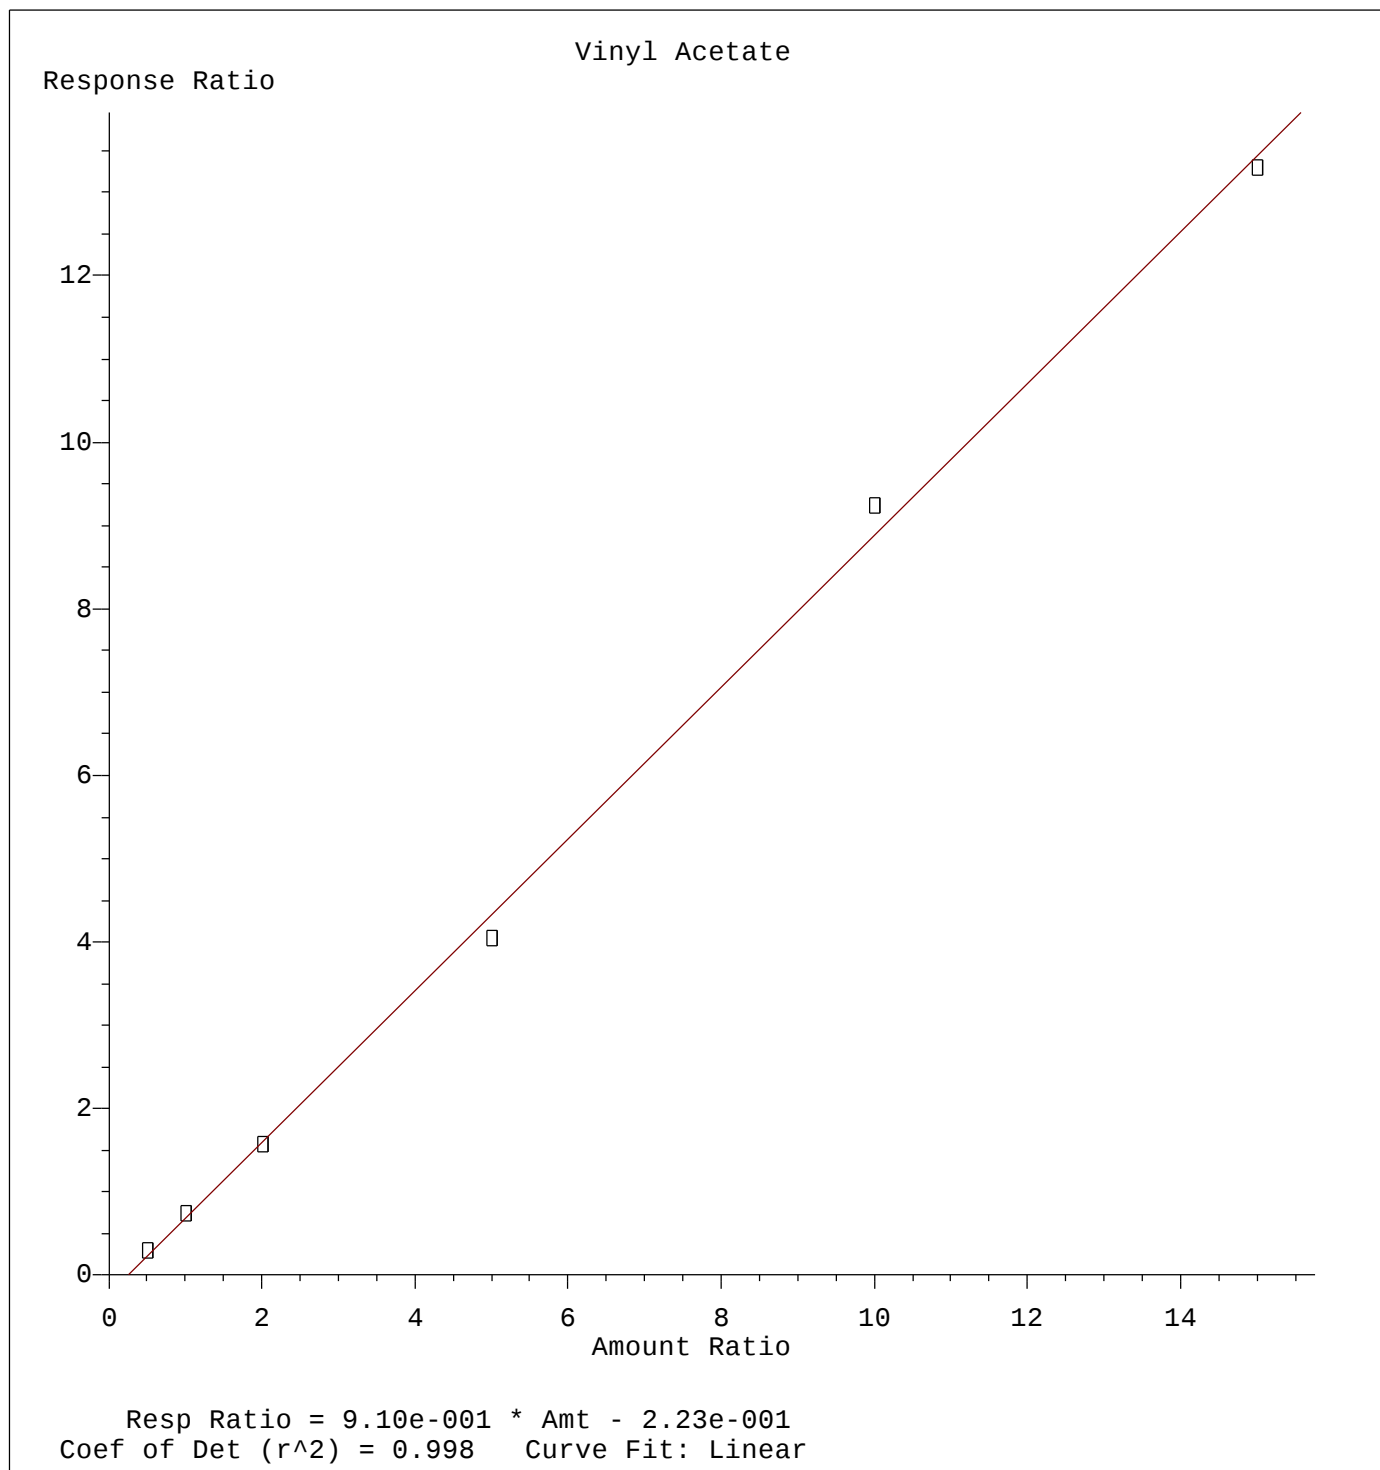


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D042420S.M
Calibration Table Last Updated: Fri Apr 24 14:44:29 2020

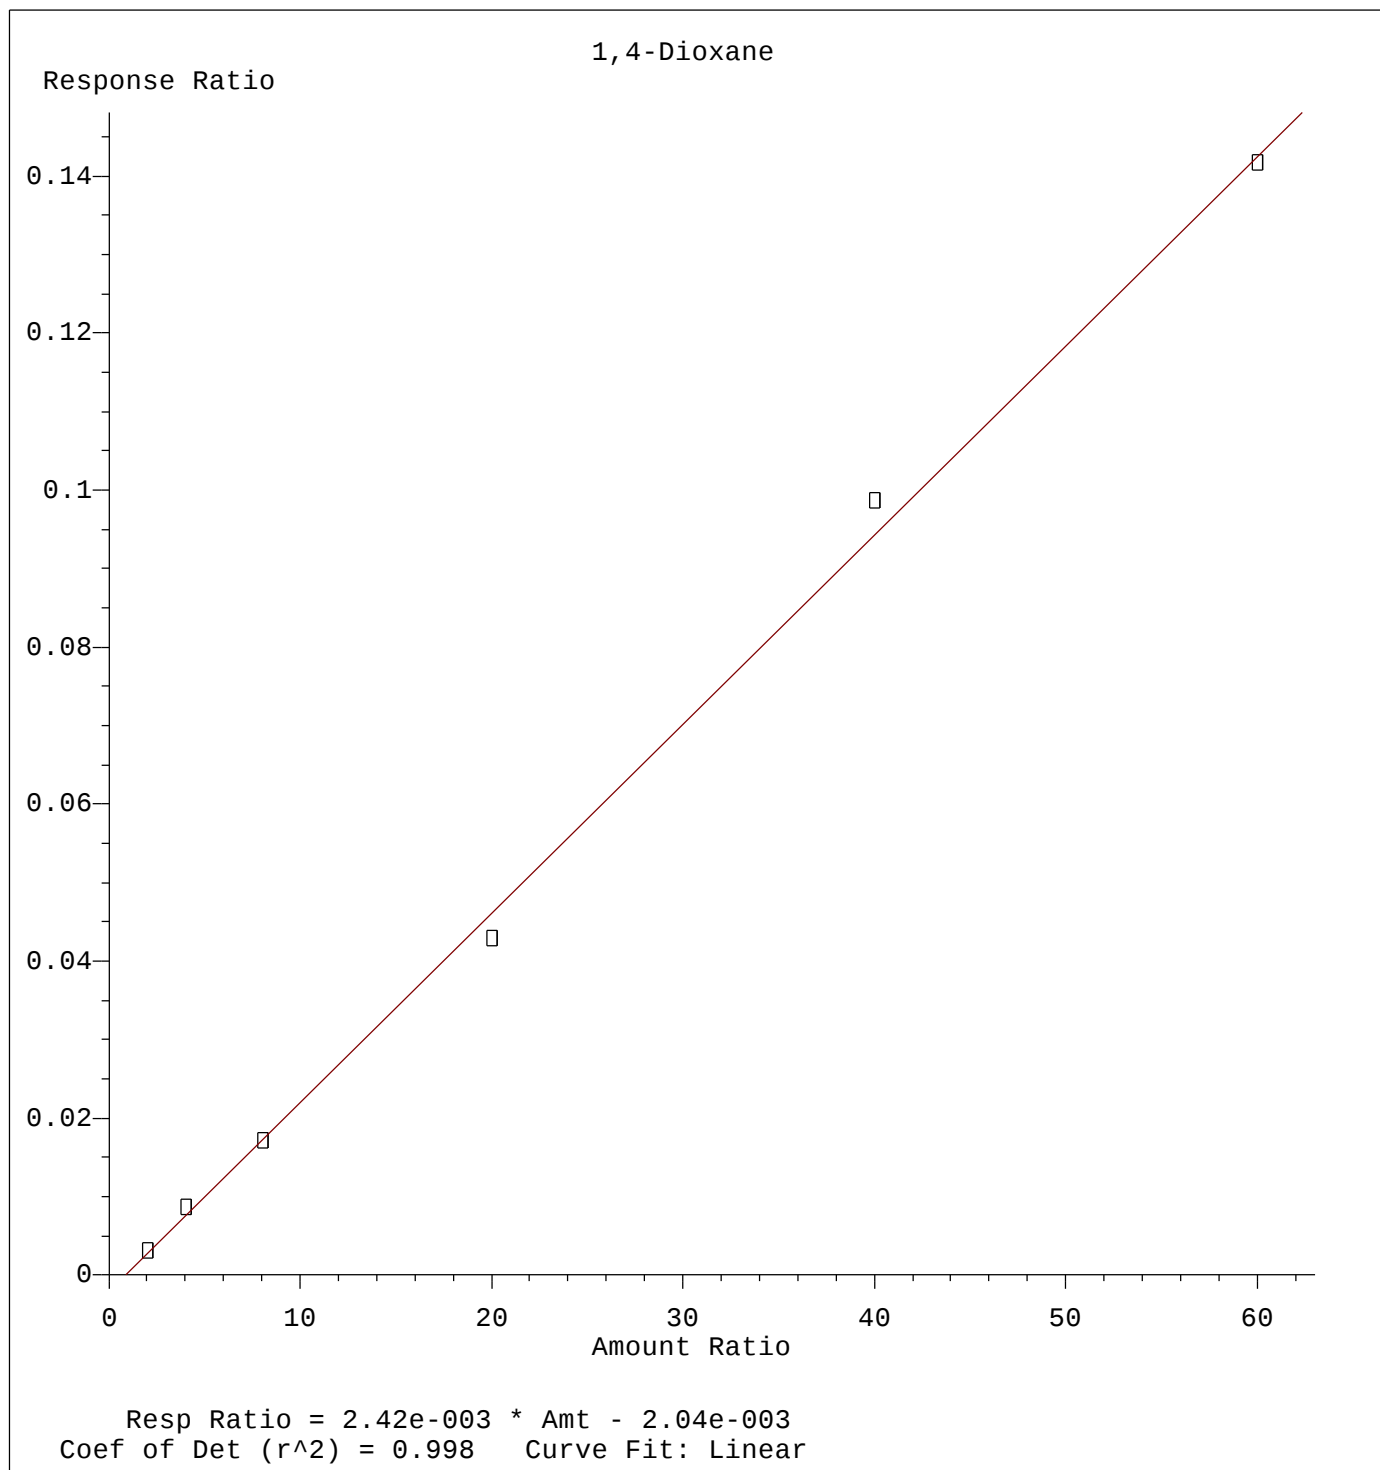

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D042420S.M
Calibration Table Last Updated: Fri Apr 24 14:44:29 2020

Ethyl methacrylate

Response Ratio

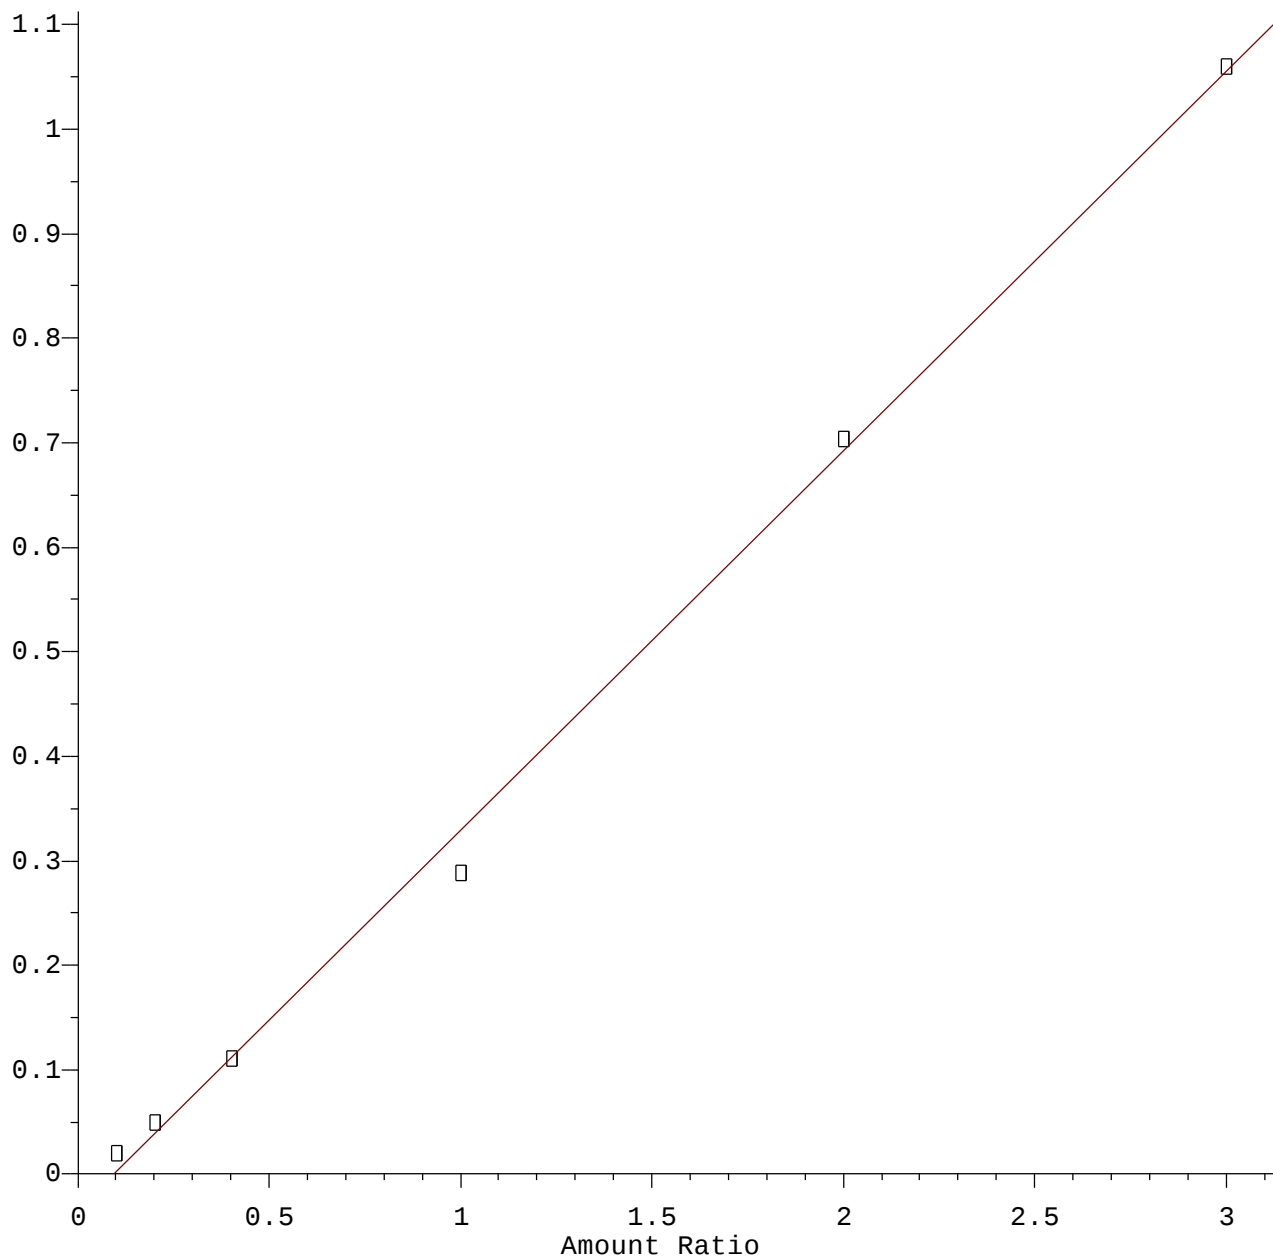

Resp Ratio = $3.63 \times 10^{-1} \times \text{Amt} - 3.34 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D042420S.M
Calibration Table Last Updated: Fri Apr 24 14:44:29 2020