


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD042420\
Data File : VD065670.D
Acq On : 24 Apr 2020 10:26
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D042420S.M
Title : SW846 8260
Last Update : Fri Apr 24 14:44:29 2020

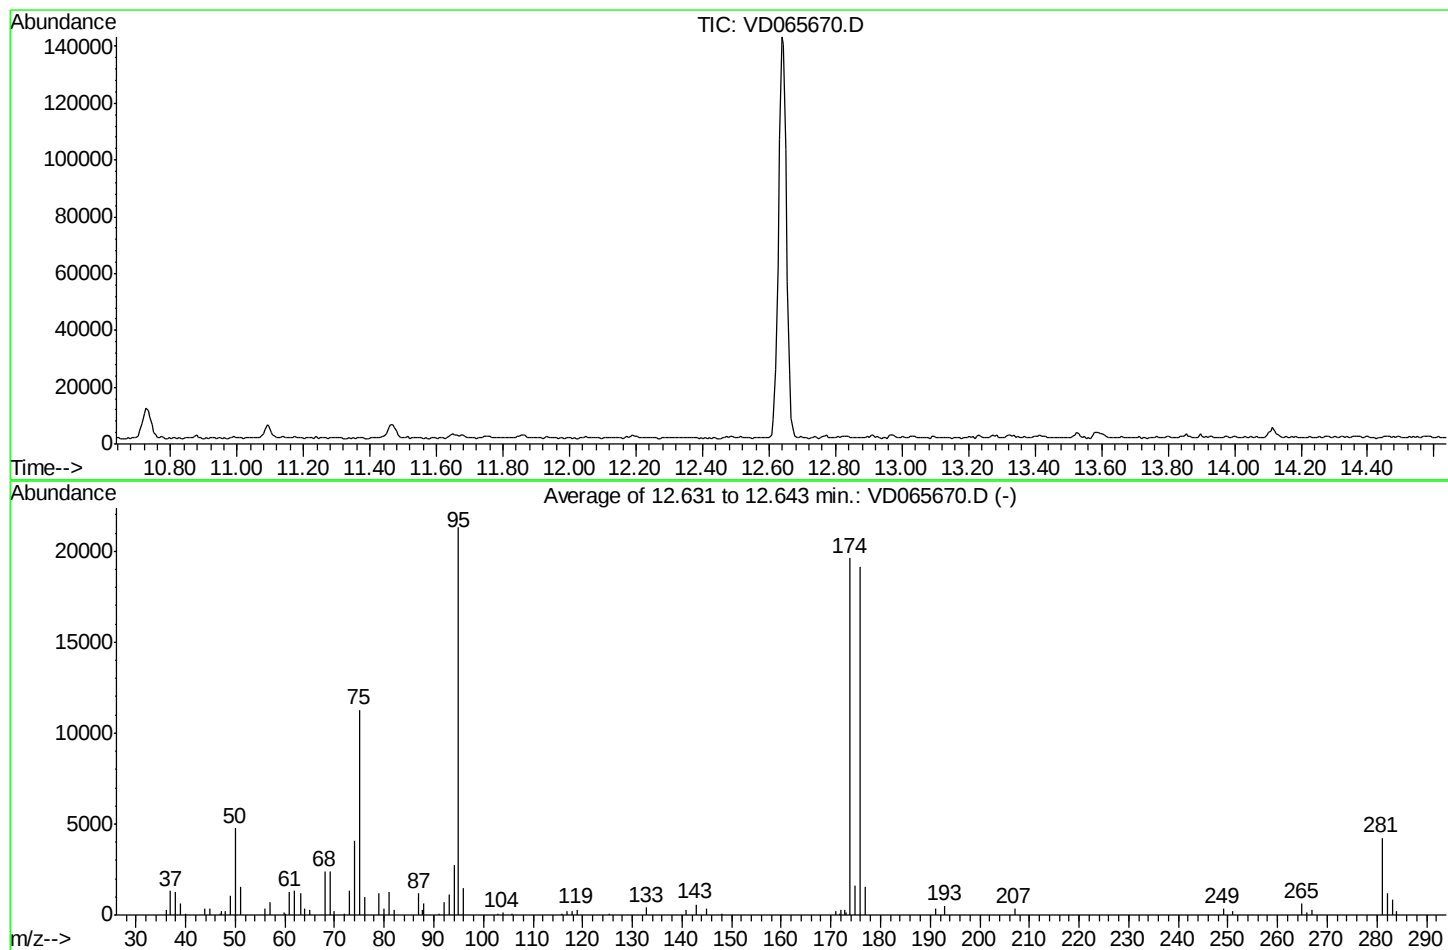

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1814

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.3	4754	PASS
75	95	30	60	52.9	11270	PASS
95	95	100	100	100.0	21309	PASS
96	95	5	9	6.9	1467	PASS
173	174	0.00	2	1.5	301	PASS
174	95	50	100	92.0	19604	PASS
175	174	5	9	8.2	1599	PASS
176	174	95	101	97.8	19173	PASS
177	176	5	9	8.0	1543	PASS