
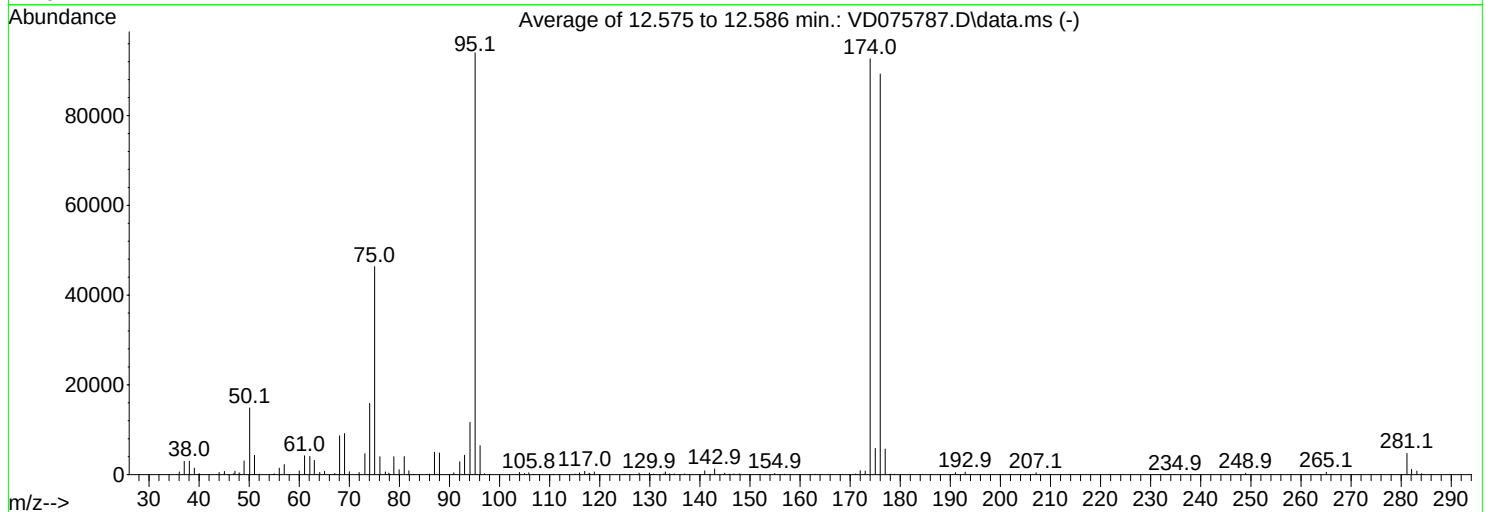


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042423\
Data File : VD075787.D
Acq On : 24 Apr 2023 09:51
Operator : KP/SY
Sample : BFB
Misc : 5.00G/10.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D041323S.M
Title : SW846 8260
Last Update : Thu Apr 13 14:16:29 2023

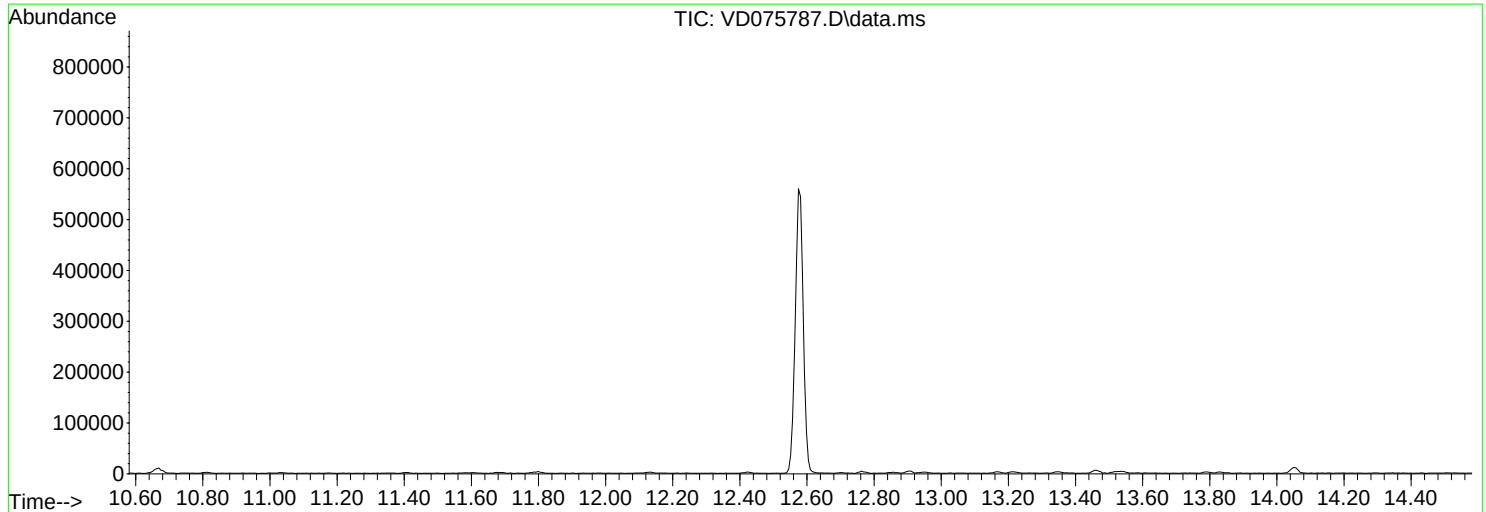

AutoFind: Scans 1868, 1869, 1870; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	14859	PASS
75	95	30	60	49.3	46325	PASS
95	95	100	100	100.0	93968	PASS
96	95	5	9	6.9	6442	PASS
173	174	0.00	2	0.9	793	PASS
174	95	50	100	98.6	92627	PASS
175	174	5	9	6.3	5848	PASS
176	174	95	101	96.3	89243	PASS
177	176	5	9	6.4	5711	PASS