


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD042519\
Data File : VD062028.D
Acq On : 25 Apr 2019 9:37
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D042319S.M
Title : SW846 8260
Last Update : Tue Apr 23 14:52:55 2019

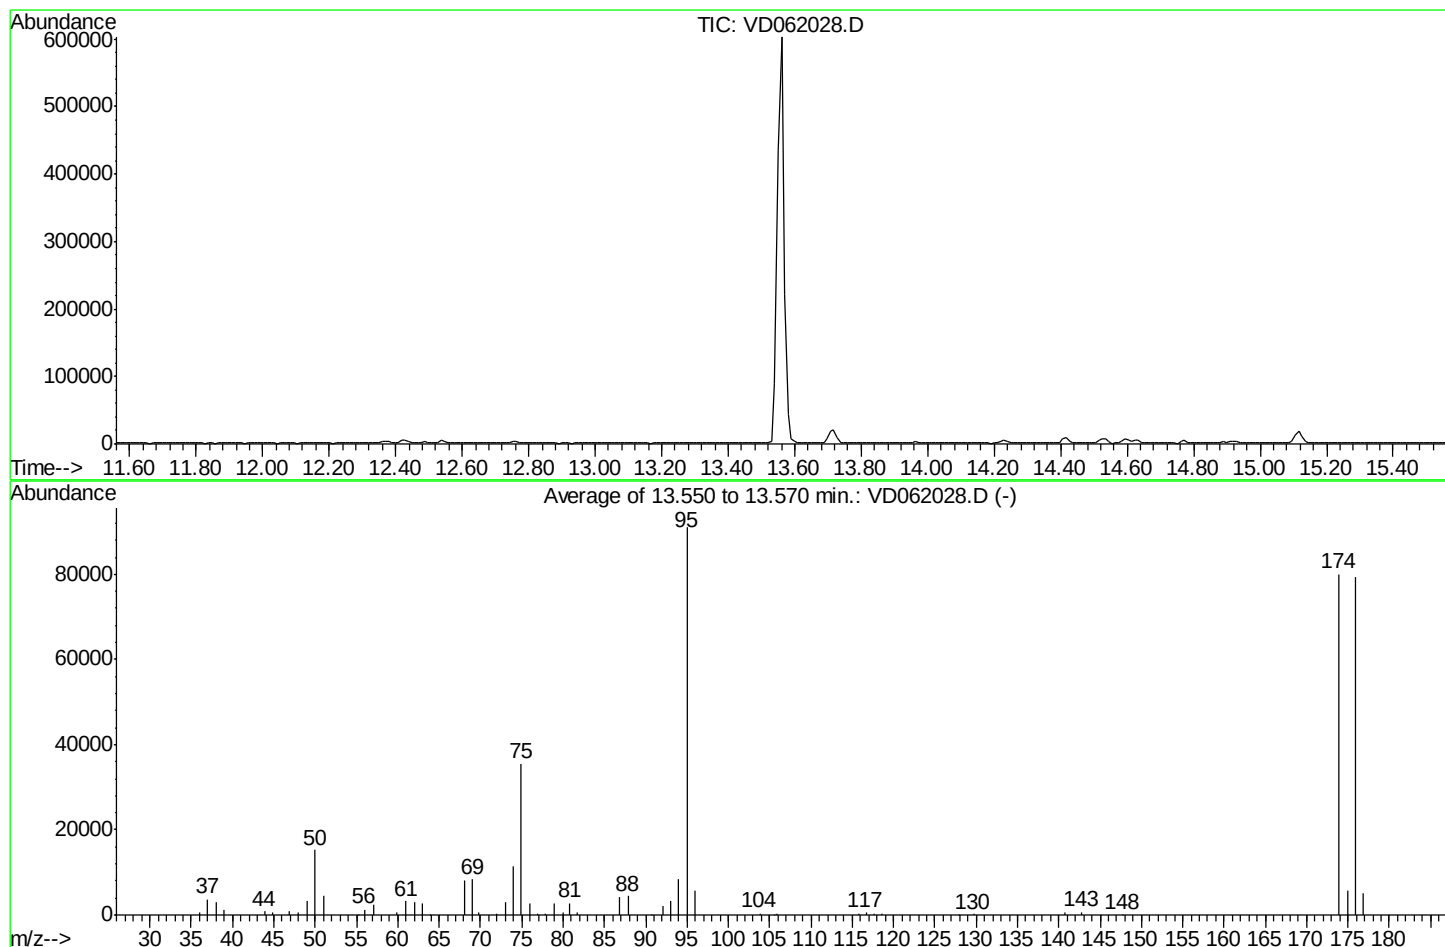

AutoFind: Scans 1232, 1233, 1234; Background Corrected with Scan 1227

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	15259	PASS
75	95	30	60	39.0	35530	PASS
95	95	100	100	100.0	91018	PASS
96	95	5	9	6.4	5802	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	87.9	80050	PASS
175	174	5	9	7.1	5678	PASS
176	174	95	101	99.0	79213	PASS
177	176	5	9	6.4	5097	PASS