




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042523\
 Data File : VD075811.D
 Acq On : 25 Apr 2023 15:02
 Operator : KP/SY
 Sample : 02447-08RE
 Misc : 4.35G/10.00mL/MSVOA_D/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 EW913RE

Manual IntegrationsAPPROVED

Quant Time: Apr 26 02:42:09 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 26 02:39:47 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/26/2023
 Supervised By :Mahesh Dadoda 04/26/2023

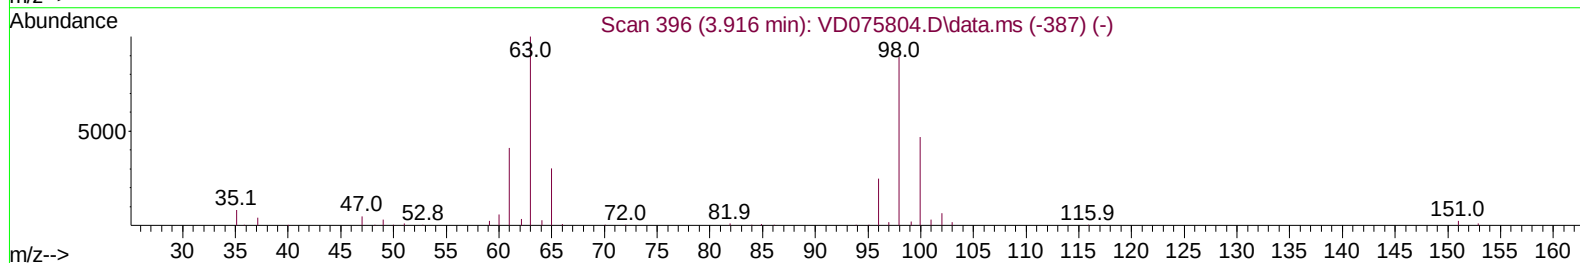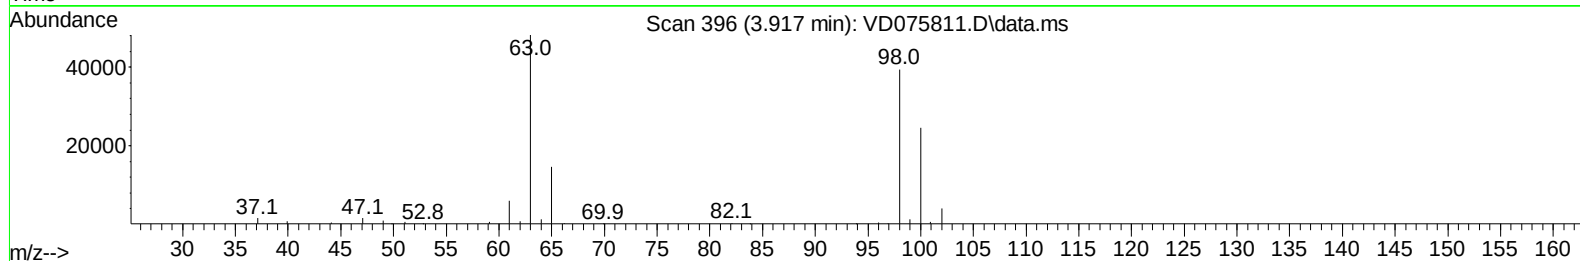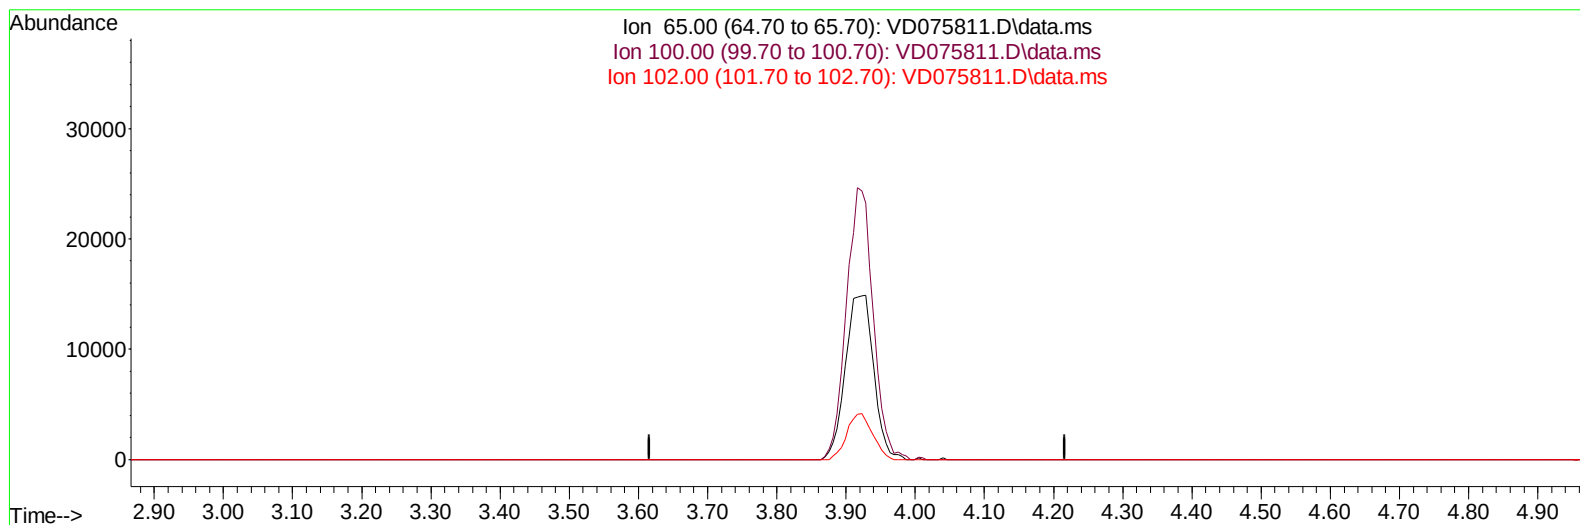

TIC: VD075811.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

3.916min (-3.916) 0.00 ug/L

response 0

Ion	Exp%	Act%
65.00	100.00	0.00
100.00	177.20	0.00#
102.00	27.10	0.00#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042523\
Data File : VD075811.D
Acq On : 25 Apr 2023 15:02
Operator : KP/SY
Sample : 02447-08RE
Misc : 4.35G/10.00mL/MSVOA_D/SOIL
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
EW913RE

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/26/2023
Supervised By :Mahesh Dadoda 04/26/2023

Quant Time: Apr 26 02:42:09 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 26 02:39:47 2023
Response via : Initial Calibration

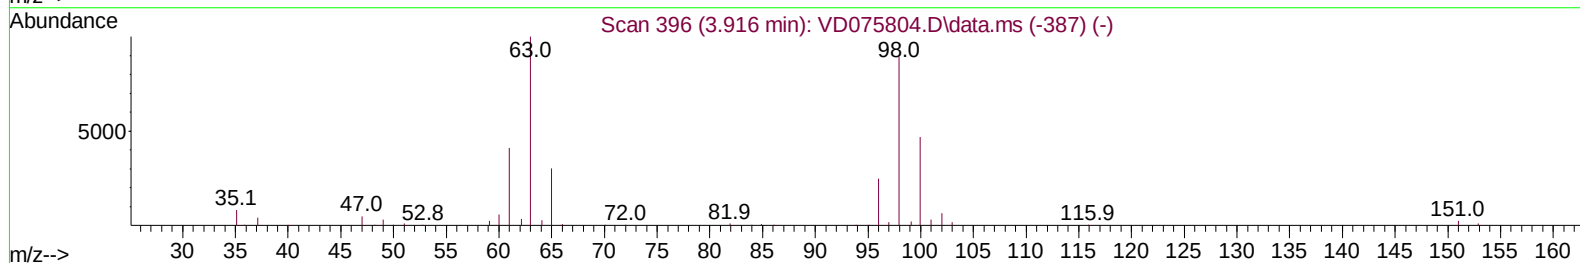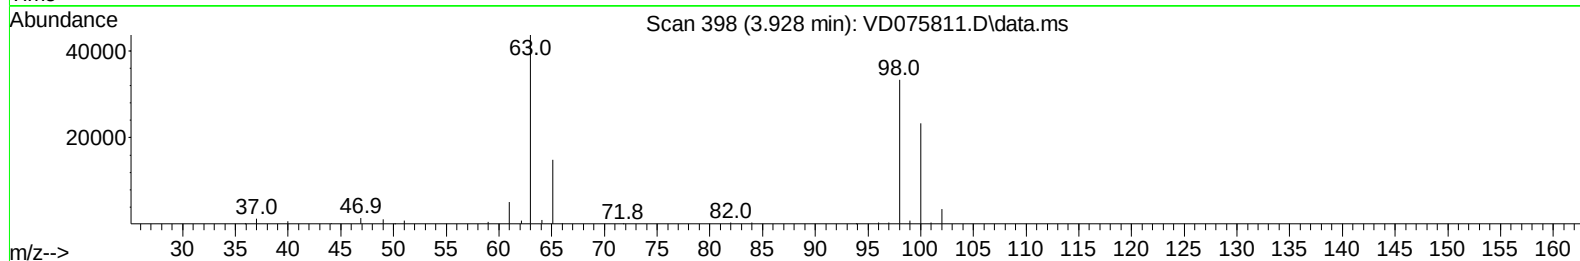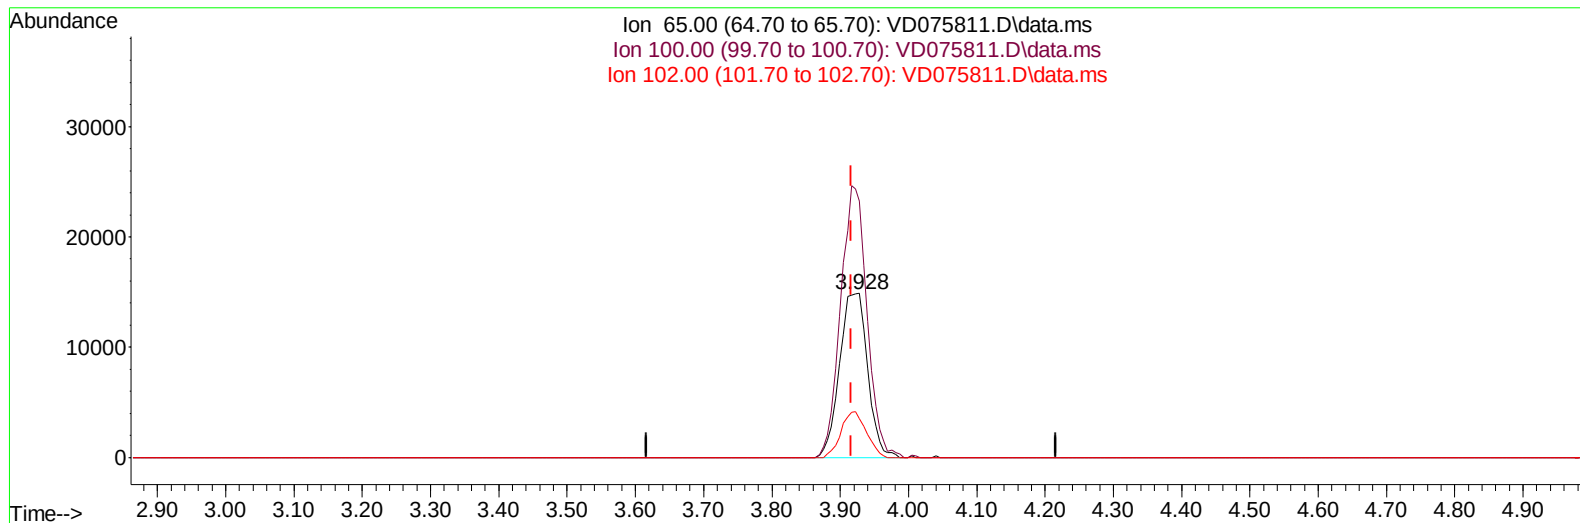

TIC: VD075811.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

3.928min (+ 0.012) 16.73 ug/L m

response 42275

Ion	Exp%	Act%
65.00	100.00	100.00
100.00	177.20	0.00#
102.00	27.10	0.00#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042523\
 Data File : VD075811.D
 Acq On : 25 Apr 2023 15:02
 Operator : KP/SY
 Sample : 02447-08RE
 Misc : 4.35G/10.00mL/MSVOA_D/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 EW913RE

Manual IntegrationsAPPROVED

Quant Time: Apr 26 02:42:09 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 26 02:39:47 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/26/2023
 Supervised By :Mahesh Dadoda 04/26/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.781	114		499563	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117		366451	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.522	152		77332	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.275	65		183464	16.741	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	66.960%	
7) Chloroethane-d5	2.805	69		172706	18.239	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	72.960%	
11) 1,1-Dichloroethene-d2	3.928	65		42275m	16.732	ug/L	0.01
Spiked Amount 25.000	Range 45	- 110		Recovery	=	66.920%	
21) 2-Butanone-d5	6.987	46		41340	43.452	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	86.900%	
24) Chloroform-d	7.569	84		250985	20.091	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	80.360%	
26) 1,2-Dichloroethane-d4	8.234	65		106307	19.927	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	79.720%	
32) Benzene-d6	8.199	84		478789	22.417	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	89.680%	
36) 1,2-Dichloropropane-d6	9.210	67		151820	25.681	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	102.720%	
41) Toluene-d8	10.269	98		374378	18.723	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	74.880%	
43) trans-1,3-Dichloroprop...	10.528	79		49529	20.269	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	81.080%	
47) 2-Hexanone-d5	10.881	63		33869	47.581	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	95.160%	
56) 1,1,2,2-Tetrachloroeth...	12.651	84		96850	21.409	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	85.640%	
66) 1,2-Dichlorobenzene-d4	13.816	152		53518	19.566	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	78.280%	
Target Compounds							
16) Methylene chloride	4.805	84		37042	3.655	ug/L	Qvalue 93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042523\
Data File : VD075811.D
Acq On : 25 Apr 2023 15:02
Operator : KP/SY
Sample : 02447-08RE
Misc : 4.35G/10.00mL/MSVOA_D/SOIL
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
EW913RE

Manual IntegrationsAPPROVED

Quant Time: Apr 26 02:42:09 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 26 02:39:47 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 04/26/2023
Supervised By :Mahesh Dadoda 04/26/2023

