




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042523\
 Data File : VD075816.D
 Acq On : 25 Apr 2023 17:26
 Operator : KP/SY
 Sample : 02419-09RE
 Misc : 5.17G/10.00mL/MSVOA_D/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 EW924RE

Manual IntegrationsAPPROVED

Quant Time: Apr 26 02:43:25 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 26 02:39:47 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/26/2023
 Supervised By :Mahesh Dadoda 04/26/2023

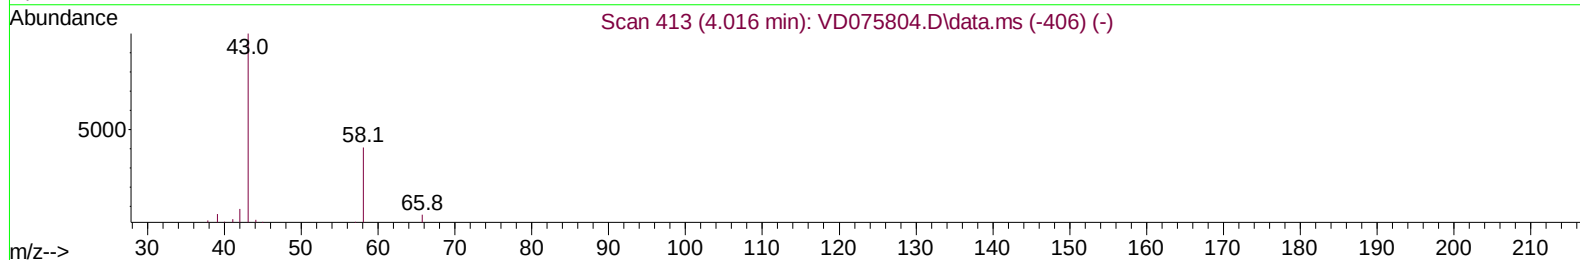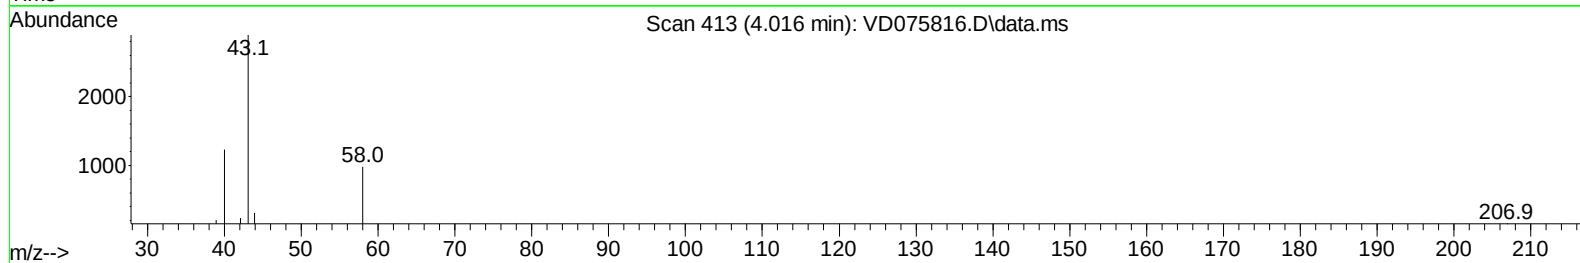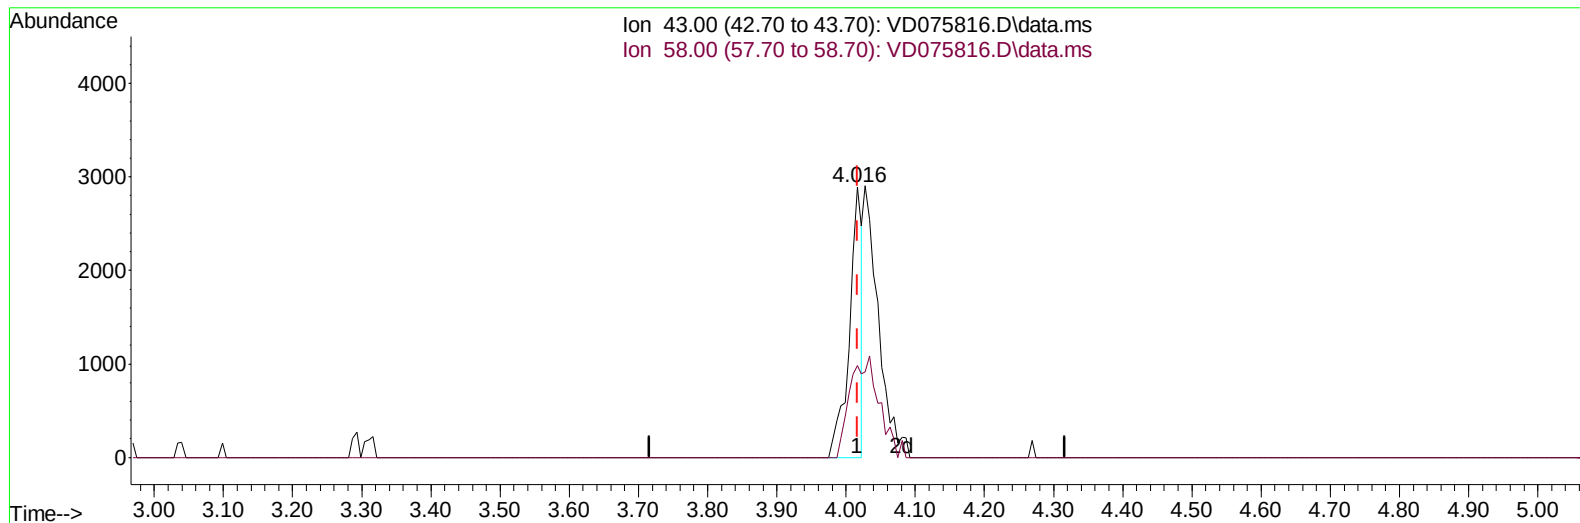

TIC: VD075816.D\data.ms

(13) Acetone (T)

4.016min (-0.000) 9.90 ug/L

response 3683

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	43.70	39.26
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042523\
 Data File : VD075816.D
 Acq On : 25 Apr 2023 17:26
 Operator : KP/SY
 Sample : 02419-09RE
 Misc : 5.17G/10.00mL/MSVOA_D/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 EW924RE

Manual IntegrationsAPPROVED

Quant Time: Apr 26 02:43:25 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 26 02:39:47 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/26/2023
 Supervised By :Mahesh Dadoda 04/26/2023

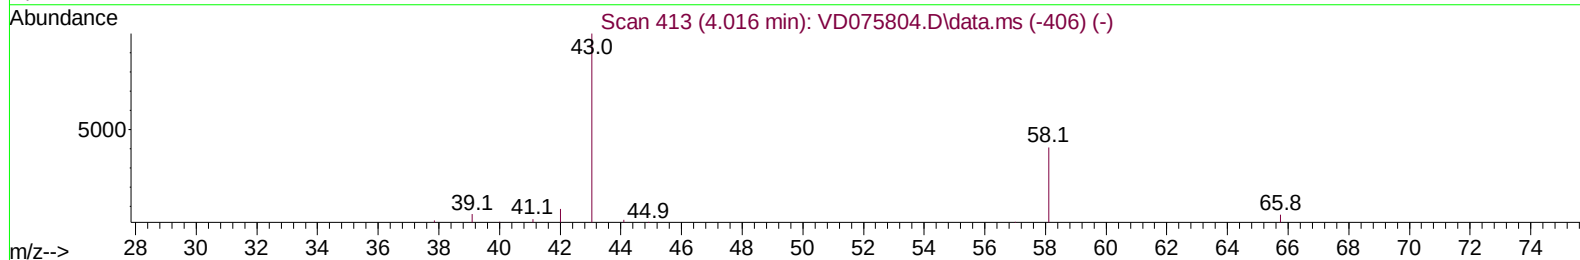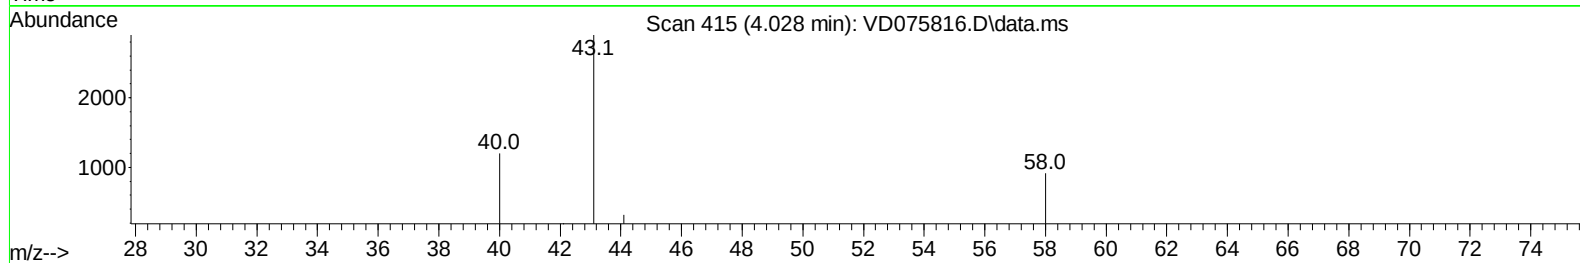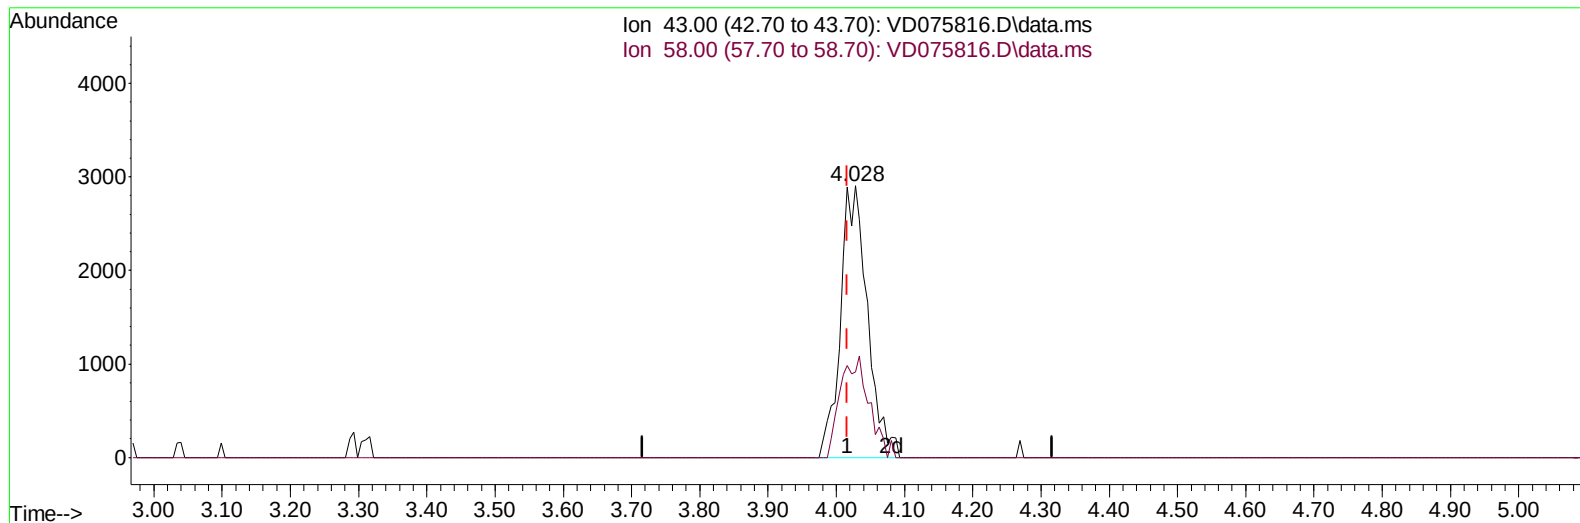

TIC: VD075816.D\data.ms

(13) Acetone (T)

4.028min (+ 0.011) 21.45 ug/L m

response 7978

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	43.70	18.12
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042523\
 Data File : VD075816.D
 Acq On : 25 Apr 2023 17:26
 Operator : KP/SY
 Sample : 02419-09RE
 Misc : 5.17G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 EW924RE

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/26/2023
 Supervised By :Mahesh Dadoda 04/26/2023

Quant Time: Apr 26 02:43:25 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 26 02:39:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.781	114	228213	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.580	117	208151	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.522	152	56302	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.275	65	80109	16.001	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	64.000%	
7) Chloroethane-d5	2.804	69	82983	19.184	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	76.720%	
11) 1,1-Dichloroethene-d2	3.916	65	18596	16.111	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	64.440%	
21) 2-Butanone-d5	6.987	46	44872	103.245	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	206.480%#	
24) Chloroform-d	7.569	84	141743	24.837	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	99.360%	
26) 1,2-Dichloroethane-d4	8.234	65	80599	33.072	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	132.280%#	
32) Benzene-d6	8.198	84	254610	20.987	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	83.960%	
36) 1,2-Dichloropropane-d6	9.210	67	90874	27.062	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	108.240%	
41) Toluene-d8	10.269	98	201606	17.750	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	71.000%	
43) trans-1,3-Dichloroprop...	10.528	79	37701	27.162	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	108.640%	
47) 2-Hexanone-d5	10.875	63	36028	89.106	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	178.220%#	
56) 1,1,2,2-Tetrachloroeth...	12.651	84	96129	37.410	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	149.640%#	
66) 1,2-Dichlorobenzene-d4	13.816	152	44953	22.573	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	90.280%	
Target Compounds					Qvalue	
13) Acetone	4.028	43	7978m	21.450	ug/L	
16) Methylene chloride	4.804	84	13261	2.864	ug/L	95
46) Tetrachloroethene	10.810	164	1643	0.615	ug/L #	80

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042523\
Data File : VD075816.D
Acq On : 25 Apr 2023 17:26
Operator : KP/SY
Sample : 02419-09RE
Misc : 5.17G/10.00mL/MSVOA_D/SOIL
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
EW924RE

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/26/2023
Supervised By :Mahesh Dadoda 04/26/2023

Quant Time: Apr 26 02:43:25 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 26 02:39:47 2023
Response via : Initial Calibration

