
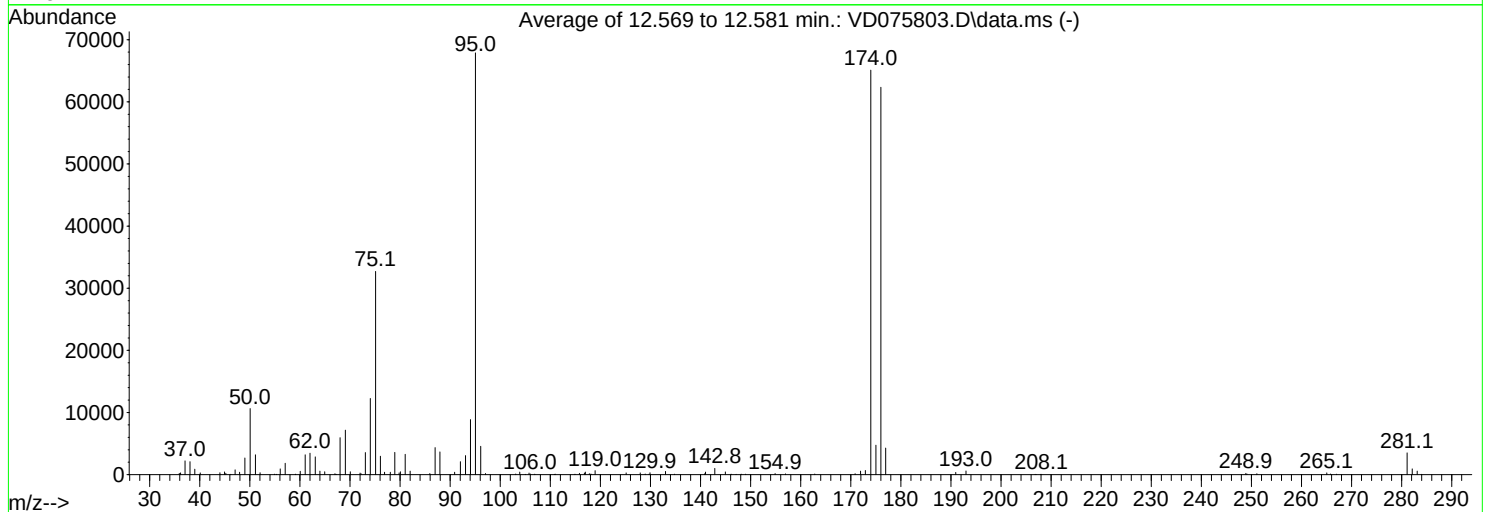


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042523\
Data File : VD075803.D
Acq On : 25 Apr 2023 10:13
Operator : KP/SY
Sample : BFB118
Misc : 5.00G/10.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB118

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Title : SFAM01.0
Last Update : Mon May 01 00:14:49 2023

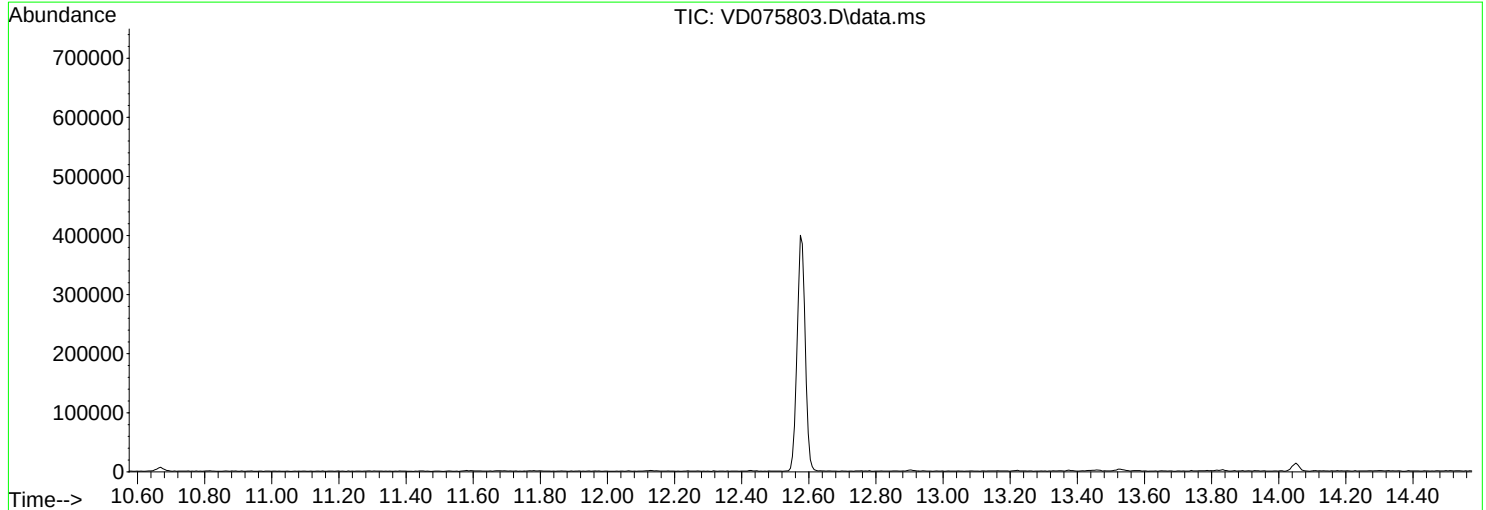

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	10649	PASS
75	95	30	80	48.2	32715	PASS
95	95	100	100	100.0	67885	PASS
96	95	5	9	6.7	4559	PASS
173	174	0.00	2	1.0	679	PASS
174	95	50	120	95.9	65091	PASS
175	174	5	9	7.3	4737	PASS
176	174	95	105	95.8	62336	PASS
177	176	5	10	6.9	4278	PASS

Scan 1860 (12.528 min): VD075803.D\data.ms
BFB118

m/z	Abundance
40.00	697.0
44.00	366.0
207.10	214.0

Instrument :
MSVOA_D
ClientSampleId :
BFB118

m/z	Abundance
35.90	325.0
37.00	2046.0
38.10	1825.0
39.00	704.0
39.90	880.0
44.00	753.0
44.90	577.0
47.00	630.0
47.90	343.0
49.00	2631.0
50.00	8806.0
51.10	2950.0
52.00	246.0
56.00	816.0
57.10	1727.0
60.10	557.0
61.00	2668.0
62.00	3248.0
63.00	2531.0
64.00	427.0
65.00	280.0
67.00	170.0
68.00	5038.0
69.00	6306.0
70.00	395.0
72.00	237.0
73.00	2698.0
74.10	10287.0
75.10	28432.0
76.10	2415.0
76.90	328.0
78.10	359.0
78.90	3438.0
80.10	523.0
81.00	2476.0
82.00	367.0
87.00	2989.0
87.90	3306.0
91.00	331.0
92.10	1624.0
93.10	2490.0
94.10	8354.0
95.10	57464.0
96.10	3983.0
97.00	204.0
103.90	379.0
106.00	285.0
114.90	213.0
116.80	761.0
117.80	249.0
118.90	572.0
128.00	251.0
129.00	161.0
129.70	258.0
133.10	217.0
140.80	417.0
142.90	1112.0
145.00	390.0
146.10	248.0
149.00	220.0
154.90	198.0
162.80	154.0
170.90	213.0
171.90	392.0
172.90	545.0
174.00	51584.0
175.00	4063.0
176.00	50472.0
176.90	4023.0
191.00	433.0
193.00	381.0
206.80	176.0
248.90	266.0
265.20	220.0
281.10	2256.0
282.10	583.0
283.10	277.0

Instrument :
MSVOA_D
ClientSampleId :
BFB118

m/z	Abundance
35.90	318.0
36.20	320.0
37.10	2387.0
38.00	2454.0
39.00	923.0
40.10	880.0
44.00	637.0
45.00	768.0
46.20	160.0
47.10	984.0
48.00	404.0
49.00	2753.0
50.00	12367.0
51.10	3244.0
52.10	401.0
55.30	165.0
56.00	1092.0
57.10	1698.0
59.90	545.0
61.10	3901.0
62.00	3728.0
63.10	2957.0
64.00	664.0
65.00	665.0
67.00	328.0
68.00	6670.0
69.10	8181.0
70.00	394.0
72.20	478.0
73.10	3735.0
74.10	13536.0
75.10	35392.0
76.10	3363.0
76.90	497.0
78.10	402.0
78.90	3939.0
79.80	838.0
81.00	4001.0
82.00	683.0
85.90	253.0
87.10	5078.0
88.00	4087.0
90.80	386.0
92.00	2247.0
93.00	3547.0
94.00	9580.0
95.10	75360.0
96.10	4879.0
97.00	164.0
103.10	305.0
103.90	578.0
105.70	429.0
106.90	209.0
110.80	173.0
115.80	303.0
117.00	712.0
117.80	191.0
119.00	632.0
125.10	369.0
127.90	350.0
129.90	402.0
133.10	554.0
141.00	575.0
142.80	937.0
144.90	516.0
147.10	179.0
148.10	267.0
154.90	171.0
157.00	184.0
162.80	158.0
170.80	247.0
172.00	569.0
173.00	554.0
174.00	72576.0
175.00	4830.0
176.00	69584.0
177.00	4218.0
191.00	174.0
193.00	712.0
207.00	228.0
207.90	171.0
249.10	302.0
251.20	213.0
265.00	372.0
281.10	3361.0
282.10	1014.0
283.00	630.0

Instrument :
MSVOA_D
ClientSampleId :
BFB118

m/z	Abundance
36.10	532.0
37.10	2178.0
38.10	2013.0
39.00	992.0
39.90	926.0
44.00	633.0
45.20	647.0
47.10	721.0
47.90	399.0
49.00	2672.0
50.10	10774.0
51.10	3407.0
52.00	256.0
54.90	224.0
56.10	850.0
57.00	2064.0
59.10	249.0
60.10	543.0
61.00	3017.0
62.00	3407.0
63.10	3093.0
64.00	607.0
64.90	440.0
67.20	194.0
68.00	6129.0
69.10	6979.0
70.10	597.0
72.00	531.0
73.00	4220.0
74.00	12956.0
75.10	34320.0
76.00	3104.0
76.90	315.0
77.90	417.0
79.00	3409.0
80.00	878.0
81.00	3342.0
82.00	684.0
86.00	277.0
86.90	4999.0
88.00	3551.0
90.90	426.0
92.10	2422.0
93.00	3155.0
94.10	8619.0
95.00	70832.0
96.10	4814.0
97.10	190.0
103.80	318.0
105.00	191.0
105.80	359.0
111.00	225.0
115.80	295.0
117.00	565.0
118.10	338.0
118.90	755.0
125.20	458.0
128.00	244.0
128.90	152.0
129.90	509.0
132.90	779.0
134.80	229.0
141.00	656.0
142.90	982.0
144.90	405.0
154.90	175.0
156.90	228.0
172.00	744.0
172.80	939.0
174.00	71112.0
175.00	5318.0
176.00	66952.0
177.00	4592.0
190.90	471.0
193.00	715.0
207.00	517.0
208.10	186.0
248.90	379.0
251.00	240.0
265.10	293.0
265.80	289.0
267.00	249.0
281.10	4888.0
282.10	1209.0
283.20	763.0
284.00	160.0

Instrument :
MSVOA_D
ClientSampleId :
BFB118