


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD042619\
Data File : VD062052.D
Acq On : 26 Apr 2019 9:25
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D042319S.M
Title : SW846 8260
Last Update : Tue Apr 23 14:52:55 2019

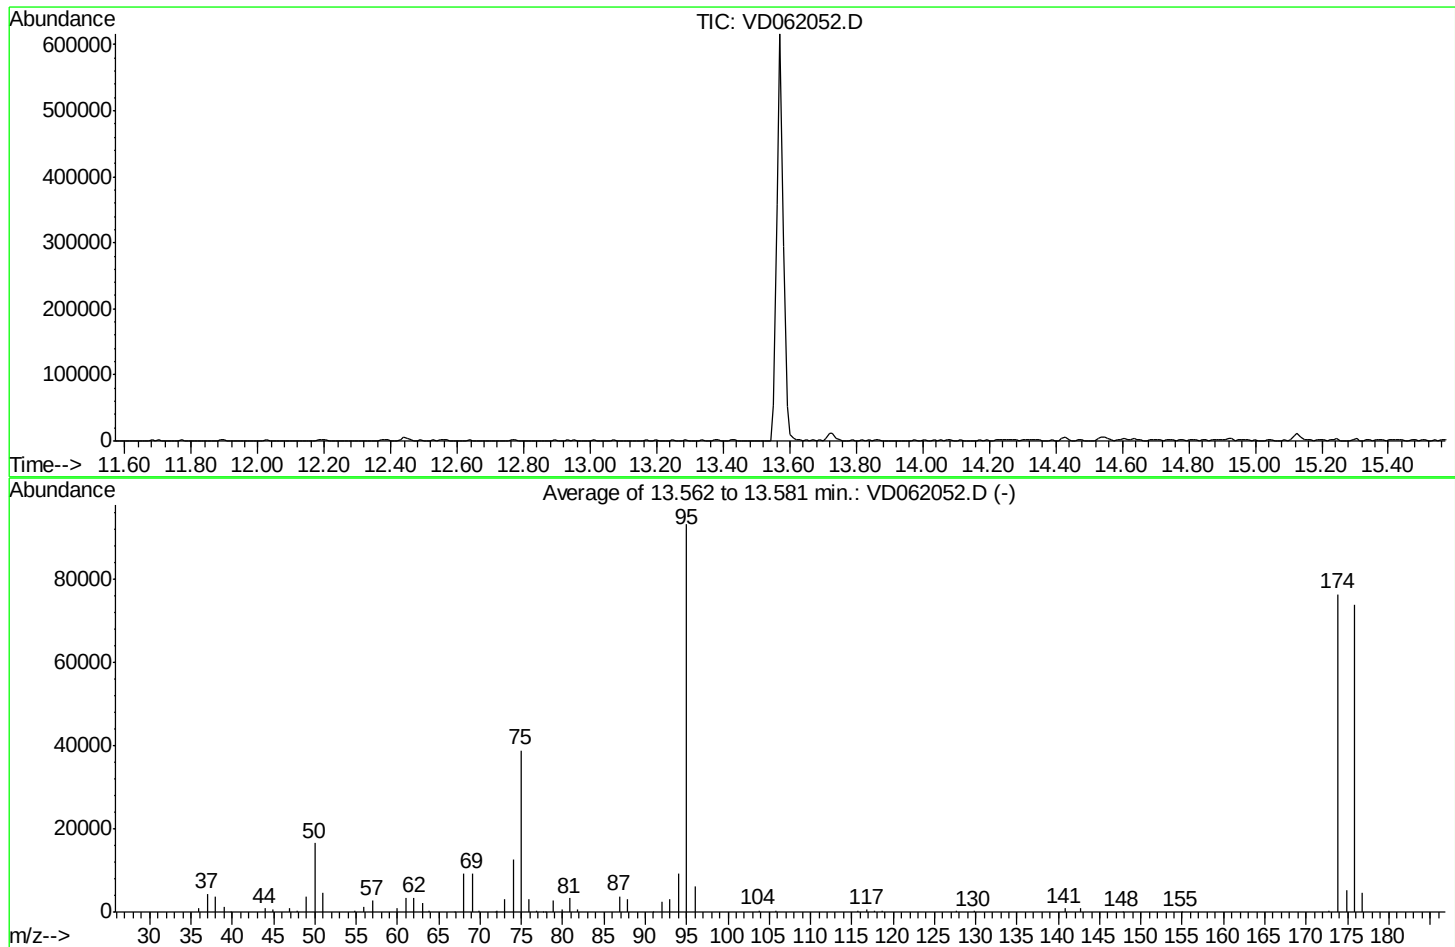

AutoFind: Scans 1233, 1234, 1235; Background Corrected with Scan 1228

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	16512	PASS
75	95	30	60	41.8	38845	PASS
95	95	100	100	100.0	93034	PASS
96	95	5	9	6.5	6082	PASS
173	174	0.00	2	0.6	470	PASS
174	95	50	100	82.0	76256	PASS
175	174	5	9	6.9	5290	PASS
176	174	95	101	96.5	73602	PASS
177	176	5	9	6.4	4694	PASS