




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042623\
 Data File : VD075846.D
 Acq On : 26 Apr 2023 20:35
 Operator : KP/SY
 Sample : 02447-20
 Misc : 5.84G/10.00mL/MSVOA_D/SOIL
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 EW938

Manual IntegrationsAPPROVED

Quant Time: Apr 27 02:06:47 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 27 02:02:18 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/27/2023
 Supervised By :Semsettin Yesilyurt 05/01/2023

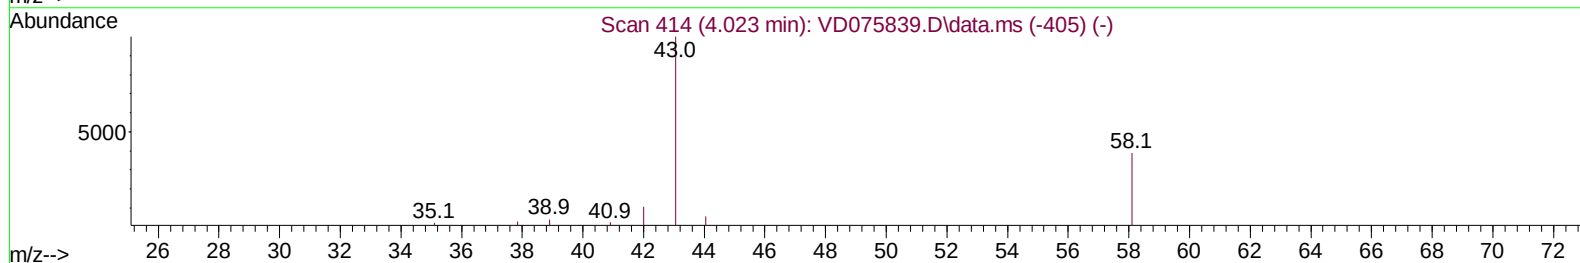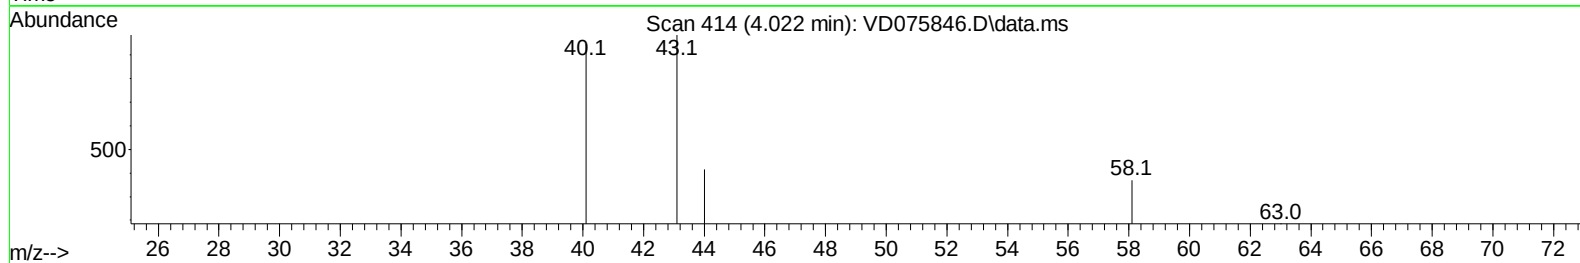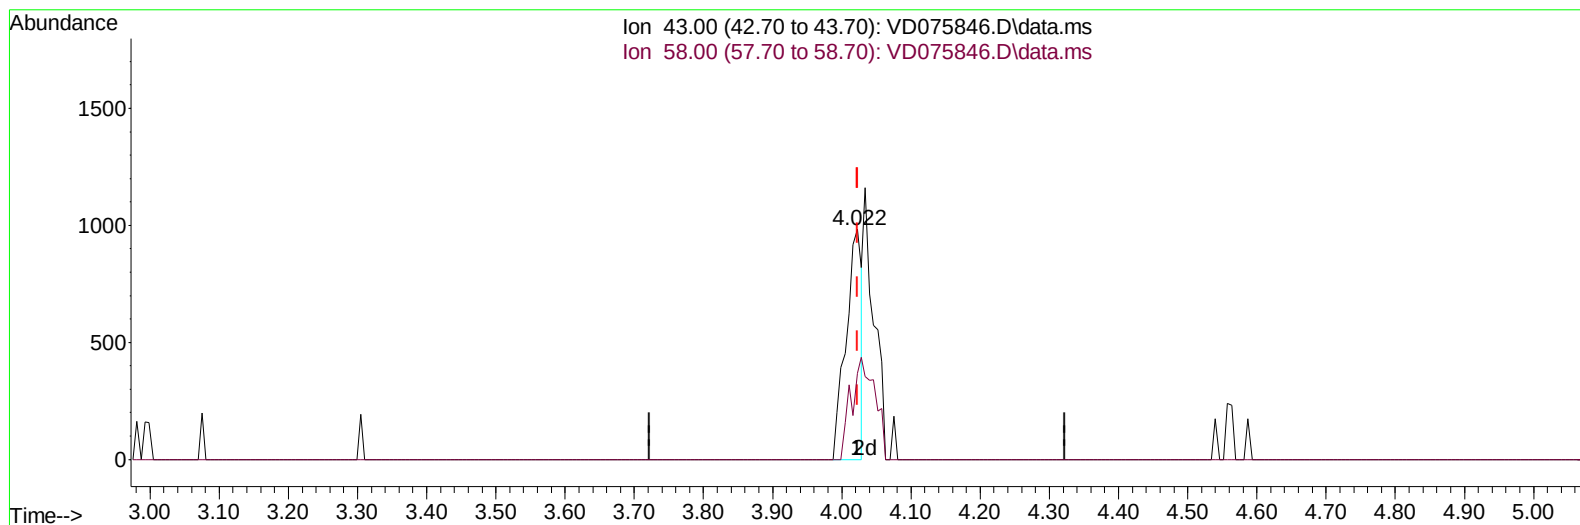

TIC: VD075846.D\data.ms

(13) Acetone (T)

4.022min (-0.000) 2.51 ug/L

response 1550

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	43.70	15.10
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042623\
Data File : VD075846.D
Acq On : 26 Apr 2023 20:35
Operator : KP/SY
Sample : 02447-20
Misc : 5.84G/10.00mL/MSVOA_D/SOIL
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
EW938

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/27/2023
Supervised By :Semsettin Yesilyurt 05/01/2023

Quant Time: Apr 27 02:06:47 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 27 02:02:18 2023
Response via : Initial Calibration

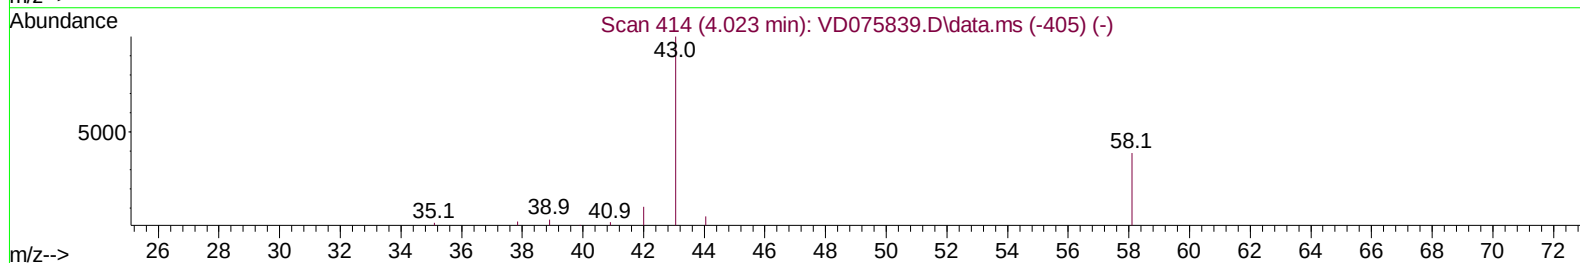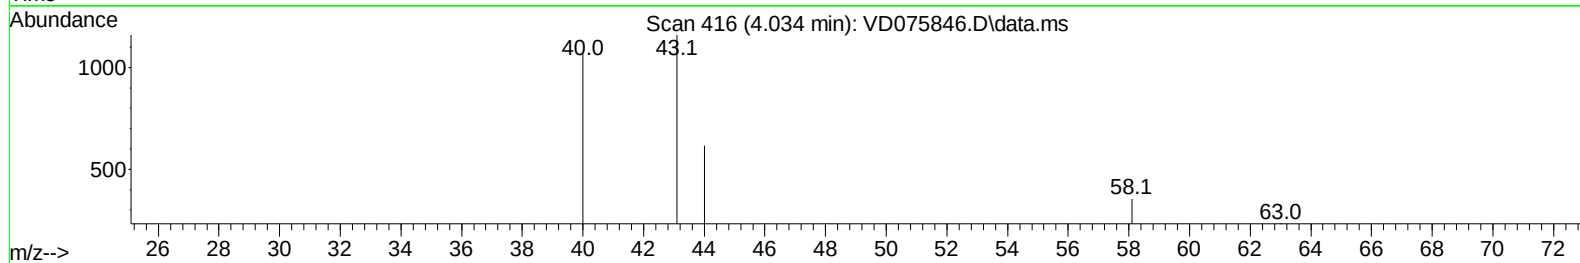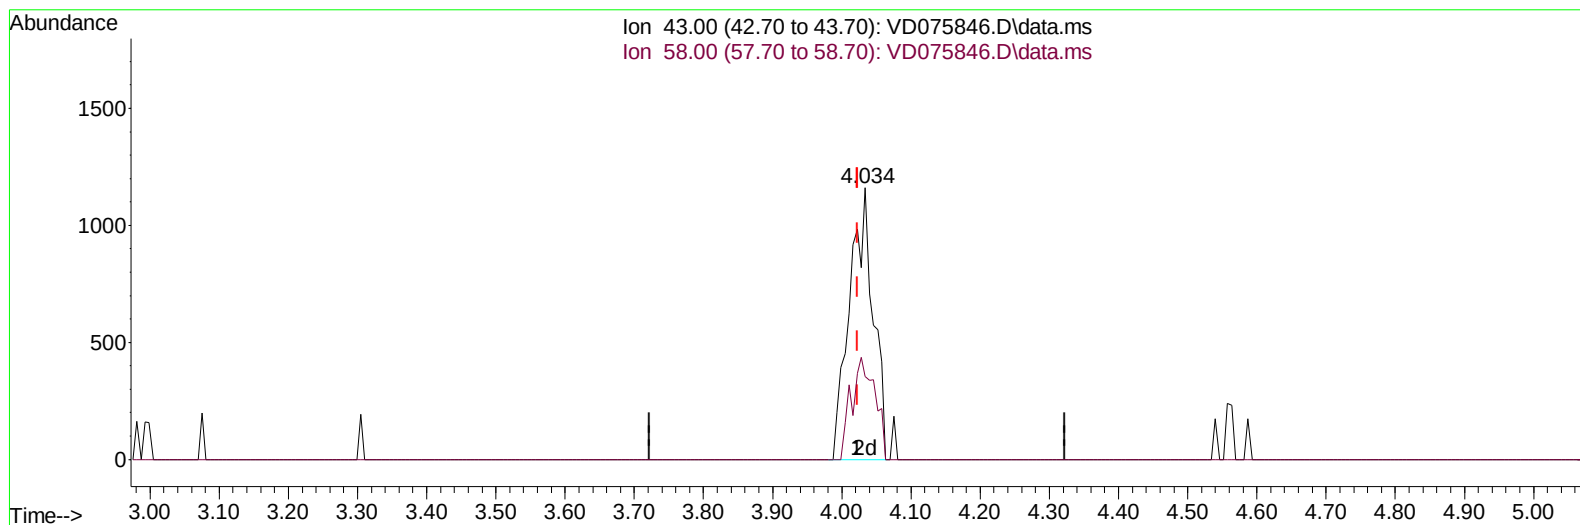

TIC: VD075846.D\data.ms

(13) Acetone (T)

4.034min (+ 0.012) 4.46 ug/L m

response 2754

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	43.70	8.50
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042623\
 Data File : VD075846.D
 Acq On : 26 Apr 2023 20:35
 Operator : KP/SY
 Sample : 02447-20
 Misc : 5.84G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 EW938

Manual IntegrationsAPPROVED

Quant Time: Apr 27 02:06:47 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 27 02:02:18 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/27/2023
 Supervised By :Semsettin Yesilyurt 05/01/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.781	114	378713	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117	227343	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.516	152	46525	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.275	65	163476	19.677	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	78.720%	
7) Chloroethane-d5	2.805	69	156535	21.807	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	87.240%	
11) 1,1-Dichloroethene-d2	3.916	65	35053	18.301	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	73.200%	
21) 2-Butanone-d5	6.987	46	40975	56.812	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	113.620%	
24) Chloroform-d	7.569	84	216873	22.900	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	91.600%	
26) 1,2-Dichloroethane-d4	8.234	65	95501	23.614	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	94.440%	
32) Benzene-d6	8.204	84	408020	30.793	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	123.160%	
36) 1,2-Dichloropropane-d6	9.210	67	132416	36.104	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	144.400%#	
41) Toluene-d8	10.269	98	275595	22.216	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	88.880%	
43) trans-1,3-Dichloroprop...	10.528	79	34318	22.638	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	90.560%	
47) 2-Hexanone-d5	10.881	63	30068	68.088	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	136.180%#	
56) 1,1,2,2-Tetrachloroeth...	12.651	84	96540	34.398	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	137.600%#	
66) 1,2-Dichlorobenzene-d4	13.816	152	37572	22.831	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	91.320%	
Target Compounds						
13) Acetone	4.034	43	2754m	4.462	ug/L	
14) Carbon disulfide	4.275	76	13661	0.785	ug/L #	94
16) Methylene chloride	4.811	84	18880	2.457	ug/L	95
62) 1,3,5-Trimethylbenzene	12.898	105	3847	0.836	ug/L #	56

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042623\
Data File : VD075846.D
Acq On : 26 Apr 2023 20:35
Operator : KP/SY
Sample : 02447-20
Misc : 5.84G/10.00mL/MSVOA_D/SOIL
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
EW938

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/27/2023
Supervised By :Semsettin Yesilyurt 05/01/2023

Quant Time: Apr 27 02:06:47 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 27 02:02:18 2023
Response via : Initial Calibration

