
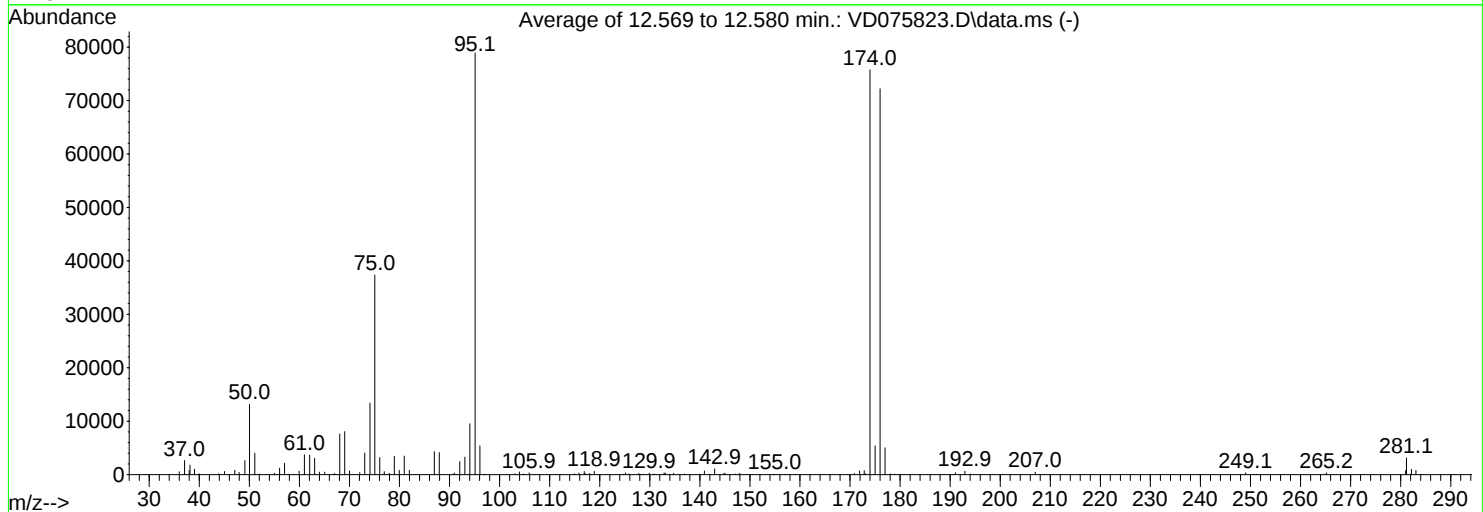


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042623\
 Data File : VD075823.D
 Acq On : 26 Apr 2023 09:18
 Operator : KP/SY
 Sample : BFB119
 Misc : 5.00G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB119

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Title : SFAM01.0
 Last Update : Mon May 01 00:14:49 2023

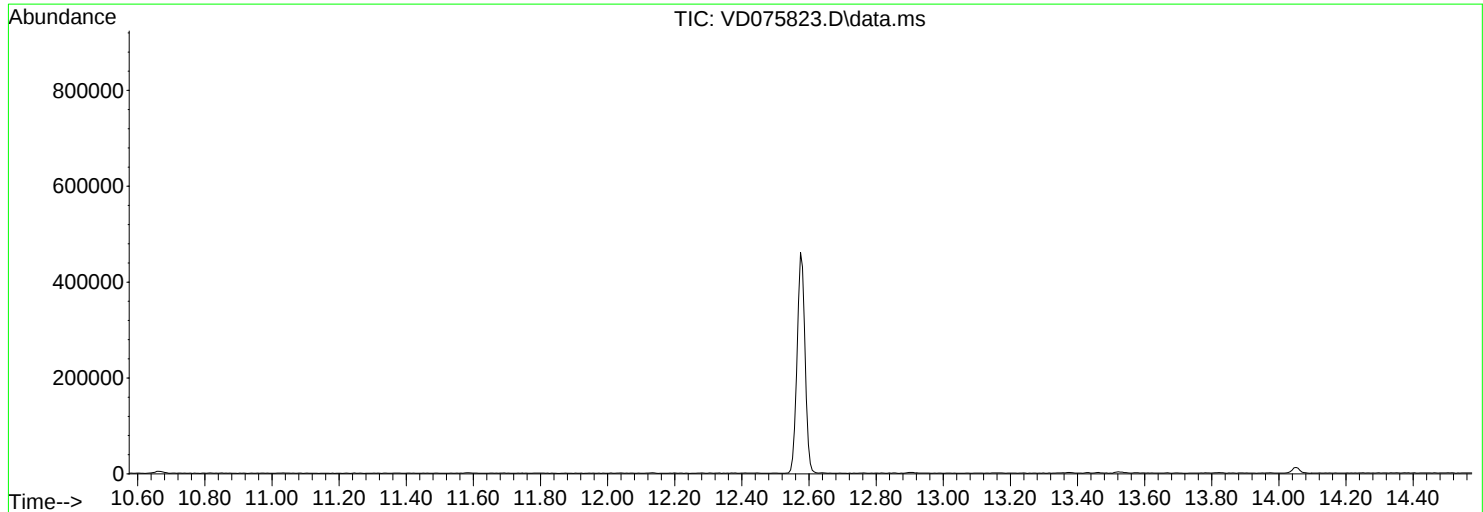

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	13173	PASS
75	95	30	80	47.4	37376	PASS
95	95	100	100	100.0	78931	PASS
96	95	5	9	6.8	5397	PASS
173	174	0.00	2	1.0	767	PASS
174	95	50	120	96.0	75752	PASS
175	174	5	9	7.1	5403	PASS
176	174	95	105	95.3	72224	PASS
177	176	5	10	7.0	5038	PASS

Scan 1860 (12.527 min): VD075823.D\data.ms
BFB119

m/z	Abundance
40.00	641.0
43.90	668.0

Instrument :
MSVOA_D
ClientSampleId :
BFB119

m/z	Abundance
36.00	352.0
37.00	2667.0
38.00	2425.0
39.00	896.0
39.90	820.0
44.00	737.0
45.00	502.0
47.10	689.0
48.10	374.0
49.20	1824.0
50.00	10589.0
51.10	3483.0
55.10	268.0
56.10	1148.0
57.00	1749.0
58.90	161.0
60.00	535.0
61.00	2950.0
62.10	3065.0
63.10	3050.0
64.00	516.0
65.00	535.0
66.00	161.0
66.80	181.0
68.10	6585.0
69.00	7405.0
70.00	347.0
72.10	350.0
73.10	3450.0
74.10	11107.0
75.10	33336.0
76.10	2711.0
76.90	497.0
78.90	3031.0
79.90	759.0
81.00	3136.0
82.00	637.0
87.00	3902.0
87.90	3907.0
90.70	278.0
92.10	2118.0
93.00	2847.0
94.10	8433.0
95.10	68024.0
96.00	4461.0
97.00	248.0
103.10	163.0
103.90	563.0
104.80	166.0
105.90	222.0
115.80	178.0
116.90	801.0
117.90	426.0
118.90	646.0
125.20	190.0
125.80	175.0
127.70	287.0
129.90	380.0
130.90	171.0
132.80	331.0
134.80	249.0
141.00	654.0
142.90	985.0
144.90	665.0
147.10	177.0
147.80	311.0
155.00	216.0
170.90	162.0
171.90	504.0
173.00	947.0
174.00	63704.0
175.00	4471.0
176.00	61328.0
177.00	4257.0
190.70	181.0
191.20	214.0
193.00	394.0
206.90	358.0
249.00	336.0
265.30	338.0
281.00	2323.0
282.10	786.0
283.00	606.0

Instrument :
MSVOA_D
ClientSampleId :
BFB119

m/z	Abundance
35.90	635.0
37.10	2881.0
38.20	2998.0
39.00	1163.0
40.00	839.0
43.90	844.0
45.10	667.0
47.10	943.0
47.90	446.0
49.10	2975.0
50.10	14567.0
51.10	4092.0
52.10	214.0
55.10	238.0
56.00	1414.0
57.00	2454.0
57.90	229.0
60.00	670.0
61.00	4206.0
62.00	4019.0
63.10	2992.0
64.00	481.0
65.10	427.0
67.10	350.0
68.00	8939.0
69.10	8693.0
70.00	1114.0
72.10	412.0
73.00	4512.0
74.10	15023.0
75.00	41776.0
76.10	3625.0
77.00	611.0
77.90	447.0
78.90	3717.0
80.00	886.0
80.90	3836.0
81.90	987.0
86.90	4359.0
87.90	4484.0
91.00	552.0
92.00	2743.0
93.10	3587.0
94.10	10219.0
95.10	89616.0
96.10	6680.0
104.00	327.0
104.70	168.0
105.90	292.0
114.90	300.0
115.80	356.0
116.90	992.0
118.10	278.0
118.90	723.0
125.10	293.0
125.80	180.0
128.00	393.0
129.80	260.0
133.10	810.0
134.70	221.0
137.00	207.0
140.10	161.0
140.90	893.0
142.90	847.0
145.10	479.0
148.00	254.0
154.70	208.0
157.00	161.0
171.00	221.0
171.90	759.0
172.80	809.0
174.00	83888.0
175.00	6397.0
176.00	77944.0
177.00	6126.0
178.00	245.0
178.90	231.0
191.00	354.0
192.90	682.0
194.10	250.0
207.00	534.0
249.10	295.0
251.10	236.0
264.90	257.0
265.20	220.0
281.20	4097.0
282.20	970.0
283.00	691.0

Instrument :
MSVOA_D
ClientSampleId :
BFB119

m/z	Abundance
36.10	603.0
37.10	2400.0
38.10	2407.0
39.10	974.0
39.90	828.0
44.00	997.0
45.10	625.0
47.10	783.0
47.90	438.0
49.00	3082.0
50.00	14364.0
51.10	4438.0
52.10	169.0
55.00	252.0
56.00	1087.0
57.10	2186.0
59.90	760.0
61.00	4001.0
62.00	3855.0
63.00	3101.0
64.00	468.0
65.00	474.0
67.00	251.0
68.00	7317.0
69.00	8113.0
70.00	621.0
71.90	421.0
73.10	4215.0
74.10	13986.0
75.10	37016.0
76.00	3307.0
77.00	640.0
78.00	359.0
79.00	3575.0
80.00	747.0
81.00	3433.0
82.00	850.0
87.00	4642.0
88.00	3973.0
90.90	373.0
92.00	2552.0
93.00	3360.0
94.00	9888.0
95.10	79152.0
96.00	5051.0
103.00	249.0
103.90	629.0
105.90	502.0
106.90	174.0
114.90	168.0
115.90	359.0
117.10	659.0
118.00	291.0
118.90	458.0
124.70	216.0
125.10	436.0
127.80	292.0
128.80	151.0
130.00	156.0
130.90	207.0
132.90	645.0
134.00	292.0
134.80	290.0
136.90	156.0
140.80	540.0
141.90	245.0
143.00	1406.0
144.80	268.0
147.00	174.0
147.90	355.0
159.10	170.0
170.80	262.0
171.90	802.0
172.70	545.0
173.10	449.0
174.00	79664.0
175.00	5342.0
176.00	77400.0
177.00	4730.0
178.10	189.0
191.00	514.0
193.00	804.0
194.00	151.0
207.10	505.0
249.00	405.0
265.10	453.0
281.10	5269.0
282.10	1248.0
283.10	1073.0
284.20	195.0

Instrument :
MSVOA_D
ClientSampleId :
BFB119