
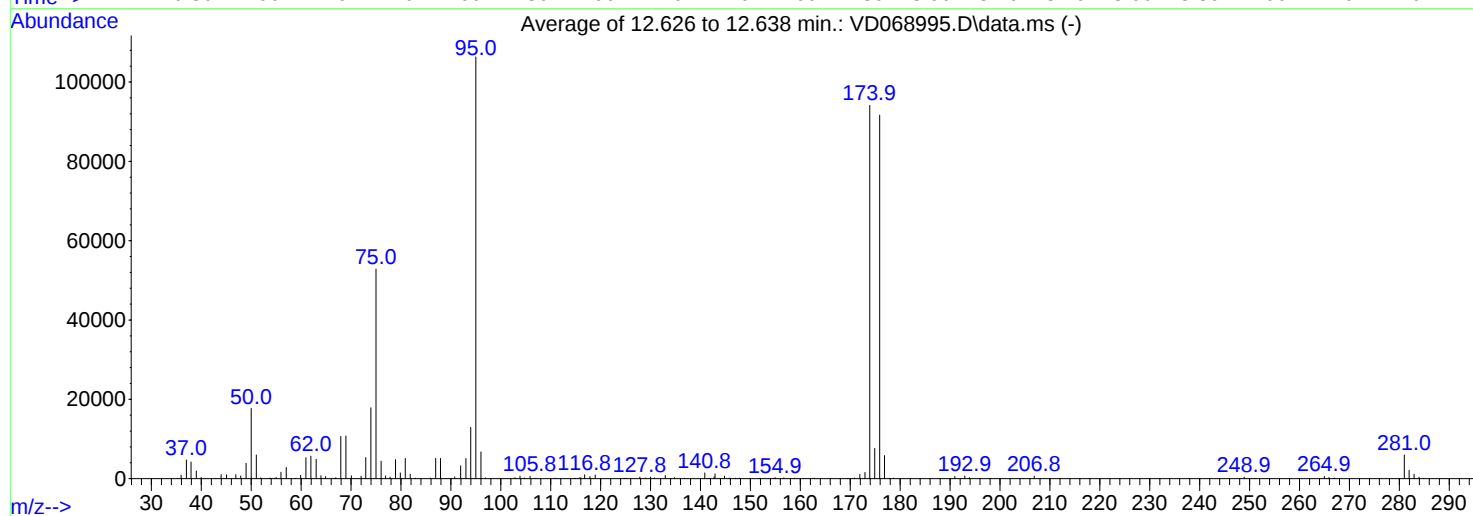


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042821\
Data File : VD068995.D
Acq On : 28 Apr 2021 09:14
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D040721S.M
Title : SW846 8260
Last Update : Thu Apr 08 03:50:31 2021

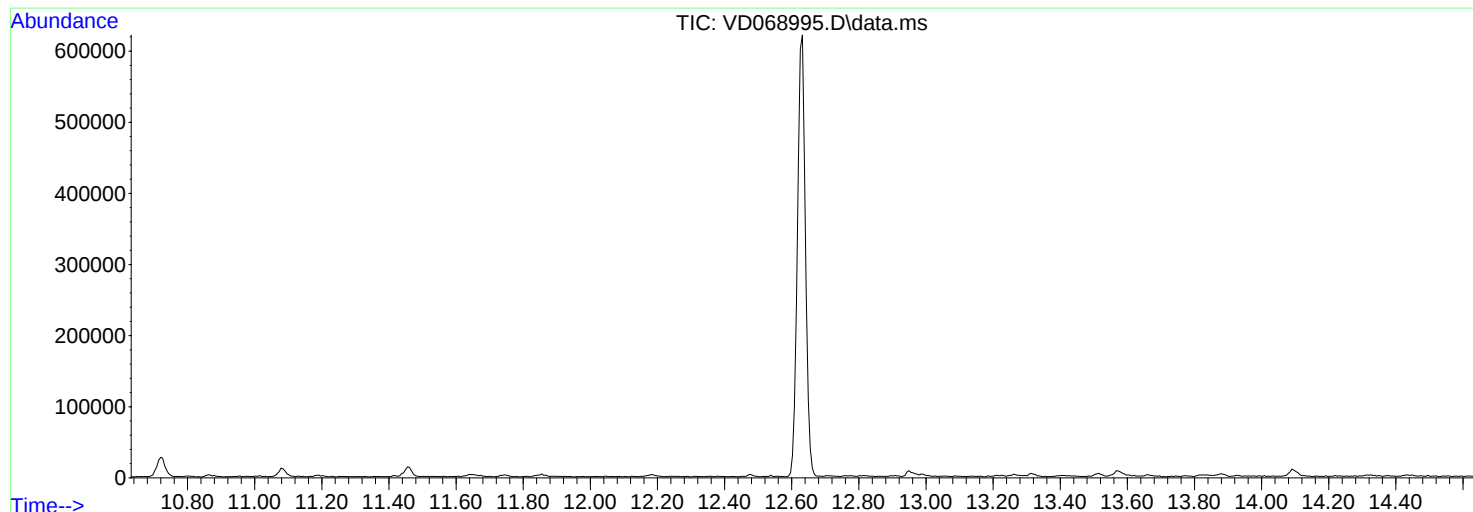

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	17704	PASS
75	95	30	60	49.7	52851	PASS
95	95	100	100	100.0	106352	PASS
96	95	5	9	6.3	6749	PASS
173	174	0.00	2	1.7	1556	PASS
174	95	50	100	88.5	94141	PASS
175	174	5	9	8.1	7625	PASS
176	174	95	101	97.4	91659	PASS
177	176	5	9	6.4	5824	PASS