




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042823\
Data File : VD075895.D
Acq On : 28 Apr 2023 18:59
Operator : KP/SY
Sample : 02548-25
Misc : 5.82G/10.00ml/MSVOA_D/SOIL
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
DCCQ5

Manual IntegrationsAPPROVED

Quant Time: Apr 29 05:14:15 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Apr 29 05:12:16 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 04/29/2023
Supervised By :Semsettin Yesilyurt 05/01/2023

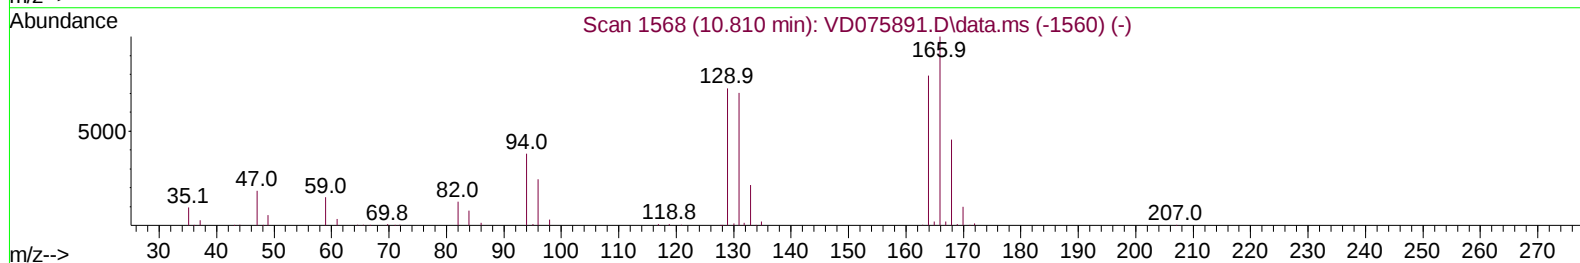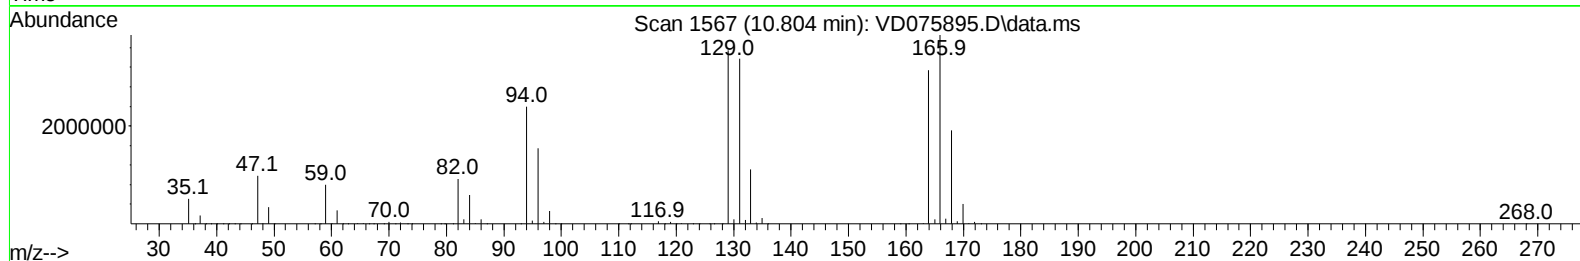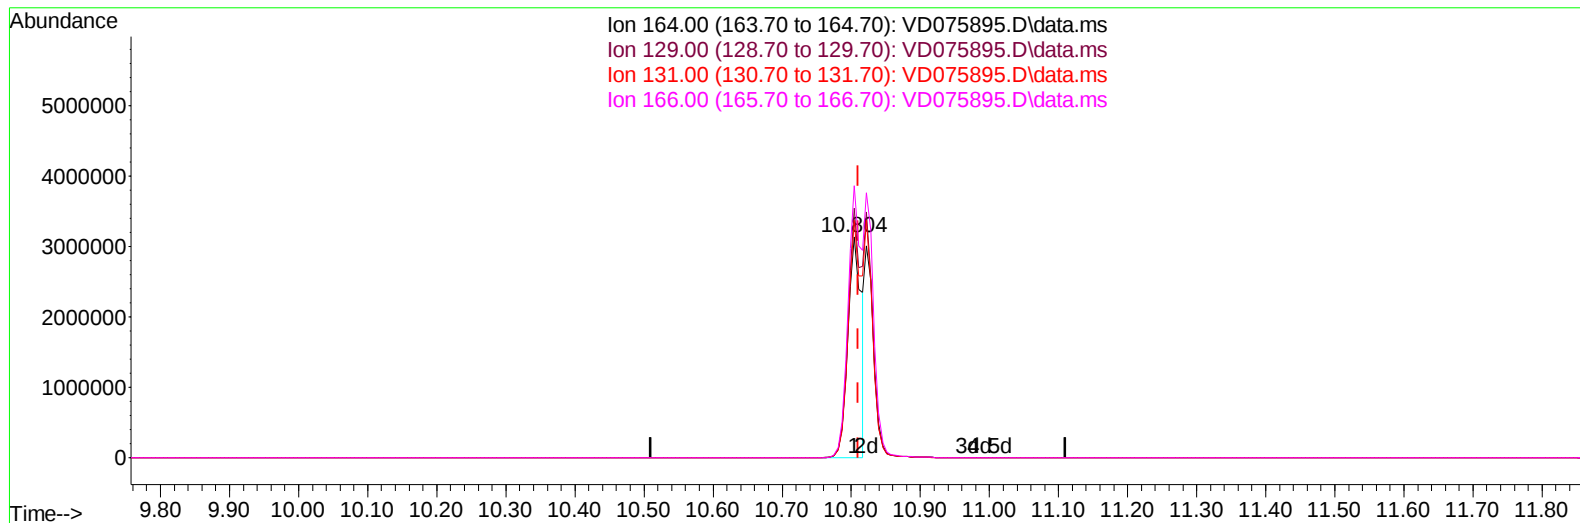

TIC: VD075895.D\data.ms

(46) Tetrachloroethene (T)

10.804min (-0.006) 621.81 ug/L

response 4240505

Ion	Exp%	Act%
164.00	100.00	100.00
129.00	86.20	113.02#
131.00	84.10	107.60
166.00	118.50	123.08




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042823\
 Data File : VD075895.D
 Acq On : 28 Apr 2023 18:59
 Operator : KP/SY
 Sample : 02548-25
 Misc : 5.82G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DCCQ5

Manual IntegrationsAPPROVED

Quant Time: Apr 29 05:14:15 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 29 05:12:16 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/29/2023
 Supervised By :Semsettin Yesilyurt 05/01/2023

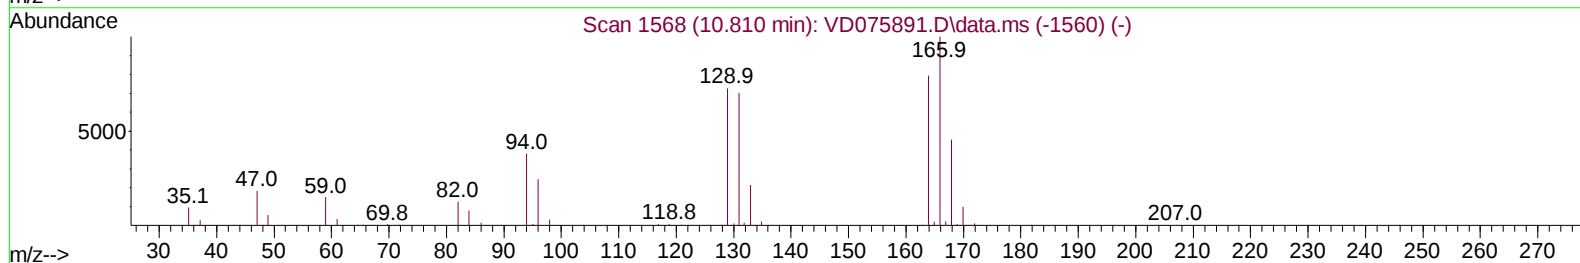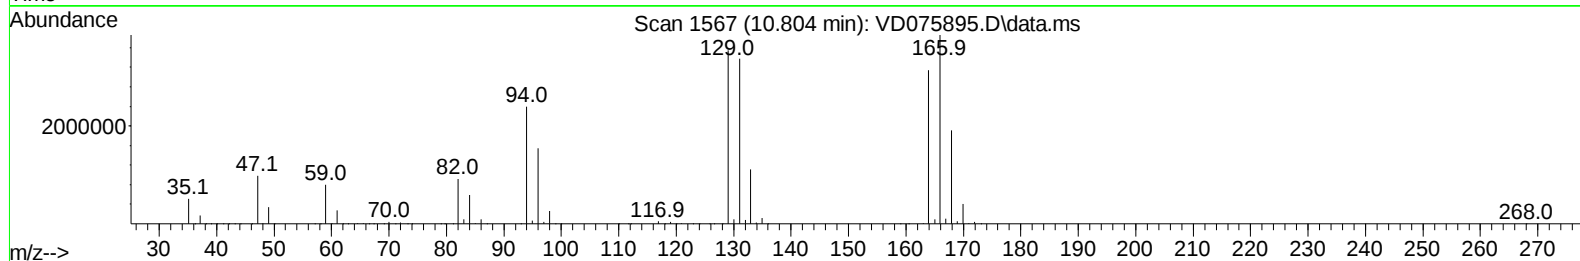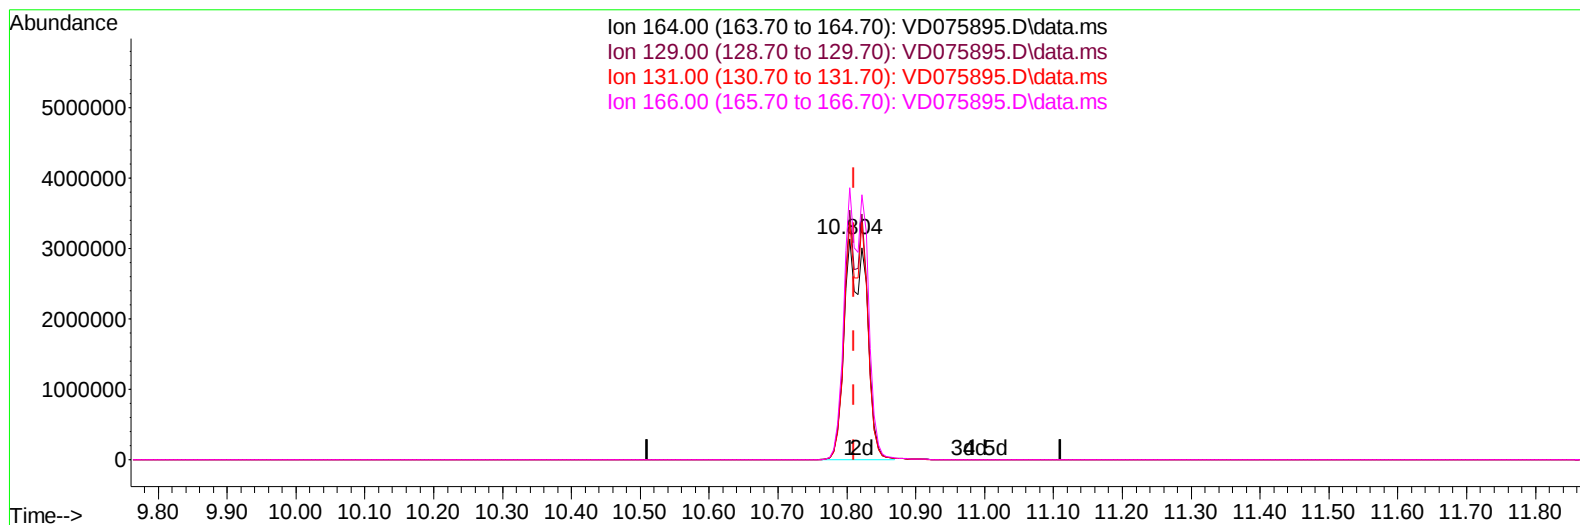

TIC: VD075895.D\data.ms

(46) Tetrachloroethene (T)

10.804min (-0.006) 1010.72 ug/L m

response 6892662

Ion	Exp%	Act%
164.00	100.00	100.00
129.00	86.20	113.02#
131.00	84.10	107.60
166.00	118.50	123.08

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042823\
 Data File : VD075895.D
 Acq On : 28 Apr 2023 18:59
 Operator : KP/SY
 Sample : 02548-25
 Misc : 5.82G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DCCQ5

Manual IntegrationsAPPROVED

Quant Time: Apr 29 05:14:15 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 29 05:12:16 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/29/2023
 Supervised By :Semsettin Yesilyurt 05/01/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.775	114		592183	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117		531520	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.522	152		242135	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.269	65		195228	15.028	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	60.120%		
7) Chloroethane-d5	2.799	69		189222	16.858	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	67.440%		
11) 1,1-Dichloroethene-d2	3.911	65		48408	16.163	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	64.640%		
21) 2-Butanone-d5	6.987	46		62691	55.588	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	111.180%		
24) Chloroform-d	7.569	84		289961	19.581	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	78.320%		
26) 1,2-Dichloroethane-d4	8.228	65		126636	20.025	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	80.120%		
32) Benzene-d6	8.199	84		555143	17.920	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	71.680%		
36) 1,2-Dichloropropane-d6	9.210	67		174814	20.387	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	81.560%		
41) Toluene-d8	10.269	98		511487	17.636	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	70.560%		
43) trans-1,3-Dichloroprop...	10.528	79		67440	19.028	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	76.120%		
47) 2-Hexanone-d5	10.875	63		59361	57.495	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	114.980%		
56) 1,1,2,2-Tetrachloroeth...	12.651	84		154683	23.574	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	94.280%		
66) 1,2-Dichlorobenzene-d4	13.816	152		162745	19.002	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	76.000%		
Target Compounds							
						Qvalue	
13) Acetone	4.016	43		1479561	1533.035	ug/L	98
16) Methylene chloride	4.799	84		22615	1.883	ug/L	93
20) cis-1,2-Dichloroethene	7.081	96		52557	5.693	ug/L	94
22) 2-Butanone	7.081	43		144253	114.649	ug/L	93
34) Trichloroethene	9.028	95		45158	5.431	ug/L	96
40) 4-Methyl-2-pentanone	10.157	43		3974	1.476	ug/L #	89
42) Toluene	10.334	91		10400	0.299	ug/L	91
46) Tetrachloroethene	10.804	164		6892662m	1010.715	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042823\
Data File : VD075895.D
Acq On : 28 Apr 2023 18:59
Operator : KP/SY
Sample : 02548-25
Misc : 5.82G/10.00ml/MSVOA_D/soil
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
DCCQ5

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/29/2023
Supervised By :Semsettin Yesilyurt 05/01/2023

Quant Time: Apr 29 05:14:15 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Apr 29 05:12:16 2023
Response via : Initial Calibration

