




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042823\
Data File : VD075901.D
Acq On : 28 Apr 2023 21:55
Operator : KP/SY
Sample : 02548-31
Misc : 6.20G/10.00mL/MSVOA_D/SOIL
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
DCCR1

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/29/2023
Supervised By :Semsettin Yesilyurt 05/01/2023

Quant Time: Apr 29 05:15:40 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Apr 29 05:12:16 2023
Response via : Initial Calibration

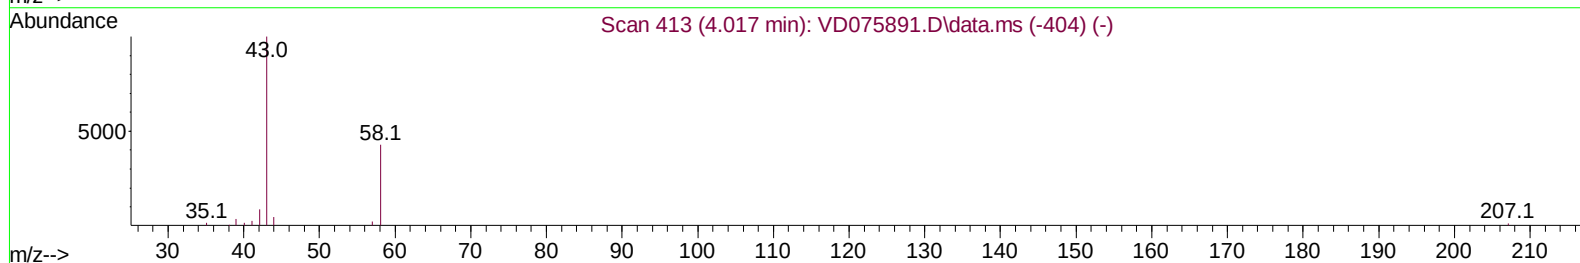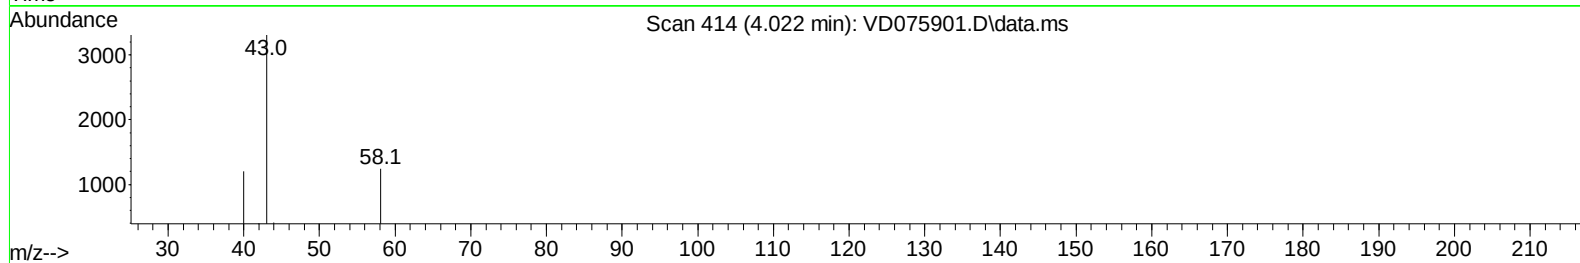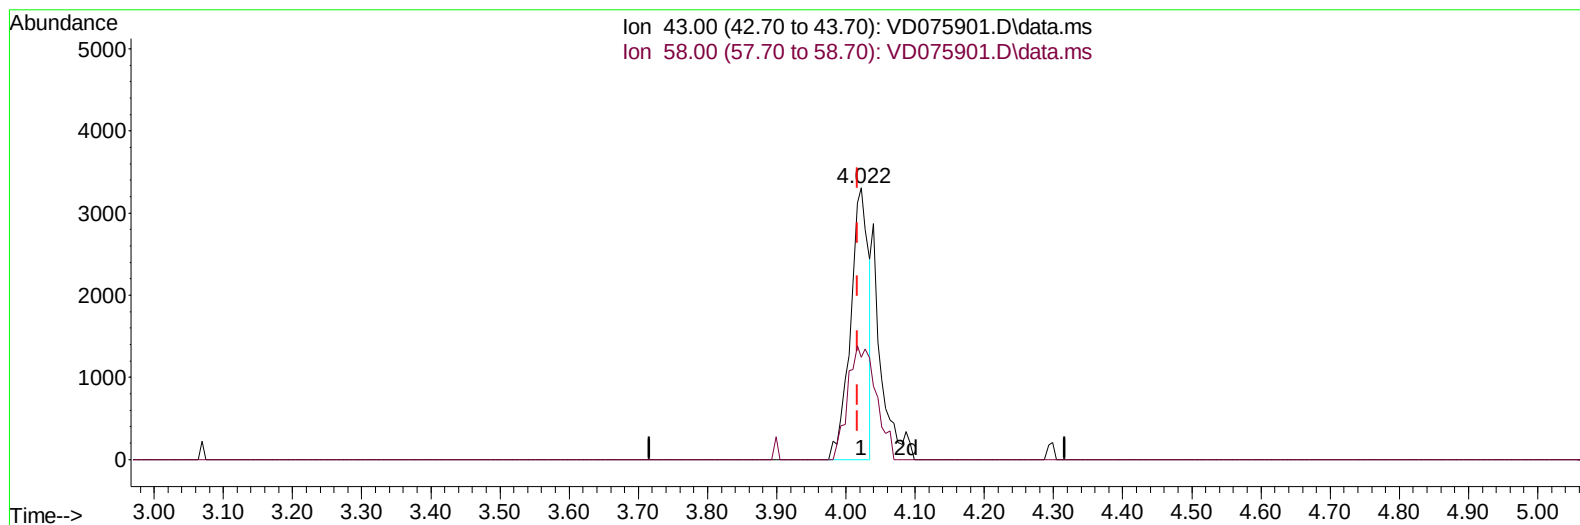

TIC: VD075901.D\data.ms

(13) Acetone (T)

4.022min (+ 0.006) 7.91 ug/L

response 5984

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	43.70	34.29
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042823\
 Data File : VD075901.D
 Acq On : 28 Apr 2023 21:55
 Operator : KP/SY
 Sample : 02548-31
 Misc : 6.20G/10.00mL/MSVOA_D/SOIL
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DCCR1

Manual IntegrationsAPPROVED

Quant Time: Apr 29 05:15:40 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 29 05:12:16 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/29/2023
 Supervised By :Semsettin Yesilyurt 05/01/2023

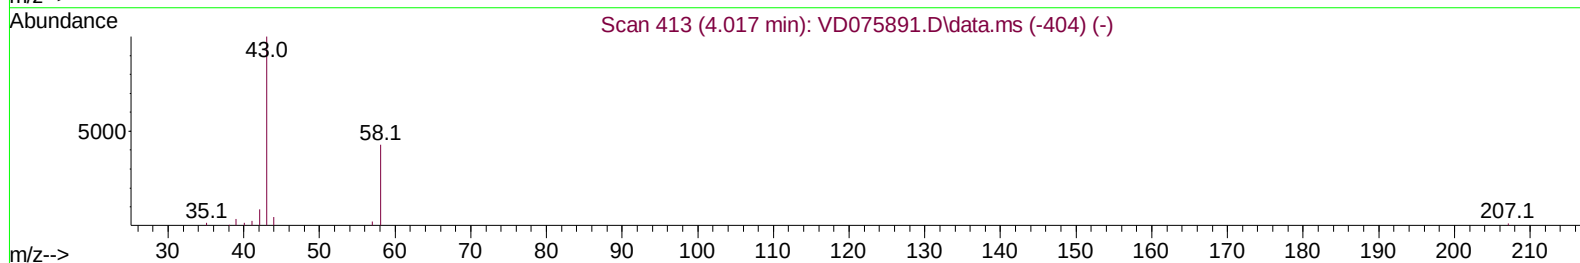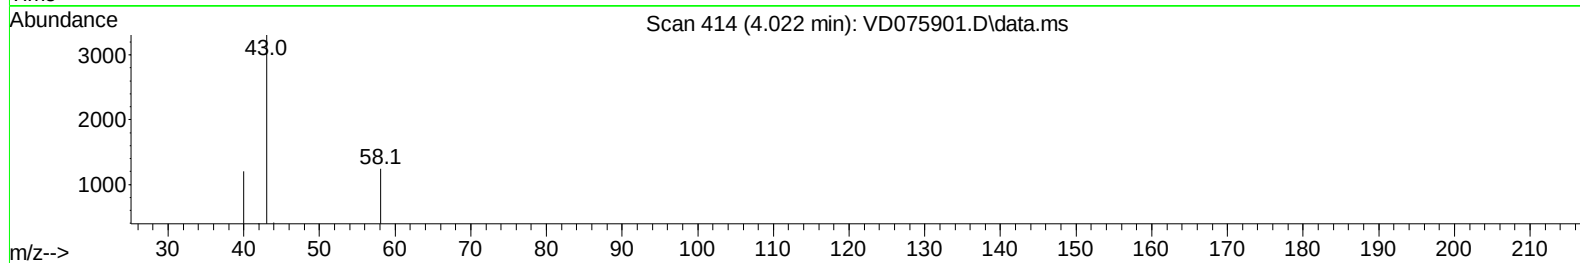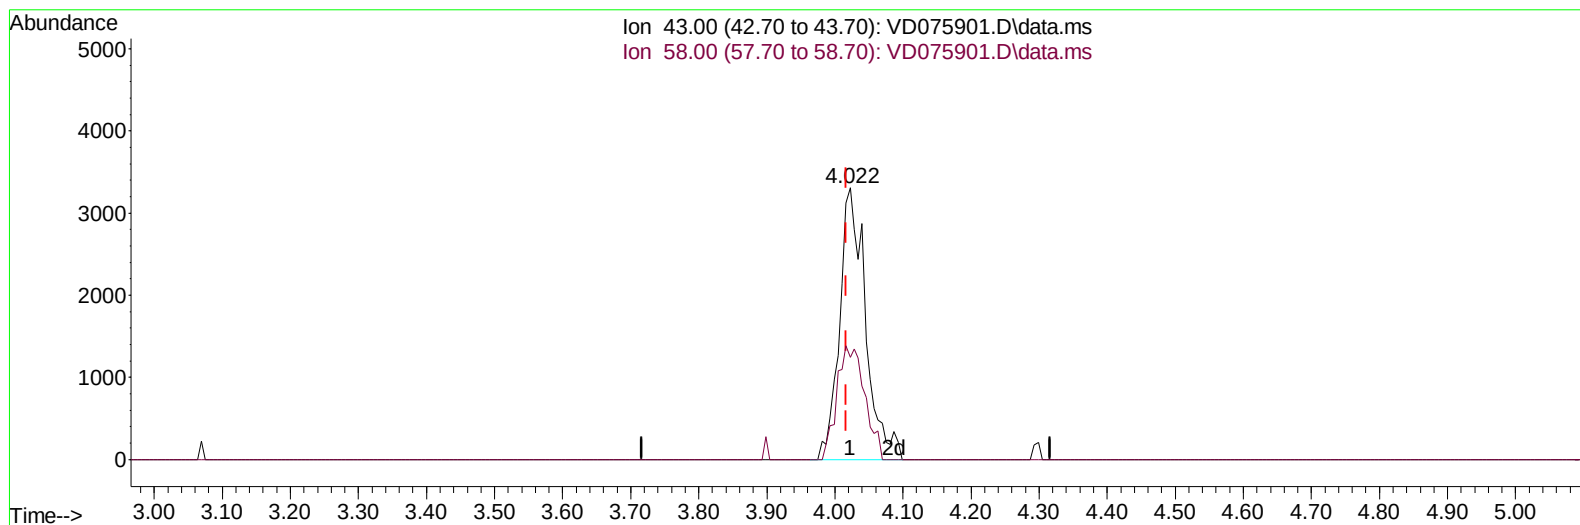

TIC: VD075901.D\data.ms

(13) Acetone (T)

4.022min (+ 0.006) 11.53 ug/L m

response 8721

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	43.70	23.53
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042823\
 Data File : VD075901.D
 Acq On : 28 Apr 2023 21:55
 Operator : KP/SY
 Sample : 02548-31
 Misc : 6.20G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DCCR1

Manual IntegrationsAPPROVED

Quant Time: Apr 29 05:15:40 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 29 05:12:16 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/29/2023
 Supervised By :Semsettin Yesilyurt 05/01/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.775	114		464117	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117		479821	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.522	152		217060	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.275	65		167143	16.416	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	65.680%	
7) Chloroethane-d5	2.799	69		165079	18.765	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	75.080%	
11) 1,1-Dichloroethene-d2	3.916	65		39492	16.824	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	67.280%	
21) 2-Butanone-d5	6.987	46		55791	63.120	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	126.240%	
24) Chloroform-d	7.569	84		260423	22.439	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	89.760%	
26) 1,2-Dichloroethane-d4	8.228	65		119388	24.088	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	96.360%	
32) Benzene-d6	8.198	84		495528	17.719	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	70.880%	
36) 1,2-Dichloropropane-d6	9.210	67		161736	20.894	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	83.560%	
41) Toluene-d8	10.269	98		443924	16.955	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	67.840%	
43) trans-1,3-Dichloroprop...	10.522	79		62788	19.624	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	78.480%	
47) 2-Hexanone-d5	10.875	63		44647	47.903	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	95.800%	
56) 1,1,2,2-Tetrachloroeth...	12.651	84		149546	25.247	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	101.000%	
66) 1,2-Dichlorobenzene-d4	13.816	152		173137	22.551	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	90.200%	
Target Compounds							
13) Acetone	4.022	43		8721m	11.530	ug/L	
16) Methylene chloride	4.799	84		18555	1.971	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042823\
Data File : VD075901.D
Acq On : 28 Apr 2023 21:55
Operator : KP/SY
Sample : 02548-31
Misc : 6.20G/10.00mL/MSVOA_D/SOIL
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
DCCR1

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/29/2023
Supervised By :Semsettin Yesilyurt 05/01/2023

Quant Time: Apr 29 05:15:40 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Apr 29 05:12:16 2023
Response via : Initial Calibration

