




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042823\
 Data File : VD075902.D
 Acq On : 28 Apr 2023 22:24
 Operator : KP/SY
 Sample : 02548-32
 Misc : 4.23G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DCCR2

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/29/2023
 Supervised By :Semsettin Yesilyurt 05/01/2023

Quant Time: Apr 29 05:15:53 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 29 05:12:16 2023
 Response via : Initial Calibration

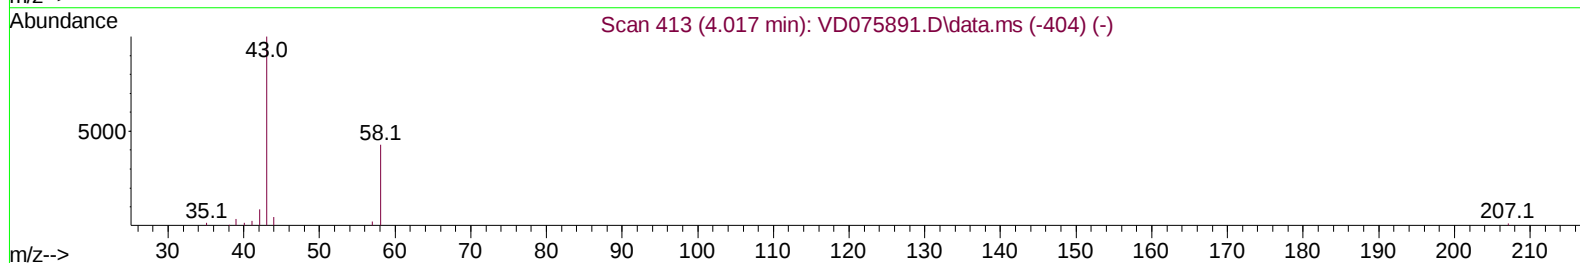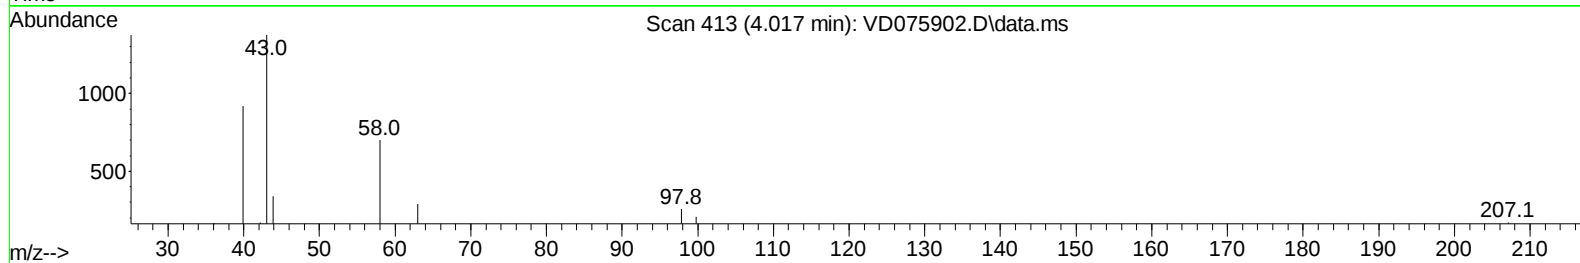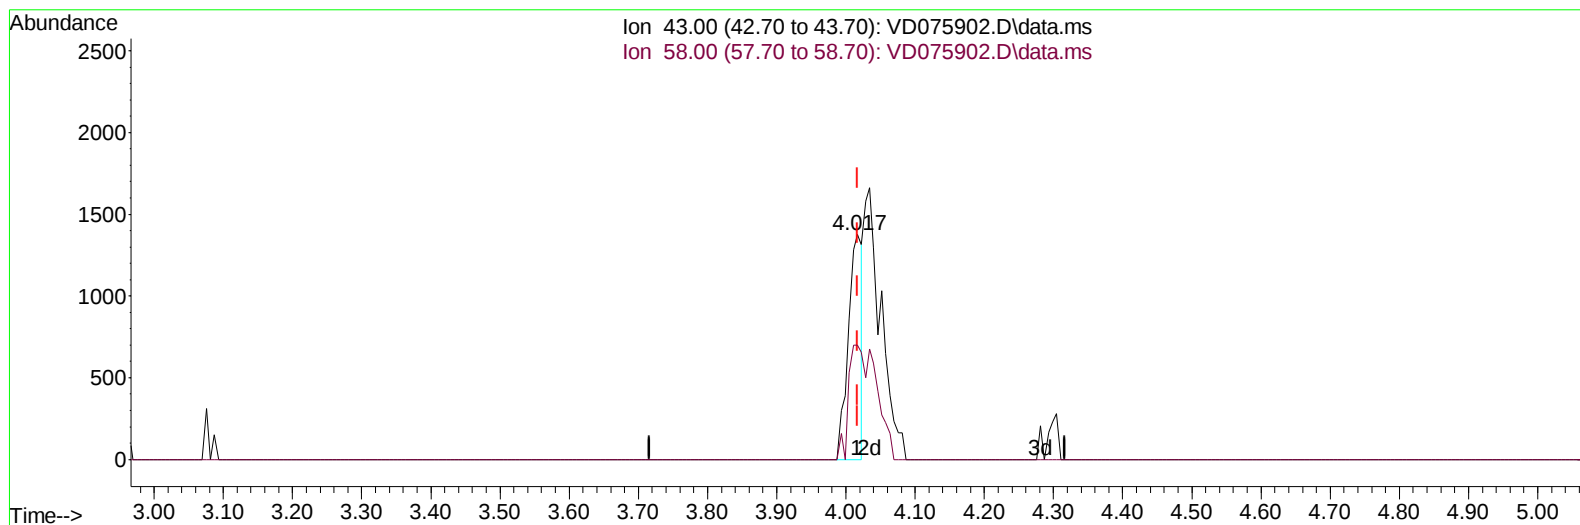

TIC: VD075902.D\data.ms

(13) Acetone (T)

4.017min (-0.000) 2.09 ug/L

response 1950

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	43.70	55.85
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042823\
 Data File : VD075902.D
 Acq On : 28 Apr 2023 22:24
 Operator : KP/SY
 Sample : 02548-32
 Misc : 4.23G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DCCR2

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/29/2023
 Supervised By :Semsettin Yesilyurt 05/01/2023

Quant Time: Apr 29 05:15:53 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 29 05:12:16 2023
 Response via : Initial Calibration

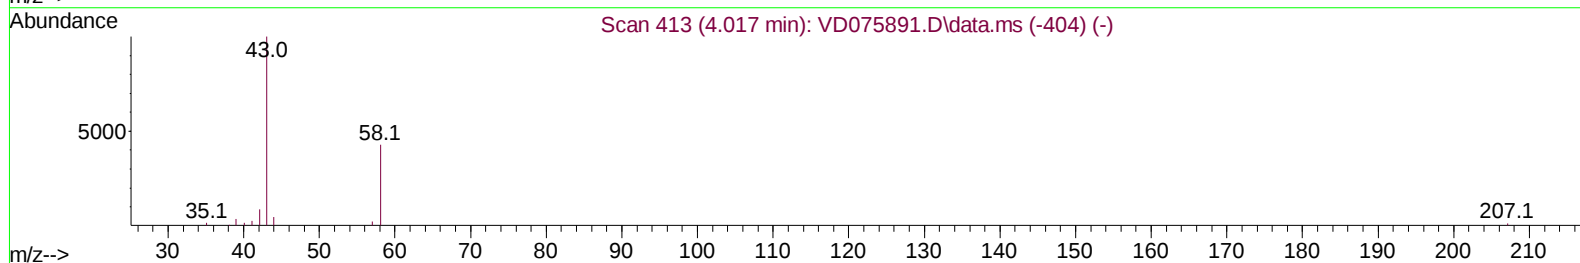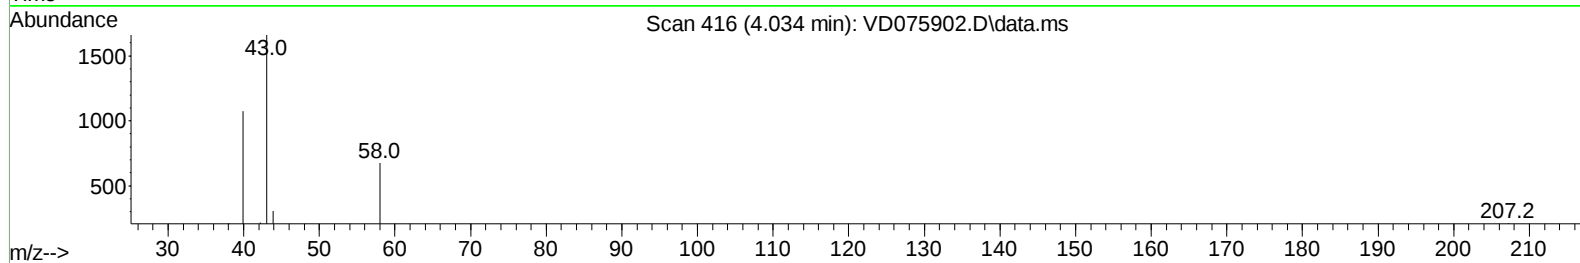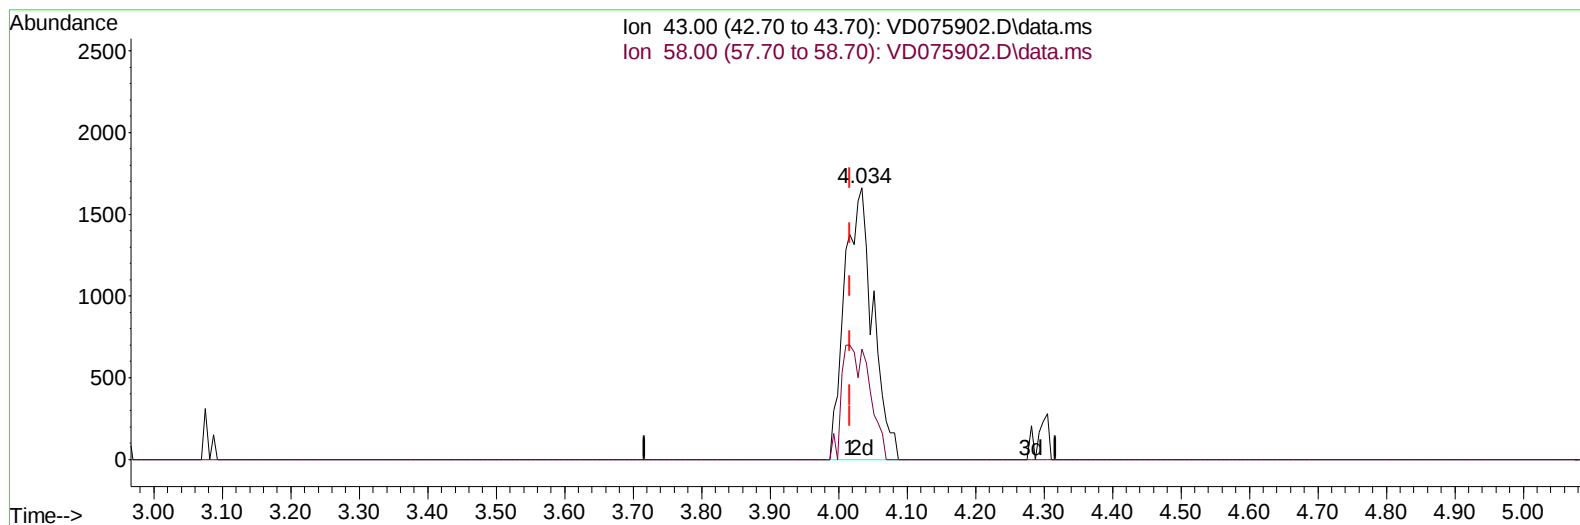

TIC: VD075902.D\data.ms

(13) Acetone (T)

4.034min (+ 0.018) 5.08 ug/L m

response 4750

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	43.70	22.93
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042823\
 Data File : VD075902.D
 Acq On : 28 Apr 2023 22:24
 Operator : KP/SY
 Sample : 02548-32
 Misc : 4.23G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DCCR2

Manual IntegrationsAPPROVED

Quant Time: Apr 29 05:15:53 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 29 05:12:16 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/29/2023
 Supervised By :Semsettin Yesilyurt 05/01/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.781	114		573426	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117		572007	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.522	152		260199	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.275	65		206538	16.419	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	65.680%	
7) Chloroethane-d5	2.799	69		201971	18.582	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	74.320%	
11) 1,1-Dichloroethene-d2	3.922	65		50725	17.490	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	69.960%	
21) 2-Butanone-d5	6.987	46		63614	58.252	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	116.500%	
24) Chloroform-d	7.569	84		321680	22.433	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	89.720%	
26) 1,2-Dichloroethane-d4	8.228	65		140131	22.884	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	91.520%	
32) Benzene-d6	8.199	84		617345	18.517	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	74.080%	
36) 1,2-Dichloropropane-d6	9.210	67		197694	21.423	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	85.680%	
41) Toluene-d8	10.269	98		563185	18.044	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	72.160%	
43) trans-1,3-Dichloroprop...	10.528	79		75994	19.924	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	79.680%	
47) 2-Hexanone-d5	10.881	63		55384	49.846	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	99.700%	
56) 1,1,2,2-Tetrachloroeth...	12.651	84		172491	24.427	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	97.720%	
66) 1,2-Dichlorobenzene-d4	13.816	152		207684	22.566	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	90.280%	
Target Compounds							
13) Acetone	4.034	43		4750m	5.083	ug/L	
16) Methylene chloride	4.799	84		22558	1.939	ug/L	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042823\
Data File : VD075902.D
Acq On : 28 Apr 2023 22:24
Operator : KP/SY
Sample : 02548-32
Misc : 4.23G/10.00ml/MSVOA_D/SOIL
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
DCCR2

Manual IntegrationsAPPROVED

Quant Time: Apr 29 05:15:53 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Apr 29 05:12:16 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 04/29/2023
Supervised By :Semsettin Yesilyurt 05/01/2023

