

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042823\
 Data File : VD075881.D
 Acq On : 28 Apr 2023 11:56
 Operator : KP/SY
 Sample : 02525-03
 Misc : 5.81G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DCCC3

Quant Time: Apr 29 02:57:32 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 29 02:40:46 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.775	114	427608	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117	428621	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.516	152	193281	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.269	65	153616	16.376	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	65.520%		
7) Chloroethane-d5	2.799	69	141305	17.434	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	69.720%		
11) 1,1-Dichloroethene-d2	3.911	65	36349	16.807	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	67.240%		
21) 2-Butanone-d5	6.987	46	45048	55.317	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	110.640%		
24) Chloroform-d	7.563	84	207873	19.440	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	77.760%		
26) 1,2-Dichloroethane-d4	8.228	65	95292	20.868	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	83.480%		
32) Benzene-d6	8.199	84	403013	16.132	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	64.520%		
36) 1,2-Dichloropropane-d6	9.210	67	127151	18.388	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	73.560%		
41) Toluene-d8	10.269	98	364042	15.565	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	62.280%		
43) trans-1,3-Dichloroprop...	10.528	79	50849	17.791	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	71.160%		
47) 2-Hexanone-d5	10.875	63	39392	47.313	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	94.620%		
56) 1,1,2,2-Tetrachloroeth...	12.651	84	129649	24.502	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	98.000%		
66) 1,2-Dichlorobenzene-d4	13.816	152	139123	20.350	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	81.400%		
Target Compounds					Qvalue	
13) Acetone	4.022	43	49253	70.674	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042823\
Data File : VD075881.D
Acq On : 28 Apr 2023 11:56
Operator : KP/SY
Sample : 02525-03
Misc : 5.81G/10.00ml/MSVOA_D/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
DCCC3

Quant Time: Apr 29 02:57:32 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Apr 29 02:40:46 2023
Response via : Initial Calibration

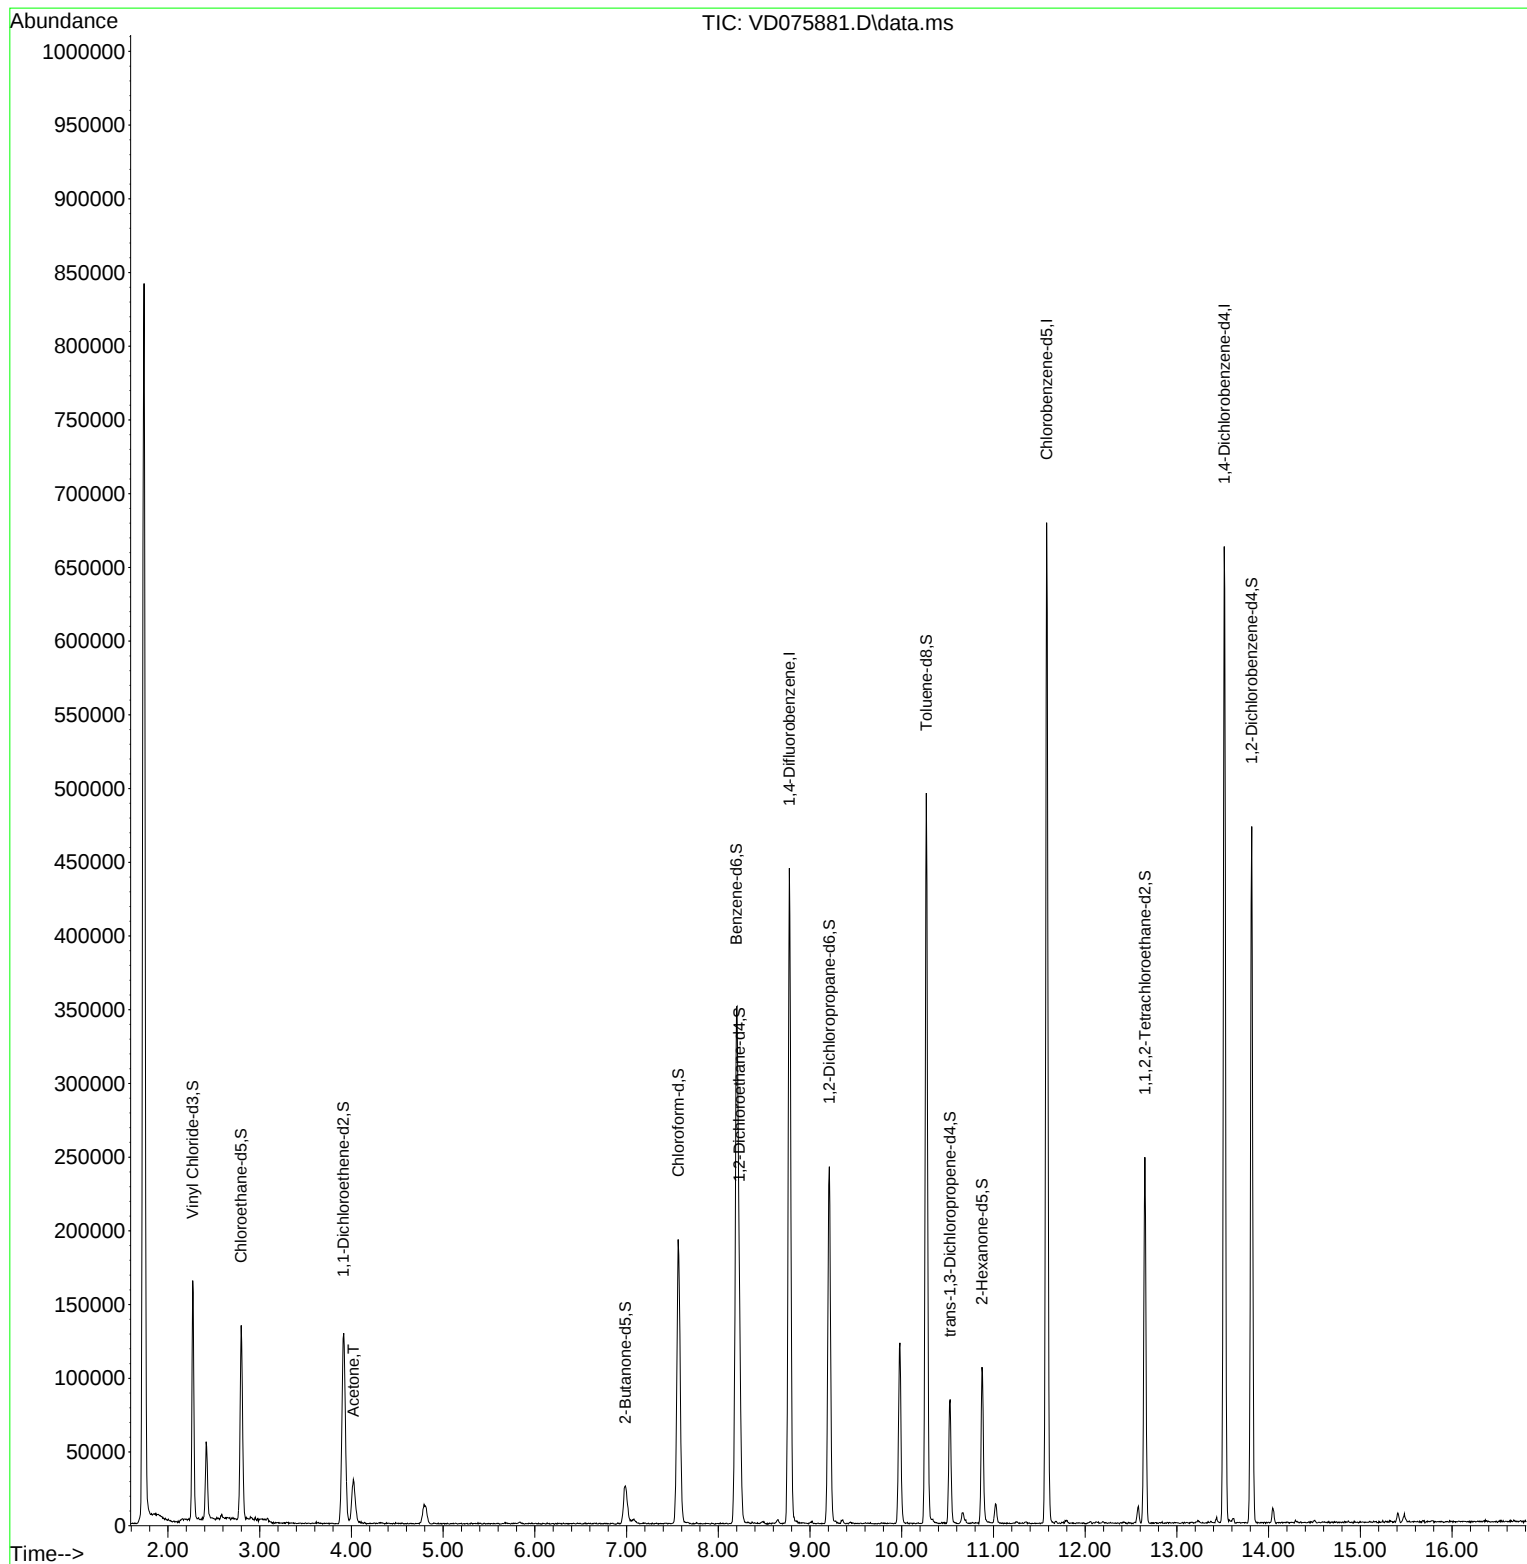

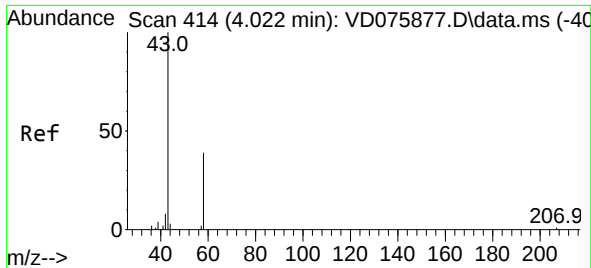

#13
 Acetone
 Concen: 70.674 ug/L
 RT: 4.022 min Scan# 41
 Delta R.T. -0.000 min
 Lab File: VD075881.D
 Acq: 28 Apr 2023 11:56

Instrument :
 MSVOA_D
 ClientSampleId :
 DCCC3

Tgt Ion: 43 Resp: 49253
 Ion Ratio Lower Upper
 43 100
 58 41.3 0.0 87.4

