
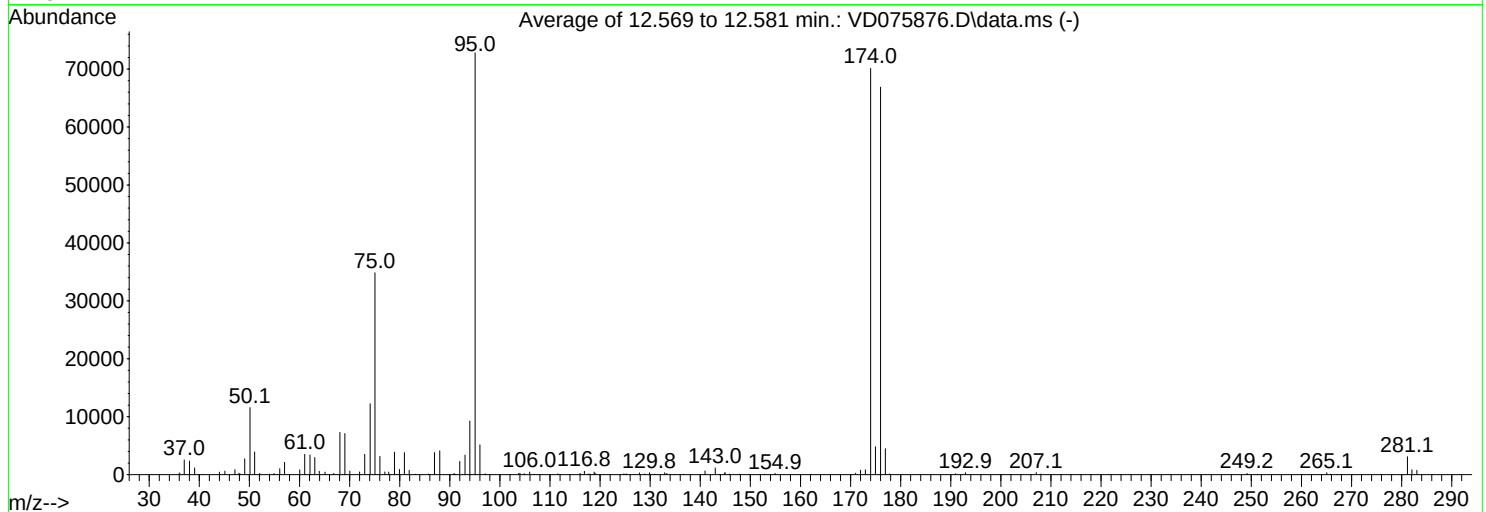


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042823\
Data File : VD075876.D
Acq On : 28 Apr 2023 09:17
Operator : KP/SY
Sample : BFB121
Misc : 5.00G/10.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB121

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Title : SFAM01.0
Last Update : Mon May 01 00:14:49 2023

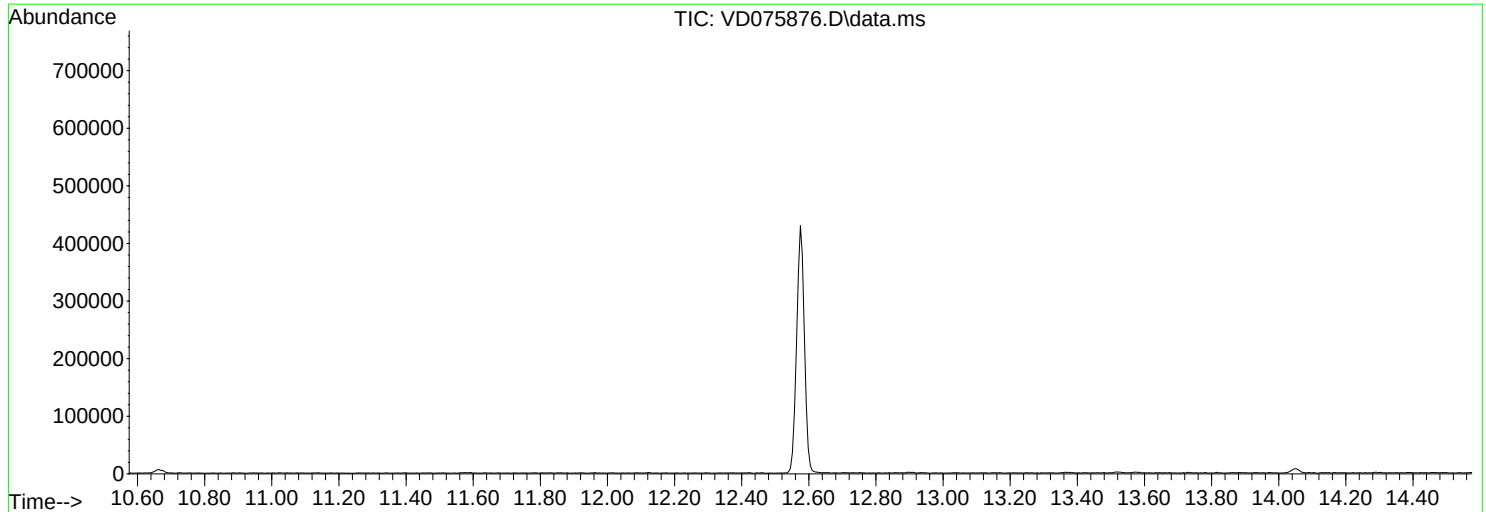

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	11577	PASS
75	95	30	80	47.9	34861	PASS
95	95	100	100	100.0	72805	PASS
96	95	5	9	7.1	5140	PASS
173	174	0.00	2	1.2	829	PASS
174	95	50	120	96.3	70120	PASS
175	174	5	9	6.9	4819	PASS
176	174	95	105	95.4	66901	PASS
177	176	5	10	6.7	4486	PASS

Scan 1860 (12.528 min): VD075876.D\data.ms
BFB121

m/z	Abundance
40.00	1230.0
43.90	358.0

Instrument :
MSVOA_D
ClientSampleId :
BFB121

m/z	Abundance
36.00	392.0
37.00	2209.0
38.00	2047.0
39.00	921.0
40.10	1090.0
40.70	170.0
44.10	751.0
45.10	574.0
47.10	936.0
47.90	366.0
49.10	2446.0
50.10	11365.0
51.00	3770.0
52.00	218.0
55.00	281.0
56.10	1043.0
57.00	1880.0
60.00	799.0
61.10	3330.0
62.10	2965.0
63.10	3141.0
64.00	557.0
65.20	371.0
66.80	193.0
68.00	6735.0
69.00	7068.0
70.00	632.0
72.00	468.0
73.00	3203.0
74.10	11557.0
75.10	31872.0
76.00	2991.0
77.00	207.0
77.80	251.0
78.90	3578.0
79.90	890.0
81.00	3482.0
82.00	475.0
87.00	3449.0
88.00	3526.0
90.80	368.0
92.00	2002.0
93.00	3130.0
94.00	8617.0
95.00	68080.0
96.00	5241.0
104.00	387.0
104.90	165.0
106.00	446.0
106.80	171.0
111.60	190.0
116.80	637.0
117.60	264.0
118.80	623.0
127.90	236.0
129.00	170.0
129.90	329.0
132.90	500.0
134.90	199.0
141.00	514.0
143.00	1020.0
144.80	553.0
152.90	173.0
154.90	185.0
171.00	272.0
172.00	500.0
172.90	792.0
174.00	61680.0
175.00	4541.0
176.00	60336.0
177.00	4265.0
192.90	311.0
207.10	355.0
265.10	405.0
265.90	167.0
281.10	1728.0
282.10	625.0
283.00	451.0

Instrument :
MSVOA_D
ClientSampleId :
BFB121

m/z	Abundance
36.00	520.0
37.00	2809.0
38.10	2513.0
39.00	1312.0
40.00	1315.0
44.00	802.0
45.00	728.0
47.10	1065.0
48.10	486.0
49.00	3113.0
50.10	12477.0
51.10	3973.0
52.10	190.0
54.00	179.0
54.80	315.0
56.10	1141.0
57.00	2326.0
60.10	819.0
61.00	4255.0
62.10	3887.0
63.10	3204.0
64.00	701.0
65.00	426.0
66.90	251.0
68.10	8113.0
69.00	7480.0
70.00	670.0
72.00	512.0
73.00	3937.0
74.10	14148.0
75.00	39064.0
76.10	3429.0
77.10	606.0
77.80	720.0
78.90	4380.0
79.90	1093.0
81.00	4186.0
81.90	1161.0
83.10	225.0
85.70	152.0
87.00	4534.0
88.00	4843.0
90.90	299.0
92.00	2460.0
93.00	3776.0
94.00	10594.0
95.10	79800.0
96.00	5566.0
97.10	223.0
103.70	558.0
104.80	180.0
105.90	573.0
111.60	194.0
116.00	399.0
116.90	626.0
117.80	256.0
119.00	765.0
124.80	193.0
125.20	202.0
127.80	291.0
128.90	166.0
129.80	386.0
130.90	221.0
132.90	488.0
140.90	766.0
143.00	1174.0
145.00	686.0
145.80	311.0
147.80	261.0
155.00	220.0
171.00	297.0
172.00	826.0
172.90	1074.0
174.00	77960.0
174.90	5000.0
176.00	73616.0
177.00	4584.0
177.90	171.0
190.90	211.0
193.00	277.0
207.00	359.0
208.00	204.0
249.10	470.0
251.20	160.0
265.10	269.0
267.10	208.0
281.20	3460.0
282.00	983.0
283.10	906.0

Instrument :
MSVOA_D
ClientSampleId :
BFB121

m/z	Abundance
36.20	306.0
37.00	2605.0
38.10	2529.0
39.10	1234.0
39.90	1193.0
44.10	817.0
45.20	558.0
47.10	596.0
47.90	420.0
49.10	2638.0
50.10	10890.0
51.10	4073.0
52.10	230.0
54.10	151.0
55.90	859.0
57.00	2158.0
60.00	851.0
61.00	2965.0
62.10	3377.0
63.00	2495.0
63.90	480.0
65.10	498.0
66.90	211.0
68.10	7061.0
69.10	6735.0
70.10	543.0
72.00	475.0
73.00	3376.0
74.10	11039.0
75.00	33648.0
76.10	3058.0
77.00	567.0
77.80	398.0
79.00	3708.0
80.00	764.0
80.90	3734.0
81.80	630.0
85.80	195.0
86.90	3444.0
88.00	3988.0
91.10	284.0
92.00	2424.0
93.10	3197.0
94.00	8549.0
95.00	70536.0
96.00	4612.0
97.00	166.0
104.00	386.0
104.80	182.0
105.90	301.0
116.00	272.0
116.80	513.0
118.00	347.0
118.80	741.0
124.70	208.0
125.20	231.0
127.90	416.0
129.90	267.0
133.30	671.0
136.70	191.0
141.00	598.0
143.00	1276.0
143.80	156.0
144.90	488.0
146.00	184.0
149.90	163.0
155.00	247.0
171.00	174.0
172.00	996.0
173.00	622.0
174.00	70720.0
174.90	4916.0
176.00	66752.0
176.90	4609.0
177.80	227.0
191.00	287.0
192.90	428.0
207.00	389.0
208.00	152.0
249.20	236.0
265.00	344.0
265.90	177.0
281.10	4066.0
282.00	937.0
283.10	876.0
284.00	189.0

Instrument :
MSVOA_D
ClientSampleId :
BFB121