


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD042919\
Data File : VD062059.D
Acq On : 29 Apr 2019 13:07
Operator : FY/SY
Sample : BFB
Misc : 5.00qm/5mL/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D042319S.M
Title : SW846 8260
Last Update : Tue Apr 23 14:52:55 2019

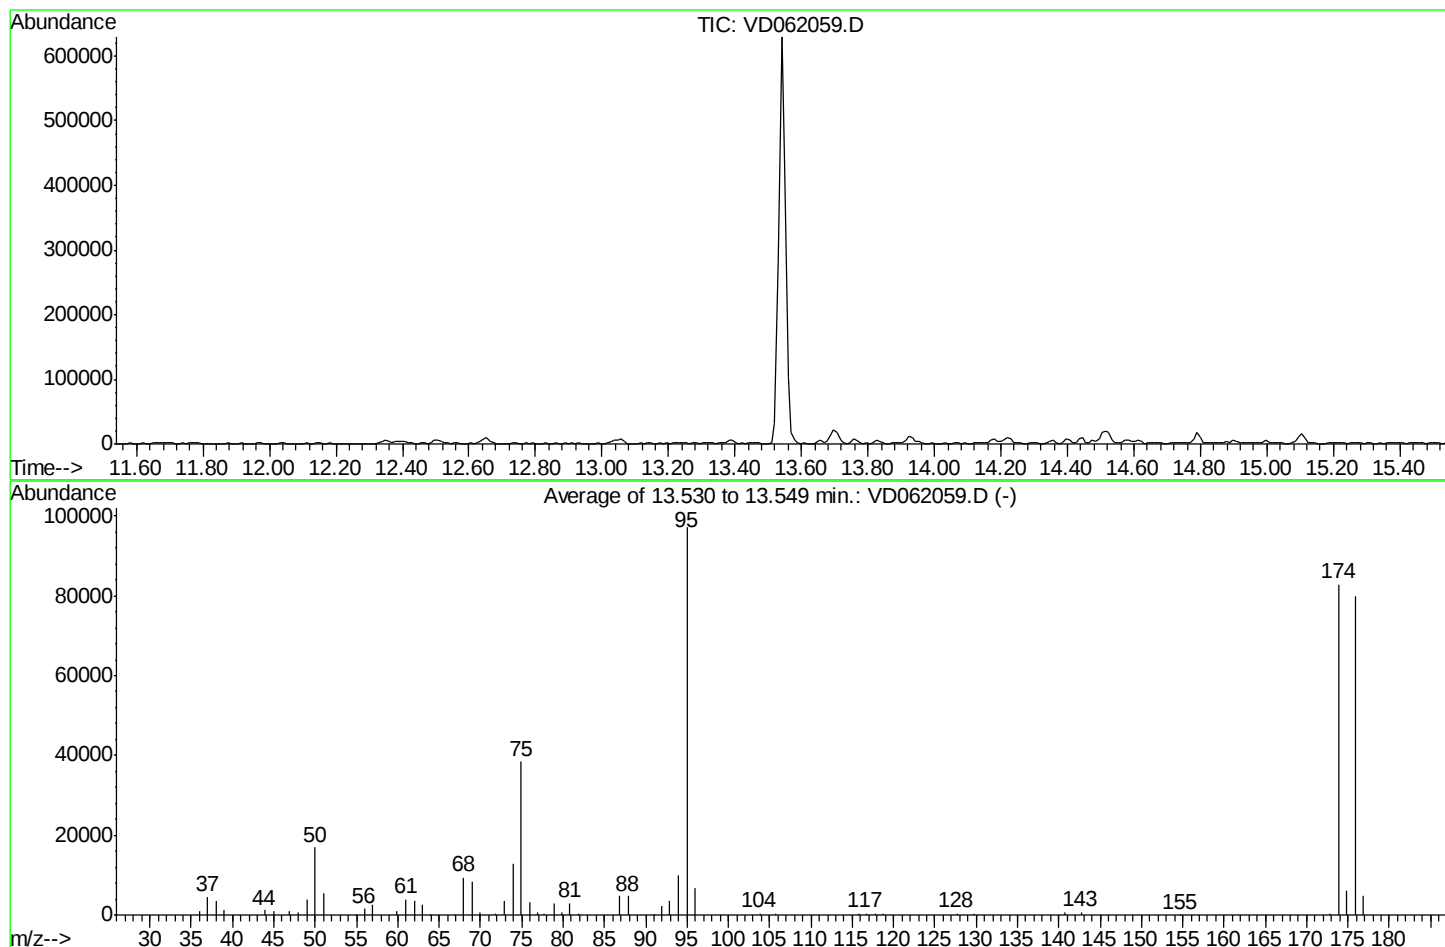

AutoFind: Scans 1230, 1231, 1232; Background Corrected with Scan 1226

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	16927	PASS
75	95	30	60	39.6	38445	PASS
95	95	100	100	100.0	97154	PASS
96	95	5	9	6.8	6596	PASS
173	174	0.00	2	0.3	282	PASS
174	95	50	100	85.3	82898	PASS
175	174	5	9	7.2	5954	PASS
176	174	95	101	96.5	80037	PASS
177	176	5	9	5.9	4734	PASS