



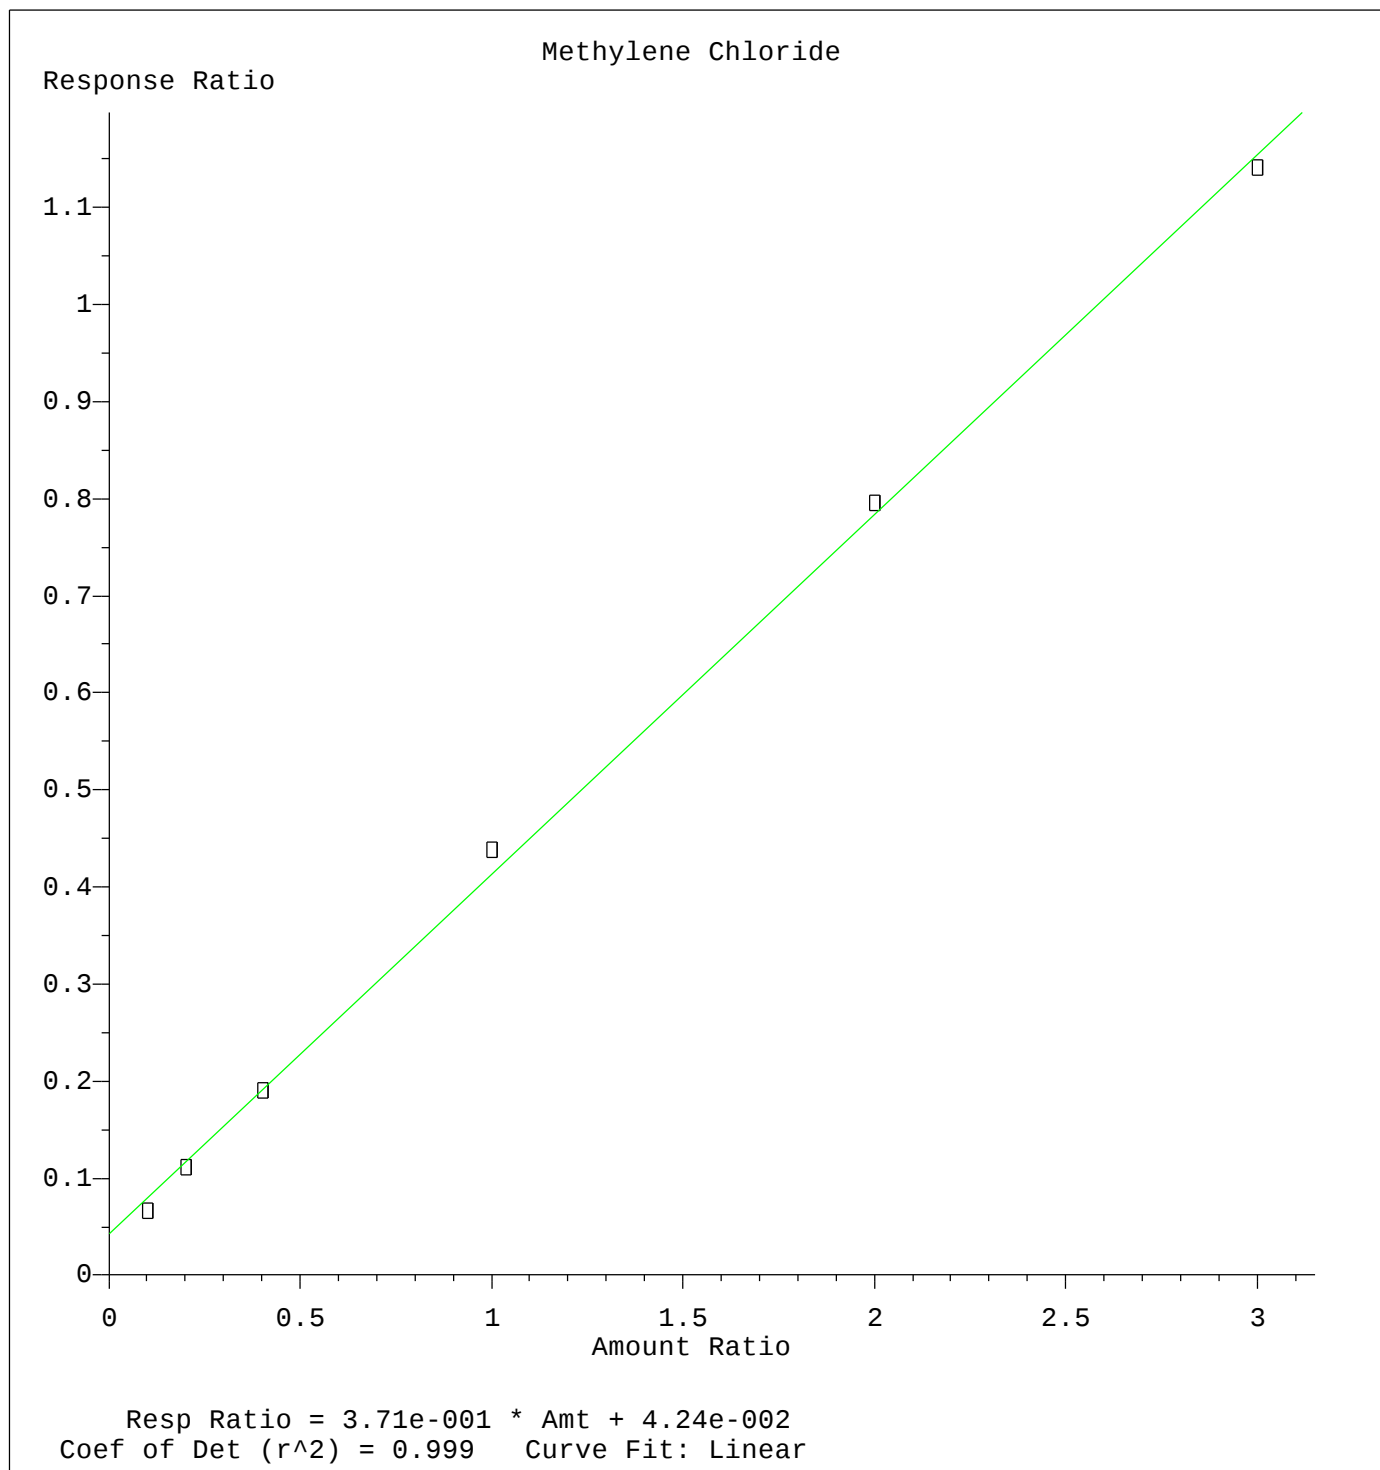


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D042920S.M
Calibration Table Last Updated: Thu Apr 30 07:35:06 2020

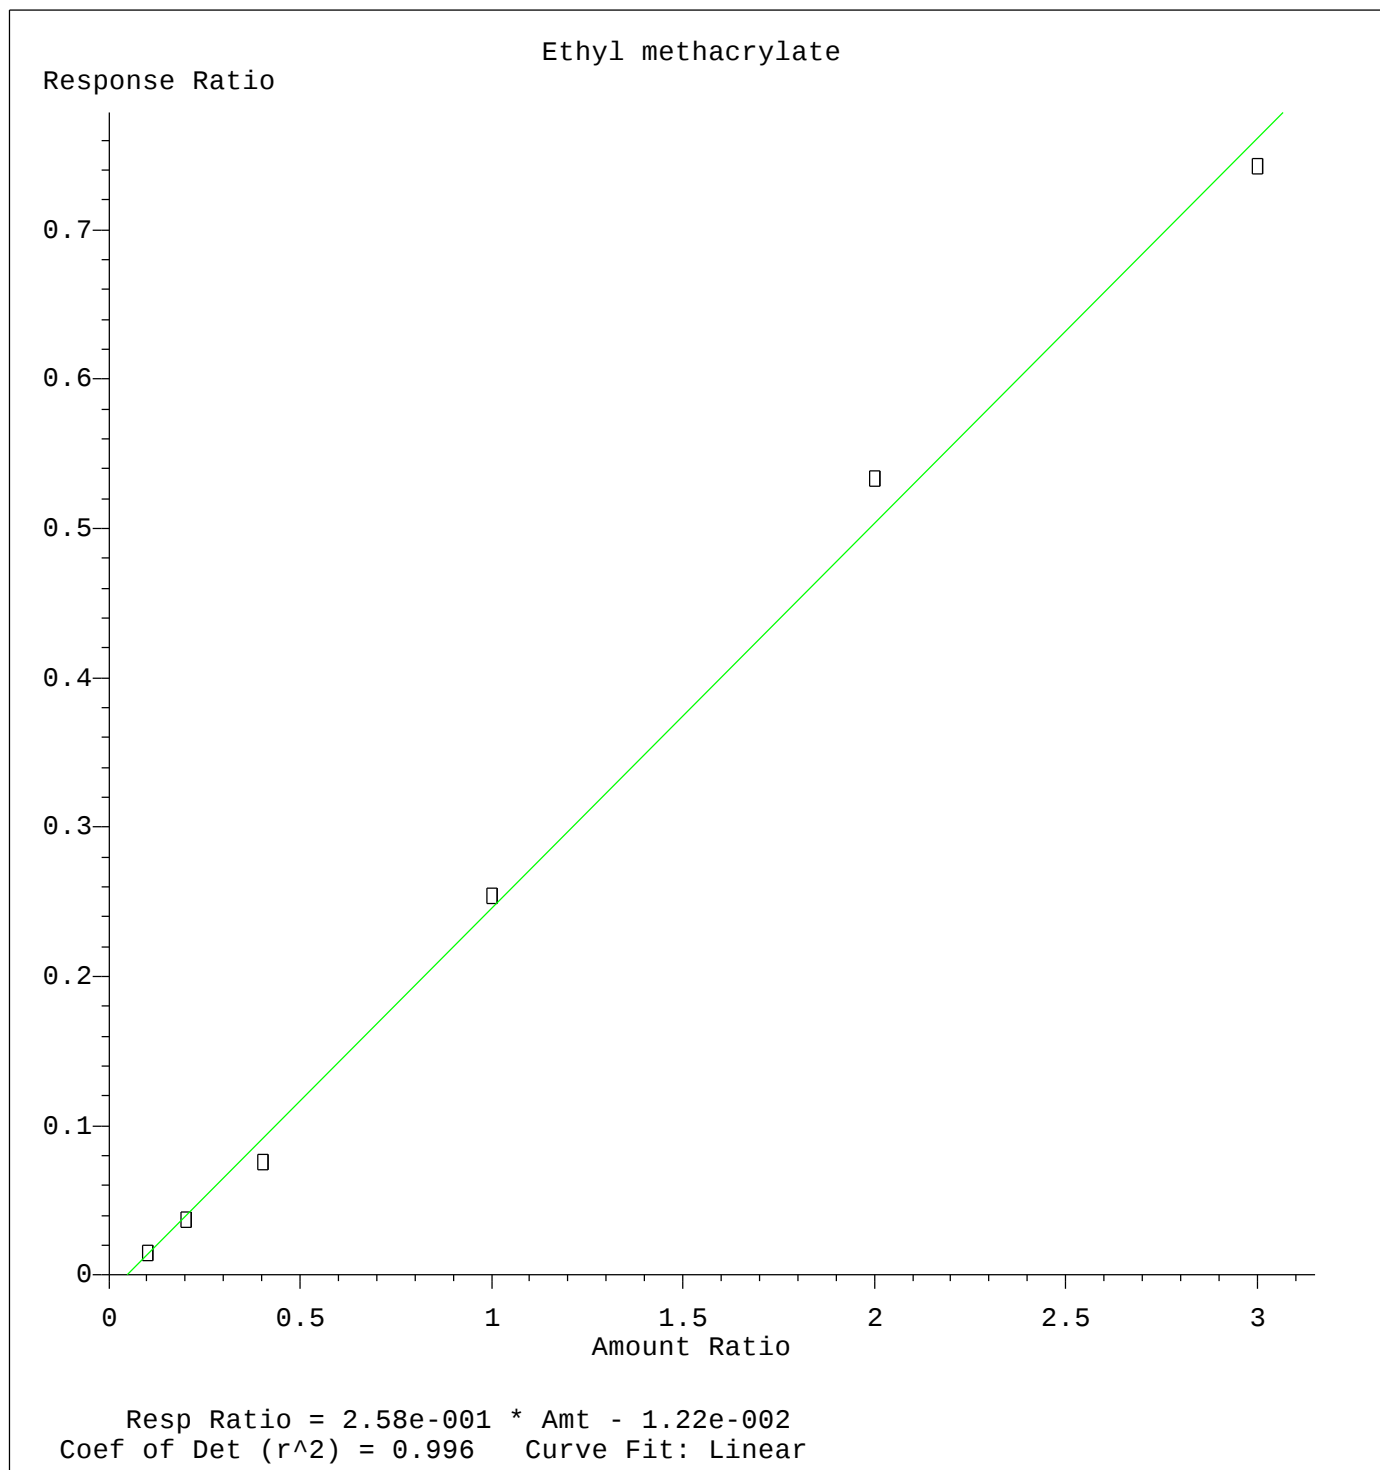

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D042920S.M
Calibration Table Last Updated: Thu Apr 30 07:35:06 2020


Naphthalene

Response Ratio

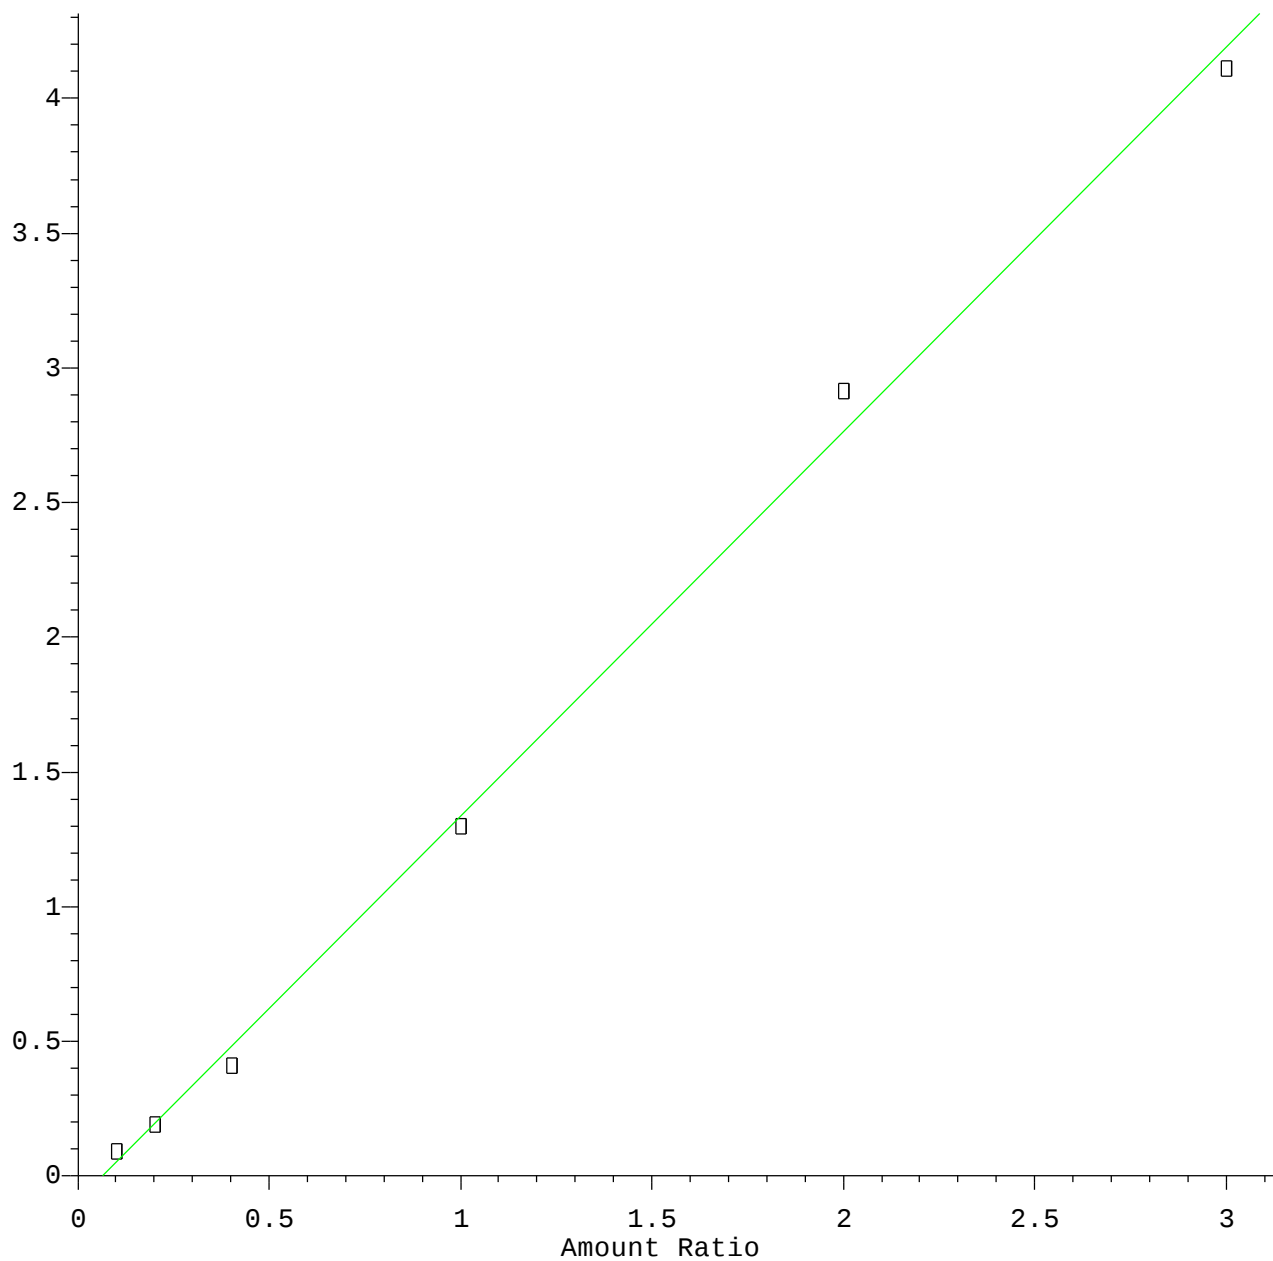


Resp Ratio = 1.43e+000 * Amt - 9.27e-002
Coef of Det (r^2) = 0.997 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D042920S.M
Calibration Table Last Updated: Thu Apr 30 07:35:06 2020

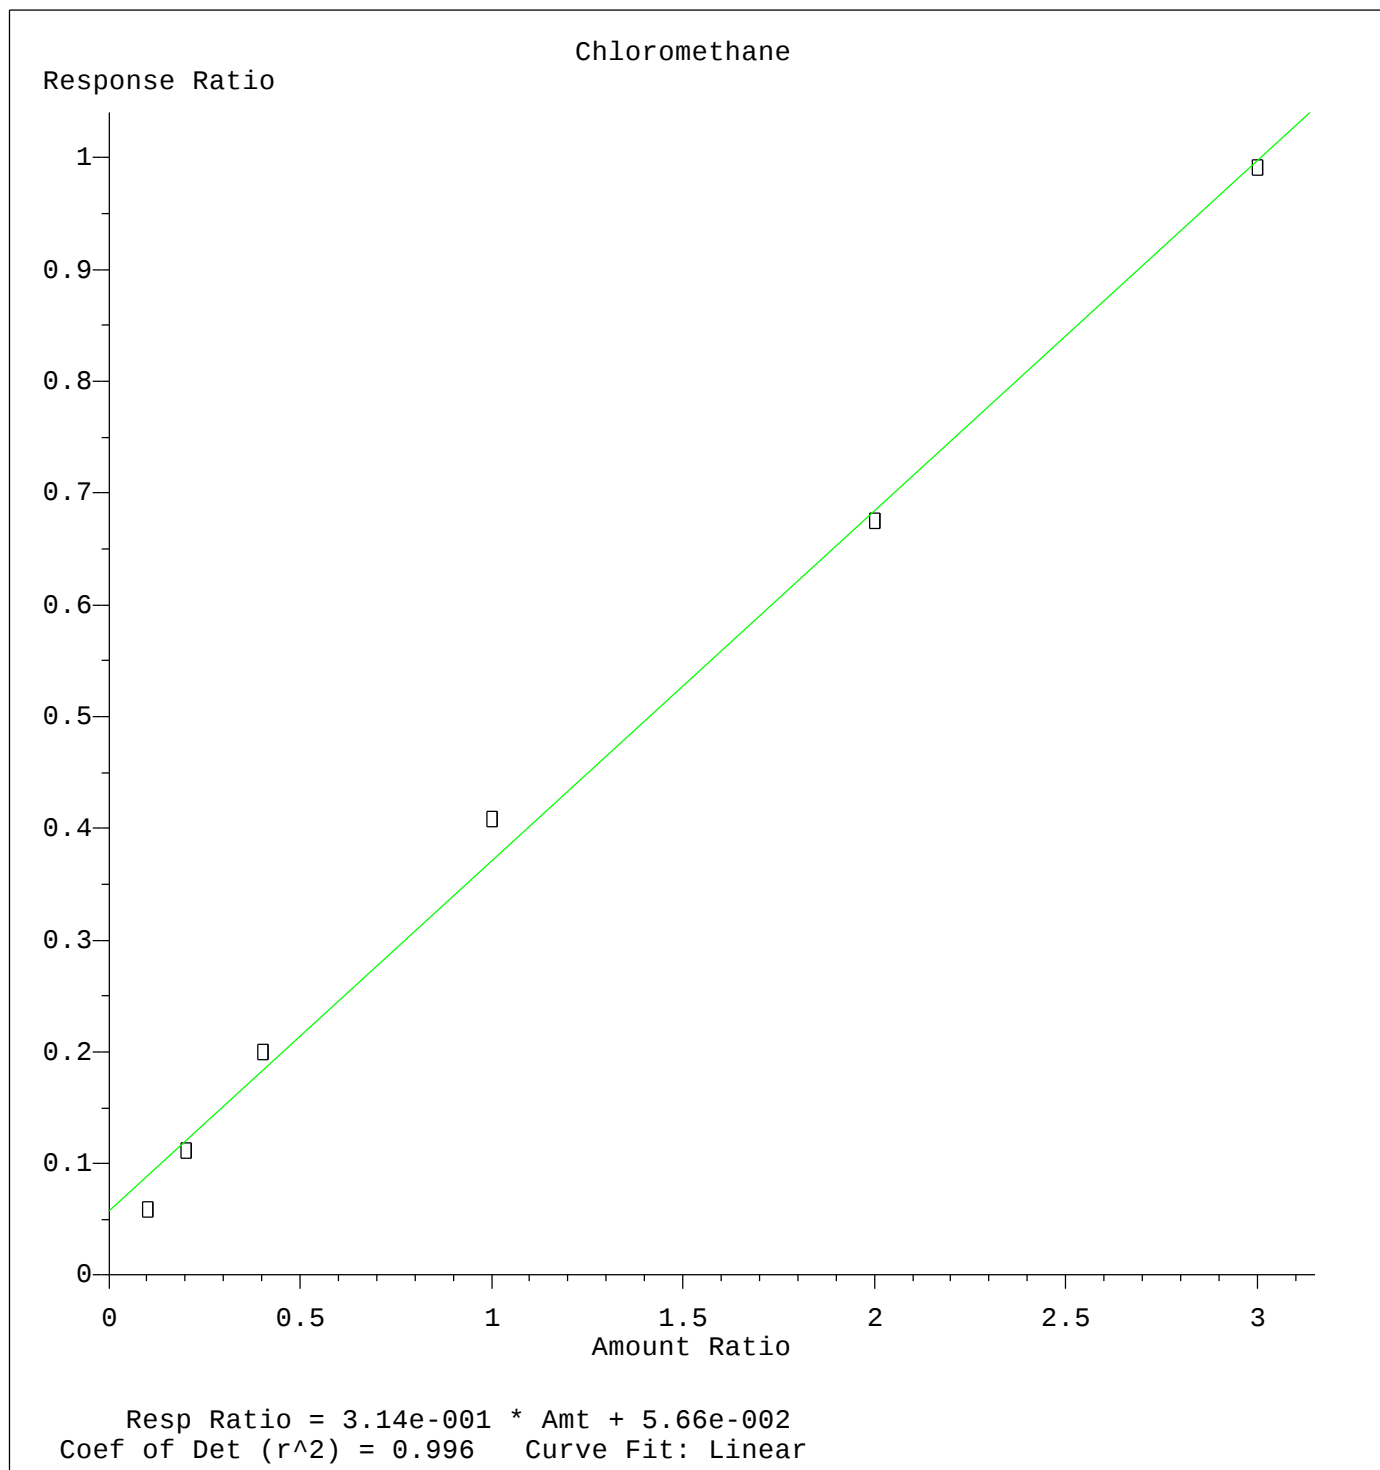

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D042920S.M
Calibration Table Last Updated: Thu Apr 30 07:35:06 2020

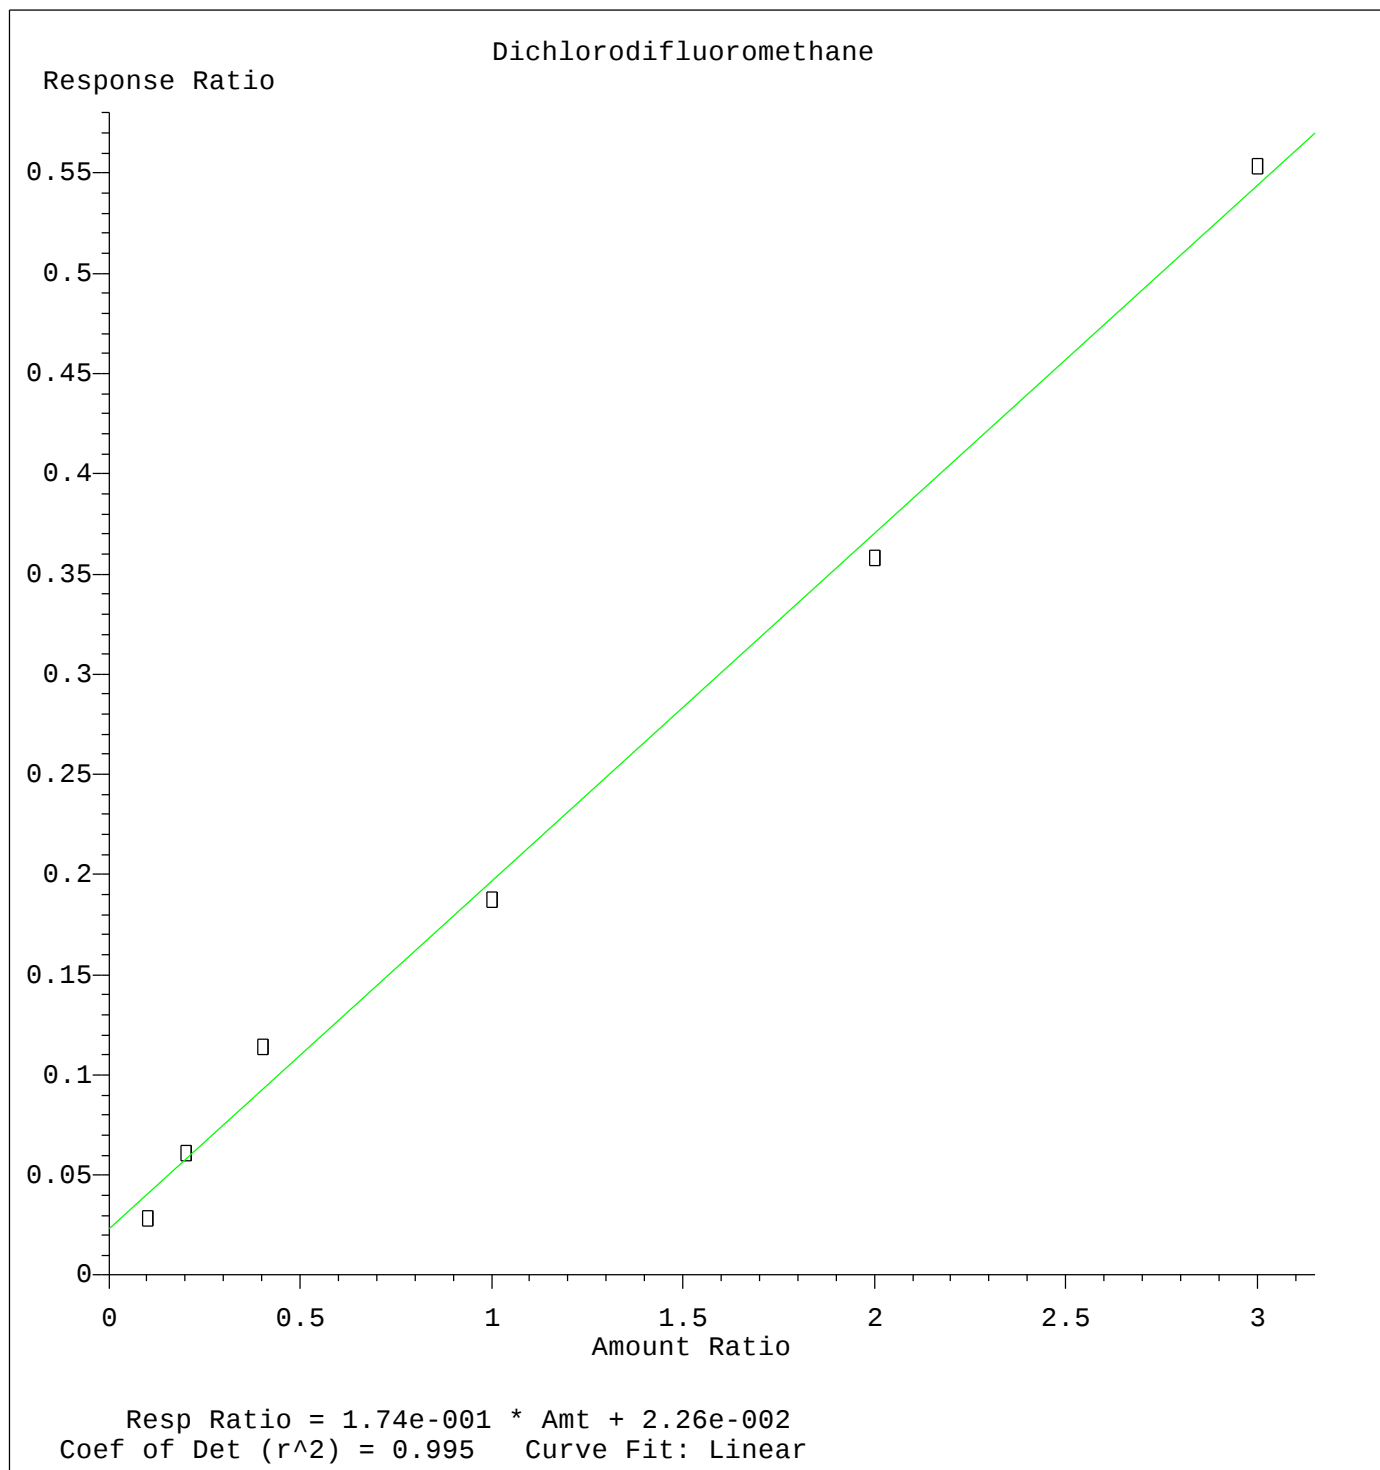

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D042920S.M
Calibration Table Last Updated: Thu Apr 30 07:35:06 2020

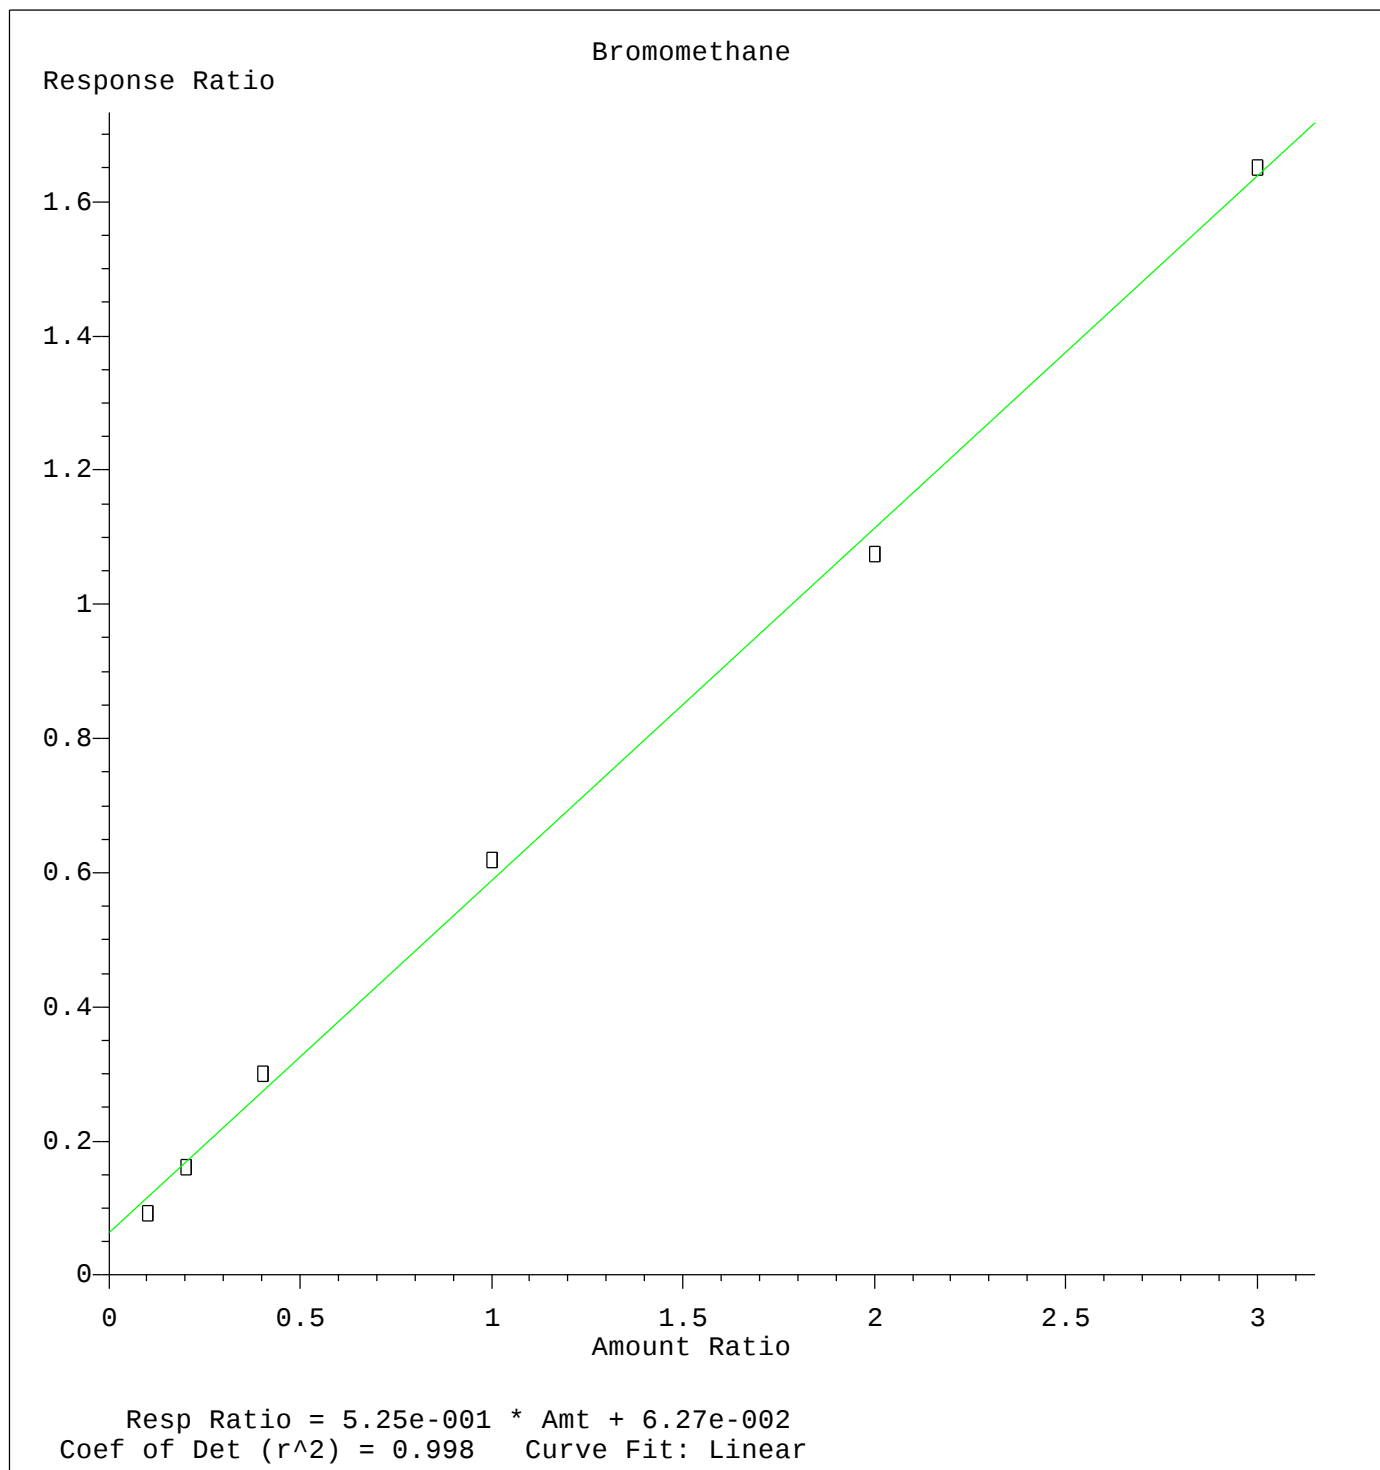

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D042920S.M
Calibration Table Last Updated: Thu Apr 30 07:35:06 2020