


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD042920\
Data File : VD065678.D
Acq On : 29 Apr 2020 12:25
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D042920S.M
Title : SW846 8260
Last Update : Thu Apr 30 07:35:06 2020

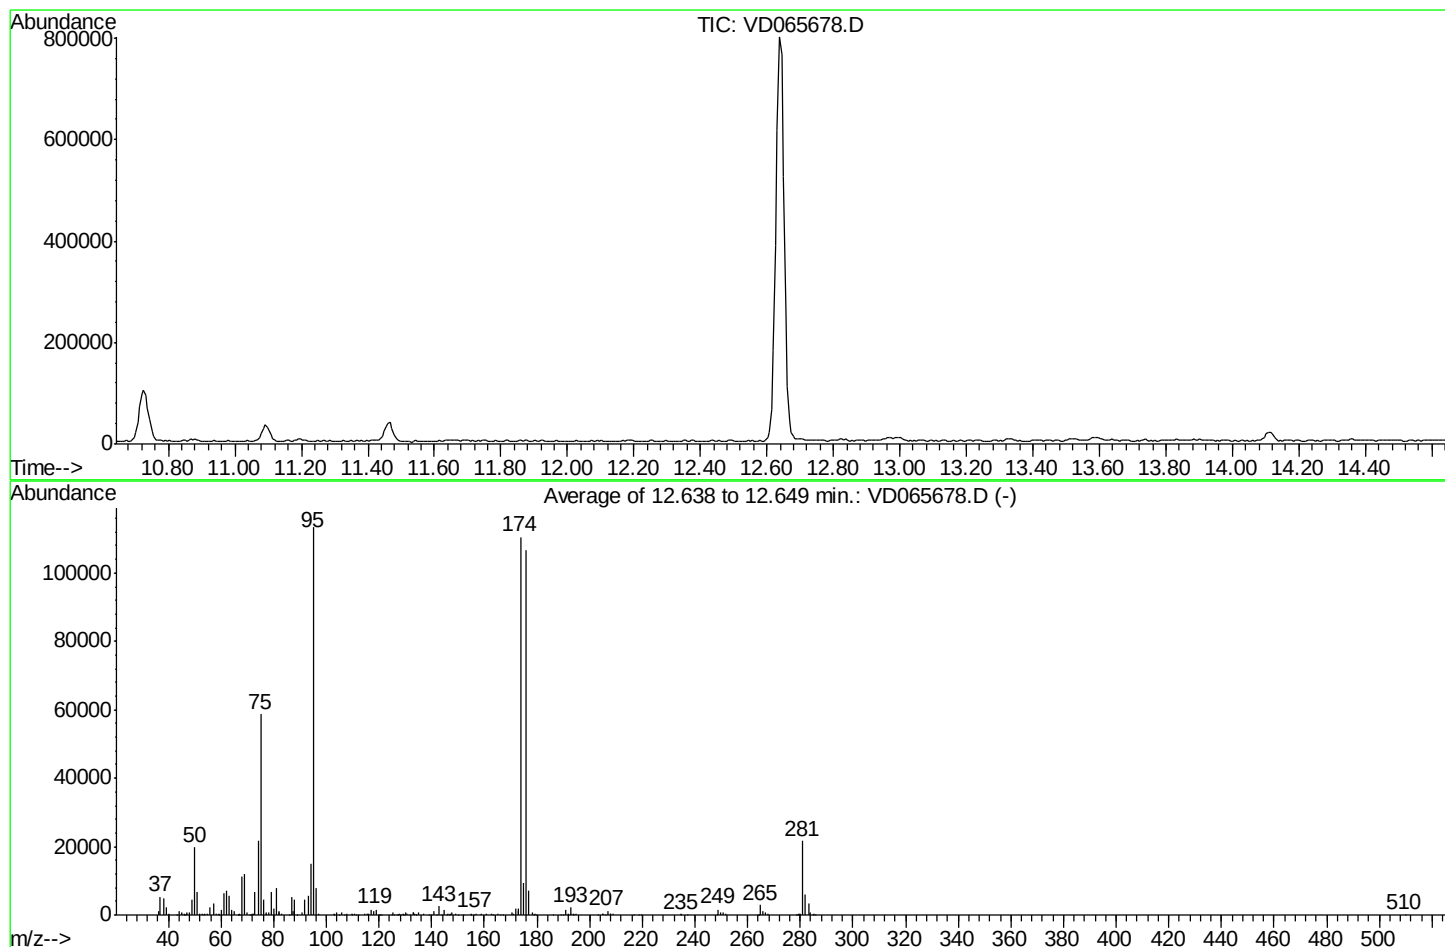

AutoFind: Scans 1822, 1823, 1824; Background Corrected with Scan 1813

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	19765	PASS
75	95	30	60	51.8	58658	PASS
95	95	100	100	100.0	113346	PASS
96	95	5	9	6.9	7835	PASS
173	174	0.00	2	1.6	1781	PASS
174	95	50	100	97.5	110466	PASS
175	174	5	9	8.4	9261	PASS
176	174	95	101	96.6	106704	PASS
177	176	5	9	6.5	6982	PASS