




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042923\
 Data File : VD075915.D
 Acq On : 29 Apr 2023 14:23
 Operator : KP/SY
 Sample : 02525-02
 Misc : 5.80G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DCCC2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2023
 Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: May 01 00:16:17 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon May 01 00:14:49 2023
 Response via : Initial Calibration

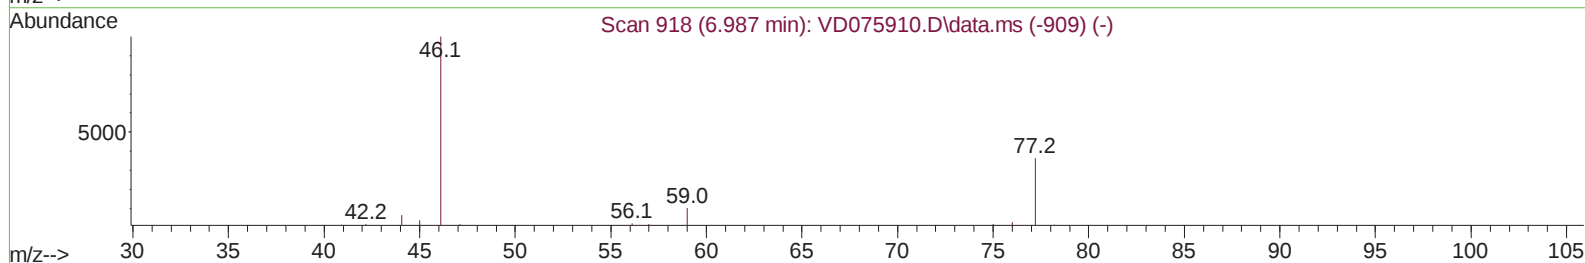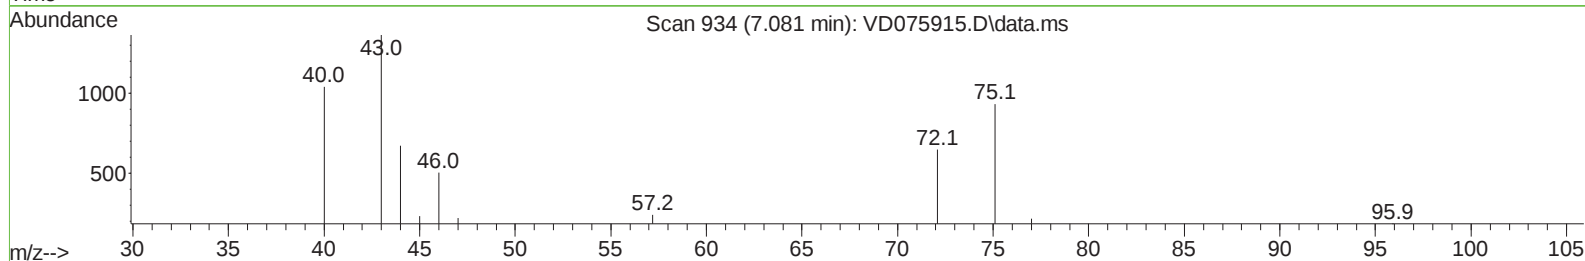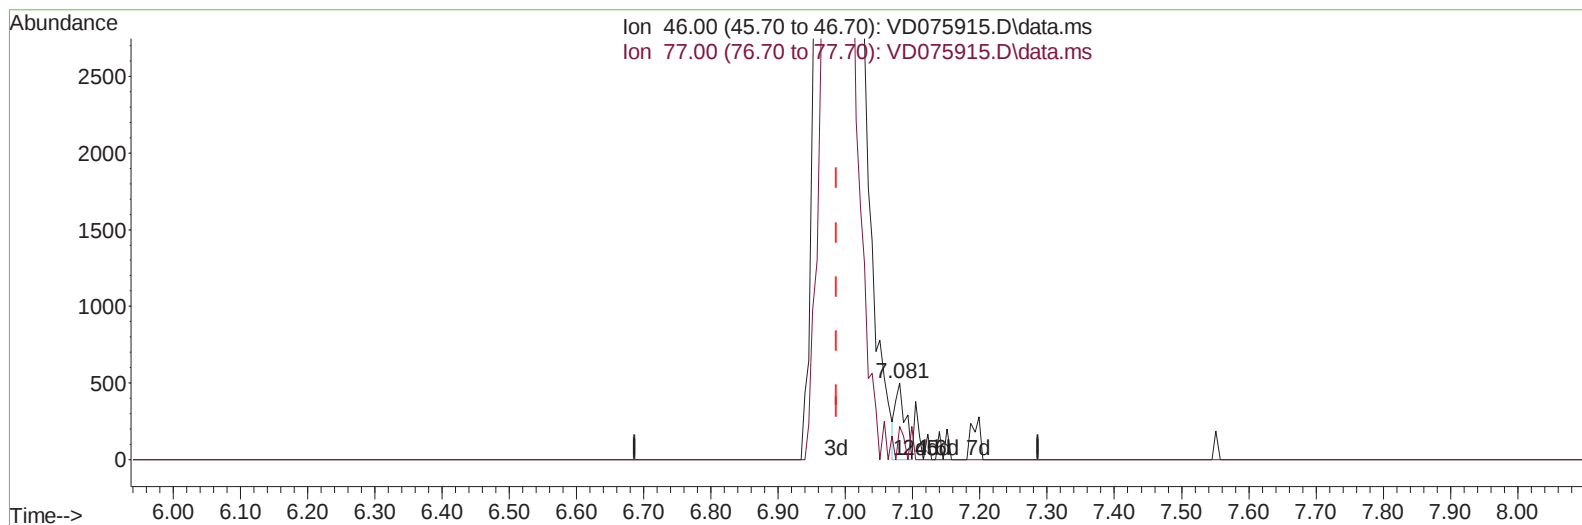

TIC: VD075915.D\data.ms

(21) 2-Butanone-d5 (S)

7.081min (+ 0.094) 0.54 ug/L

response 502

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	33.50	26.10
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042923\
 Data File : VD075915.D
 Acq On : 29 Apr 2023 14:23
 Operator : KP/SY
 Sample : 02525-02
 Misc : 5.80G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DCCC2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2023
 Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: May 01 00:16:17 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon May 01 00:14:49 2023
 Response via : Initial Calibration

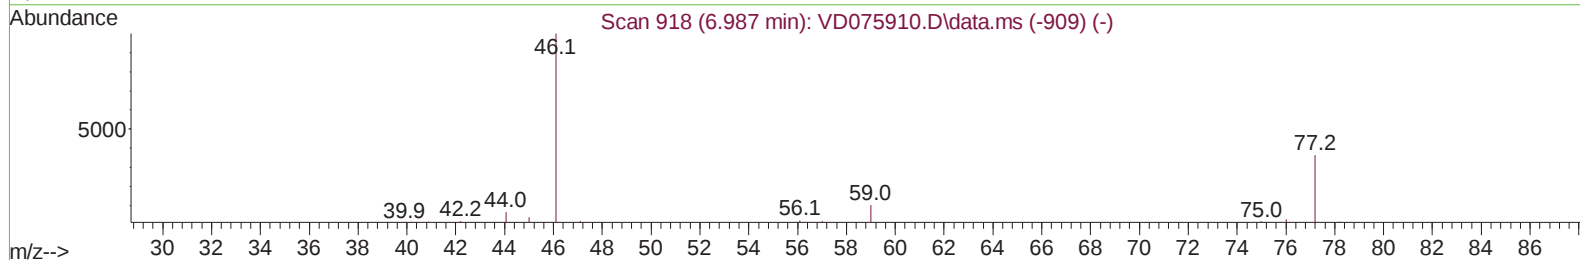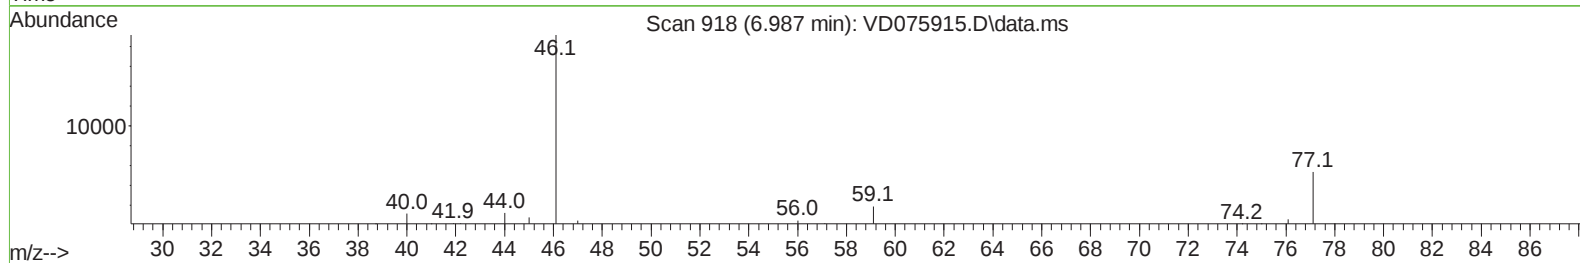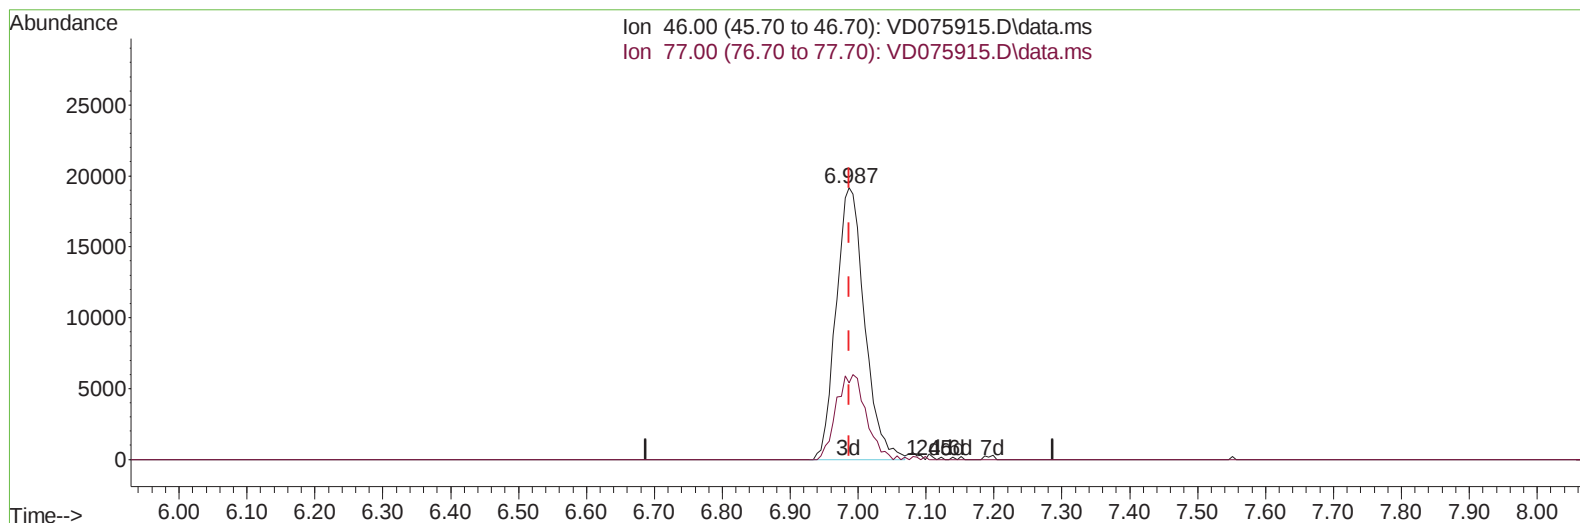

TIC: VD075915.D\data.ms

(21) 2-Butanone-d5 (S)

6.987min (-0.000) 59.62 ug/L m

response 55586

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	33.50	0.24#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042923\
 Data File : VD075915.D
 Acq On : 29 Apr 2023 14:23
 Operator : KP/SY
 Sample : 02525-02
 Misc : 5.80G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DCCC2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2023
 Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: May 01 00:16:17 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon May 01 00:14:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.781	114	489556	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117	505494	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.522	152	232231	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.275	65	187374	17.447	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	69.800%	
7) Chloroethane-d5	2.799	69	182111	19.626	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	78.520%	
11) 1,1-Dichloroethene-d2	3.916	65	44728	18.065	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	72.240%	
21) 2-Butanone-d5	6.987	46	55586m	59.620	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	119.240%	
24) Chloroform-d	7.569	84	284069	23.204	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	92.800%	
26) 1,2-Dichloroethane-d4	8.234	65	125802	24.063	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	96.240%	
32) Benzene-d6	8.204	84	537839	18.255	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	73.040%	
36) 1,2-Dichloropropane-d6	9.210	67	171317	21.008	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	84.040%	
41) Toluene-d8	10.269	98	490102	17.768	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	71.080%	
43) trans-1,3-Dichloroprop...	10.528	79	66672	19.780	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	79.120%	
47) 2-Hexanone-d5	10.881	63	45870	46.715	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	93.440%	
56) 1,1,2,2-Tetrachloroeth...	12.651	84	153460	24.592	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	98.360%	
66) 1,2-Dichlorobenzene-d4	13.816	152	185782	22.617	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	90.480%	
Target Compounds						
					Qvalue	
13) Acetone	4.022	43	73653	92.313	ug/L	98
16) Methylene chloride	4.799	84	10577	1.065	ug/L	89
22) 2-Butanone	7.087	43	5271	5.068	ug/L	78

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042923\
Data File : VD075915.D
Acq On : 29 Apr 2023 14:23
Operator : KP/SY
Sample : 02525-02
Misc : 5.80G/10.00ml/MSVOA_D/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
DCCC2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2023
Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: May 01 00:16:17 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Quant Title : SFAM01.0
QLast Update : Mon May 01 00:14:49 2023
Response via : Initial Calibration

