




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042923\
Data File : VD075926.D
Acq On : 29 Apr 2023 19:46
Operator : KP/SY
Sample : 02548-41
Misc : 5.47G/10.00ml/MSVOA_D/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
DCCS0MS

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2023
Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: May 01 00:18:41 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Quant Title : SFAM01.0
QLast Update : Mon May 01 00:14:49 2023
Response via : Initial Calibration

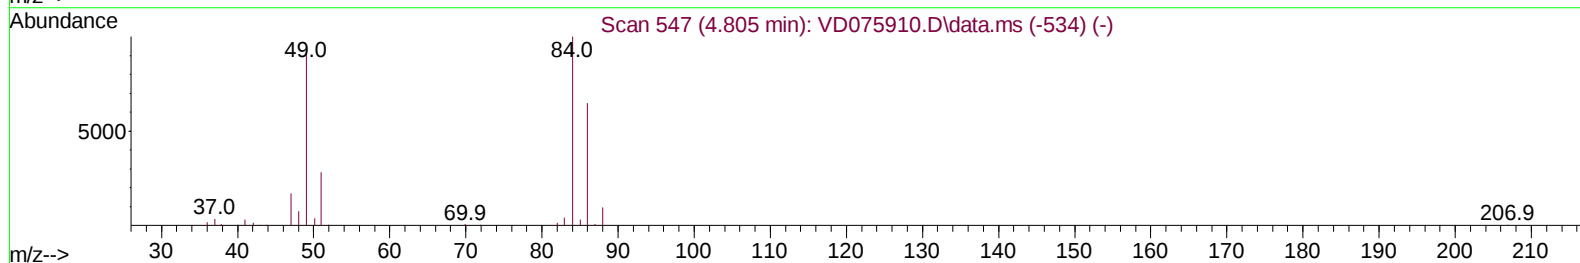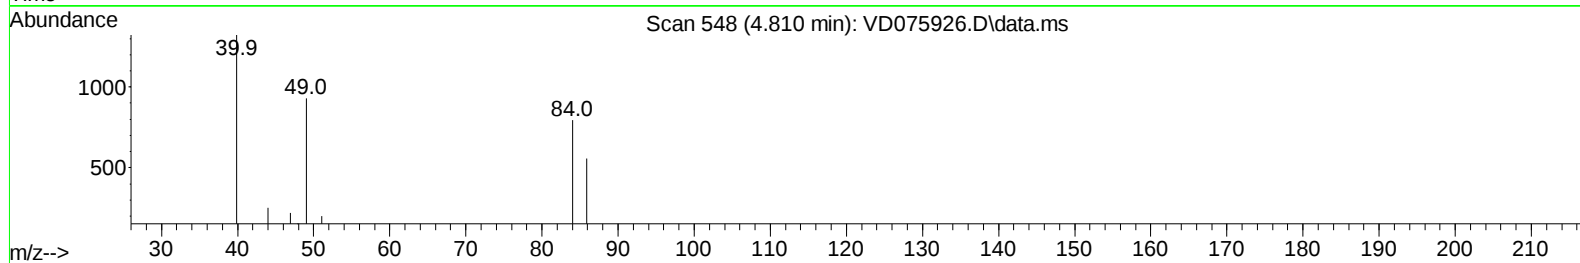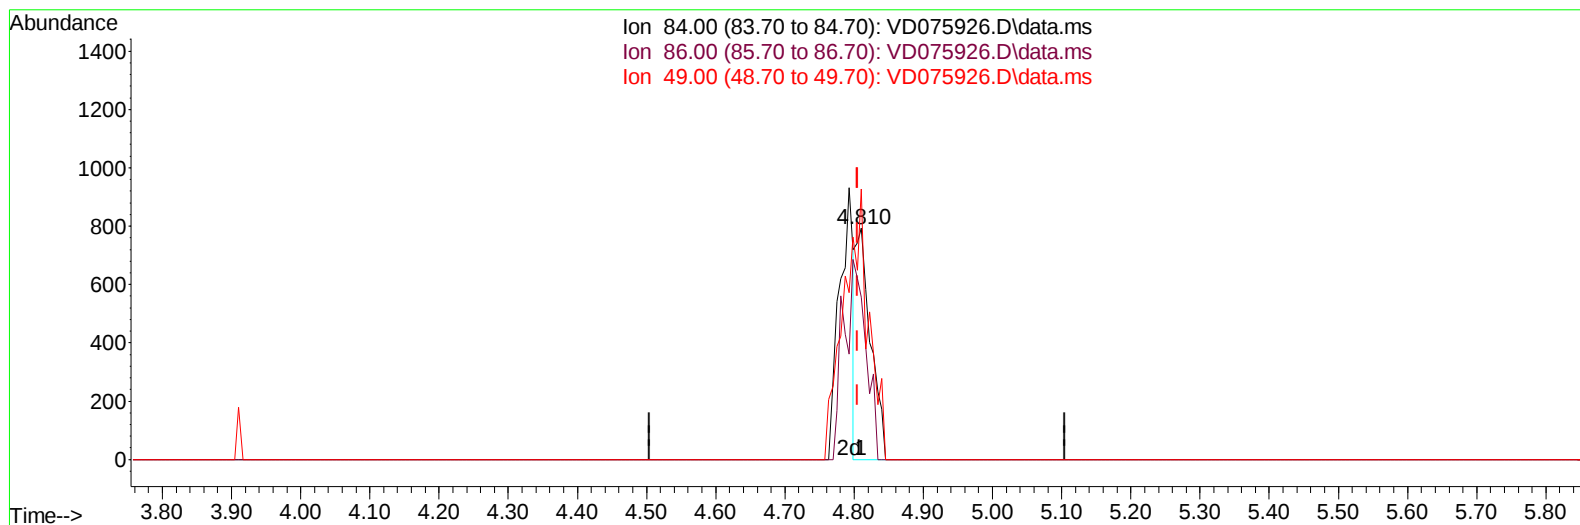

TIC: VD075926.D\data.ms

(16) Methylene chloride (T)**4.810min (+ 0.006) 1.09 ug/L****response 1160**

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	65.50	70.11
49.00	86.80	117.02#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042923\
 Data File : VD075926.D
 Acq On : 29 Apr 2023 19:46
 Operator : KP/SY
 Sample : 02548-41
 Misc : 5.47G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DCCS0MS

Manual IntegrationsAPPROVED

Quant Time: May 01 00:18:41 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon May 01 00:14:49 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/01/2023
 Supervised By :Mahesh Dadoda 05/01/2023

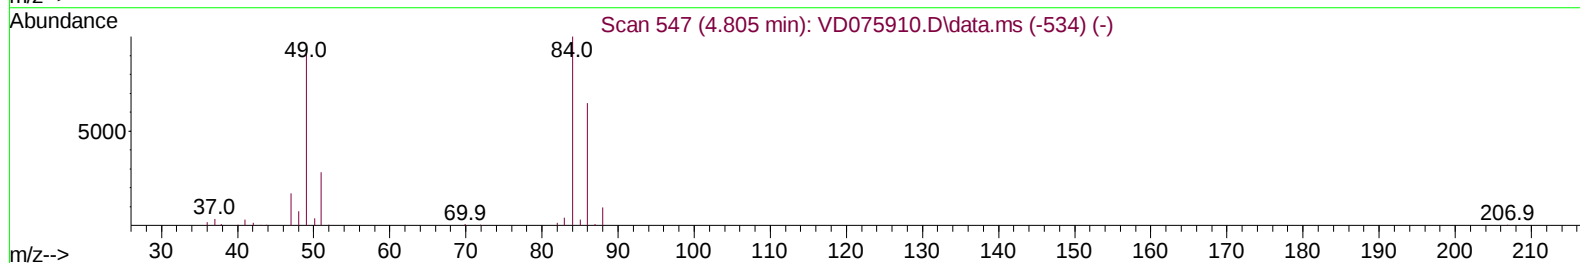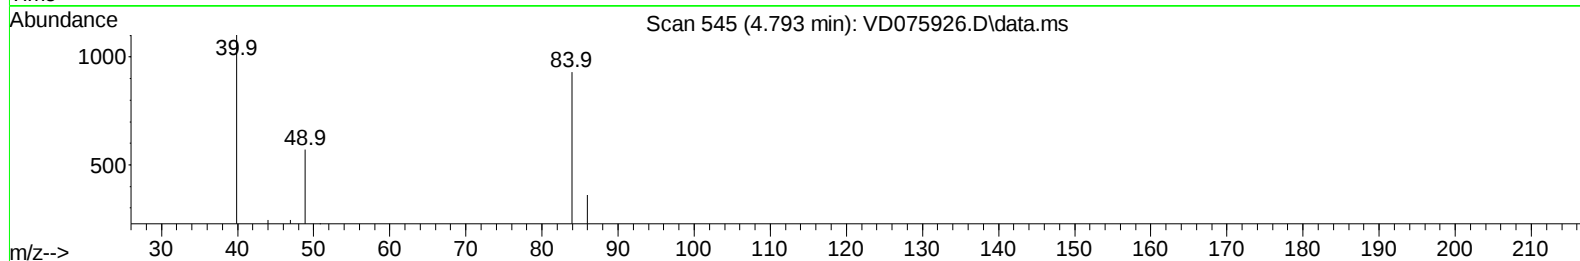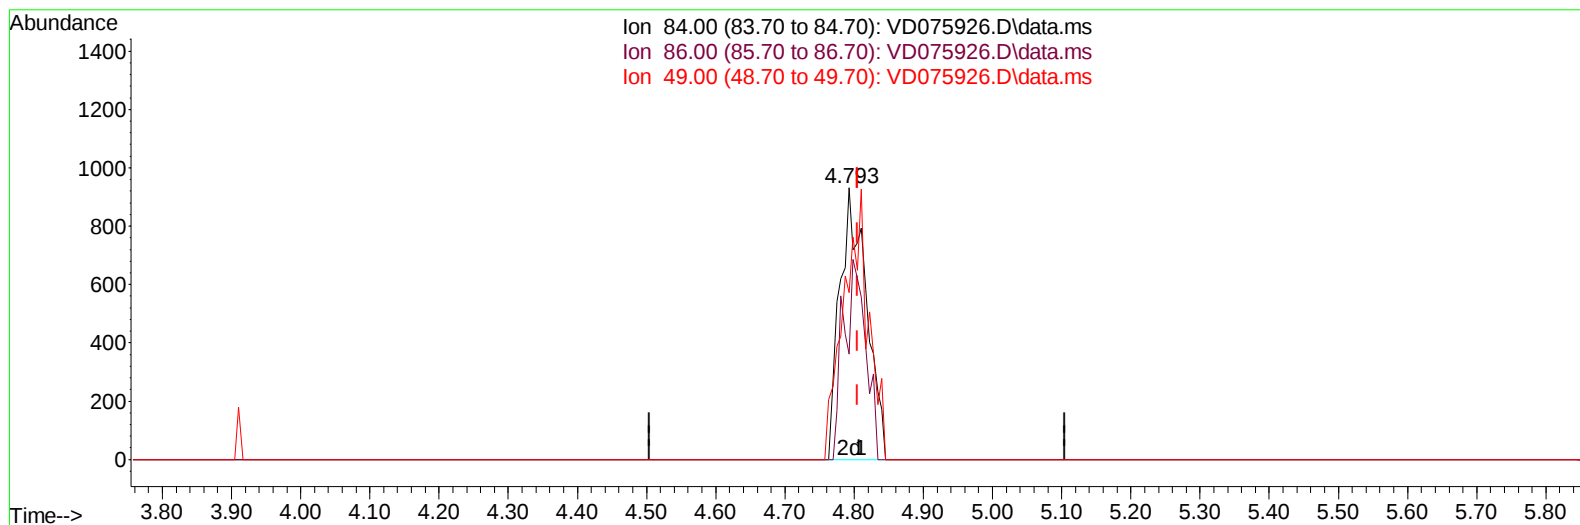

TIC: VD075926.D\data.ms

(16) Methylene chloride (T)

4.793min (-0.012) 2.32 ug/L m

response 2482

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	65.50	38.78#
49.00	86.80	61.33
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042923\
 Data File : VD075926.D
 Acq On : 29 Apr 2023 19:46
 Operator : KP/SY
 Sample : 02548-41
 Misc : 5.47G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DCCS0MS

Manual IntegrationsAPPROVED

Quant Time: May 01 00:18:41 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon May 01 00:14:49 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/01/2023
 Supervised By :Mahesh Dadoda 05/01/2023

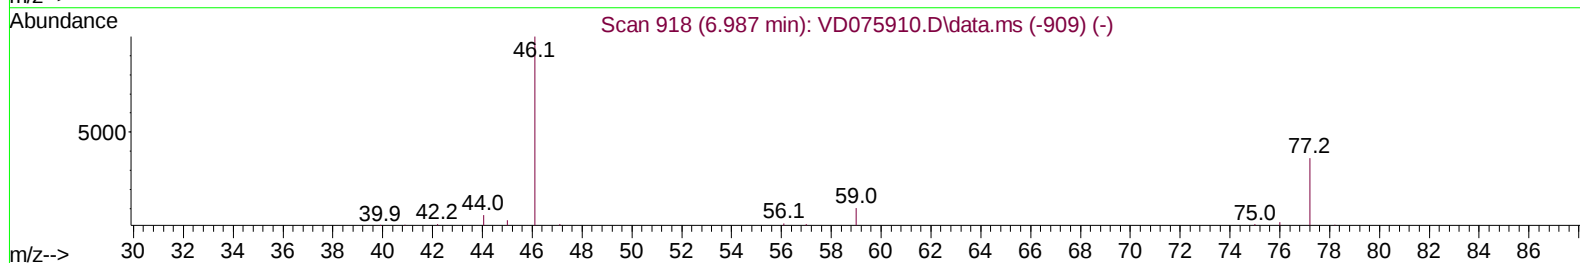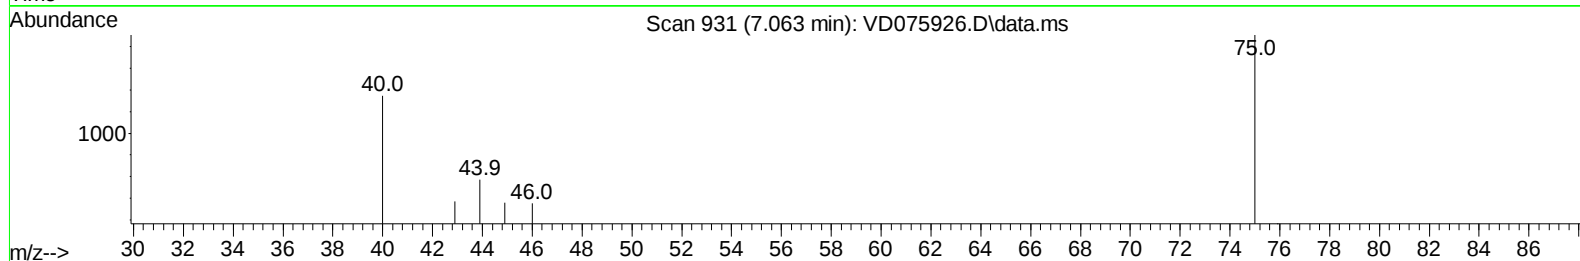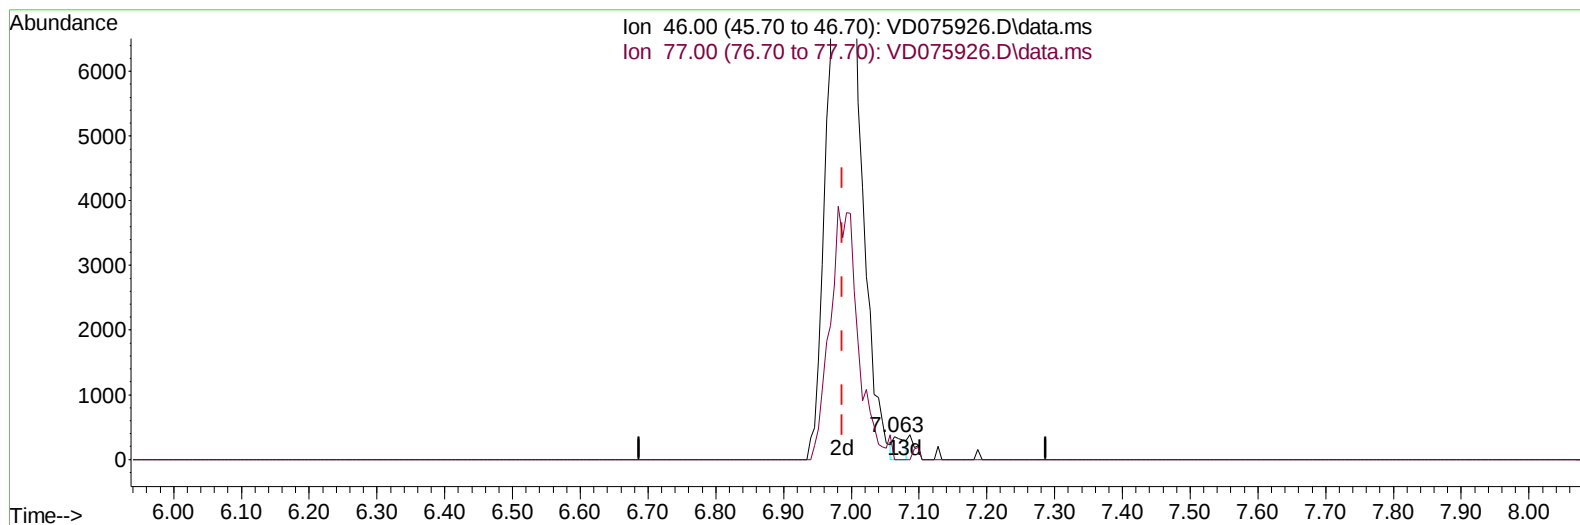

TIC: VD075926.D\data.ms

(21) 2-Butanone-d5 (S)

7.063min (+ 0.076) 4.45 ug/L

response 446

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	33.50	30.27
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042923\
Data File : VD075926.D
Acq On : 29 Apr 2023 19:46
Operator : KP/SY
Sample : 02548-41
Misc : 5.47G/10.00ml/MSVOA_D/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
DCCS0MS

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2023
Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: May 01 00:18:41 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Quant Title : SFAM01.0
QLast Update : Mon May 01 00:14:49 2023
Response via : Initial Calibration

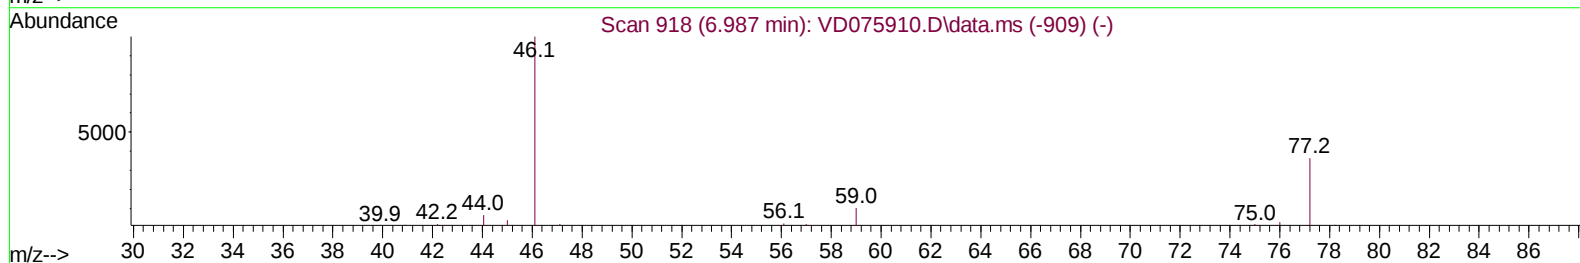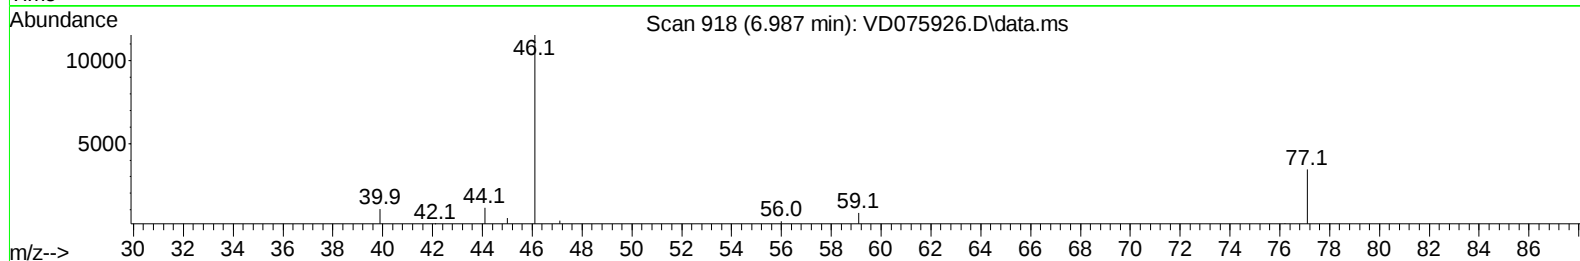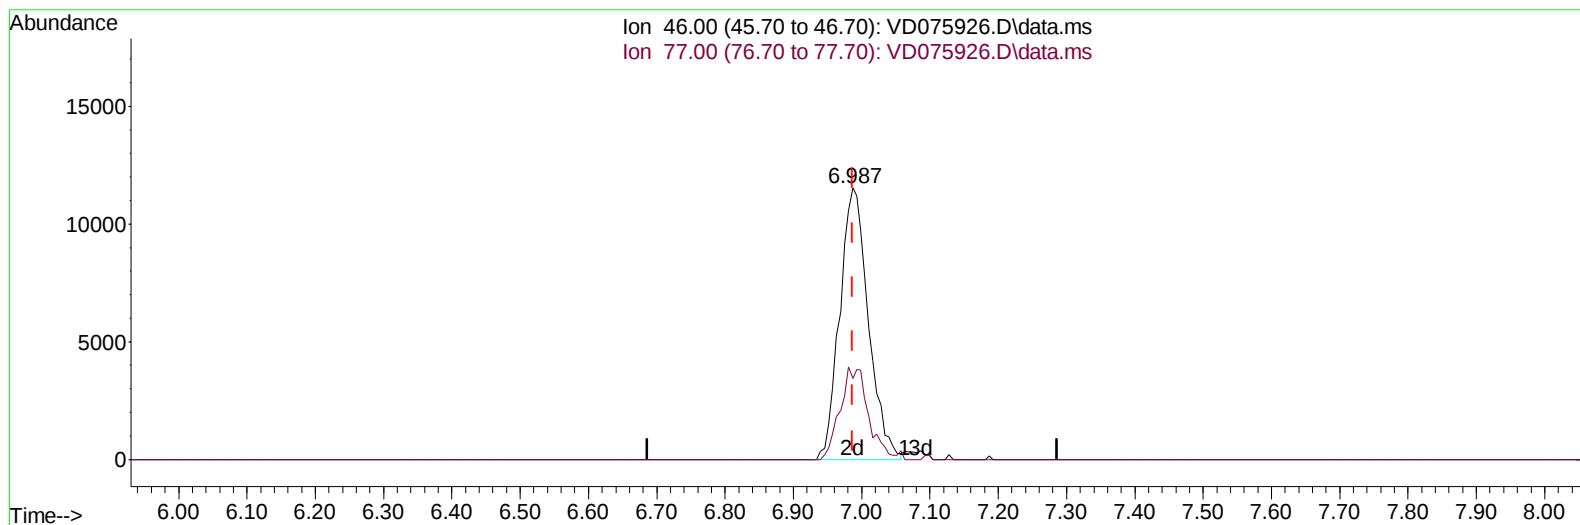

TIC: VD075926.D\data.ms

(21) 2-Butanone-d5 (S)

6.987min (-0.000) 333.70 ug/L m

response 33460

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	33.50	0.40#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042923\
 Data File : VD075926.D
 Acq On : 29 Apr 2023 19:46
 Operator : KP/SY
 Sample : 02548-41
 Misc : 5.47G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DCCS0MS

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2023
 Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: May 01 00:18:41 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon May 01 00:14:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.781	114	52650	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117	67724	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.522	152	34079	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.269	65	17268	14.951	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery =	59.800%		
7) Chloroethane-d5	2.799	69	21009	21.052	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery =	84.200%		
11) 1,1-Dichloroethene-d2	3.916	65	4564	17.140	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery =	68.560%		
21) 2-Butanone-d5	6.987	46	33460m	333.703	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery =	667.400%#		
24) Chloroform-d	7.569	84	41738	31.701	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery =	126.800%		
26) 1,2-Dichloroethane-d4	8.234	65	28343	50.410	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery =	201.640%#		
32) Benzene-d6	8.198	84	69065	17.497	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery =	70.000%		
36) 1,2-Dichloropropane-d6	9.210	67	27579	25.243	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery =	100.960%		
41) Toluene-d8	10.269	98	55646	15.058	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery =	60.240%		
43) trans-1,3-Dichloroprop...	10.528	79	13674	30.279	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery =	121.120%		
47) 2-Hexanone-d5	10.875	63	22191	168.687	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery =	337.380%#		
56) 1,1,2,2-Tetrachloroeth...	12.651	84	60764	72.680	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery =	290.720%#		
66) 1,2-Dichlorobenzene-d4	13.816	152	30430	25.244	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery =	100.960%		
Target Compounds						
13) Acetone	4.022	43	19173	223.443	ug/L	99
16) Methylene chloride	4.793	84	2482m	2.324	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042923\
Data File : VD075926.D
Acq On : 29 Apr 2023 19:46
Operator : KP/SY
Sample : 02548-41
Misc : 5.47G/10.00mL/MSVOA_D/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
DCCS0MS

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2023
Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: May 01 00:18:41 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Quant Title : SFAM01.0
QLast Update : Mon May 01 00:14:49 2023
Response via : Initial Calibration

