

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042923\
 Data File : VD075921.D
 Acq On : 29 Apr 2023 17:20
 Operator : KP/SY
 Sample : 02548-36
 Misc : 5.85G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DCCR6

Quant Time: May 01 00:17:36 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon May 01 00:14:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.775	114	477636	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117	490470	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.522	152	226992	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.275	65	191361	18.263	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	73.040%		
7) Chloroethane-d5	2.799	69	184184	20.344	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	81.360%		
11) 1,1-Dichloroethene-d2	3.916	65	45059	18.653	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	74.600%		
21) 2-Butanone-d5	6.987	46	60822	66.865	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	133.720%		
24) Chloroform-d	7.569	84	281359	23.556	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	94.240%		
26) 1,2-Dichloroethane-d4	8.234	65	128628	25.218	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	100.880%		
32) Benzene-d6	8.198	84	529903	18.537	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	74.160%		
36) 1,2-Dichloropropane-d6	9.210	67	171492	21.673	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	86.680%		
41) Toluene-d8	10.269	98	489344	18.284	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	73.120%		
43) trans-1,3-Dichloroprop...	10.528	79	68177	20.846	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	83.400%		
47) 2-Hexanone-d5	10.881	63	52699	55.314	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	110.620%		
56) 1,1,2,2-Tetrachloroeth...	12.651	84	165500	27.334	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	109.320%		
66) 1,2-Dichlorobenzene-d4	13.816	152	188820	23.517	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	94.080%		
Target Compounds					Qvalue	
13) Acetone	4.028	43	16007	20.563	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042923\
Data File : VD075921.D
Acq On : 29 Apr 2023 17:20
Operator : KP/SY
Sample : 02548-36
Misc : 5.85G/10.00ml/MSVOA_D/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
DCCR6

Quant Time: May 01 00:17:36 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Quant Title : SFAM01.0
QLast Update : Mon May 01 00:14:49 2023
Response via : Initial Calibration

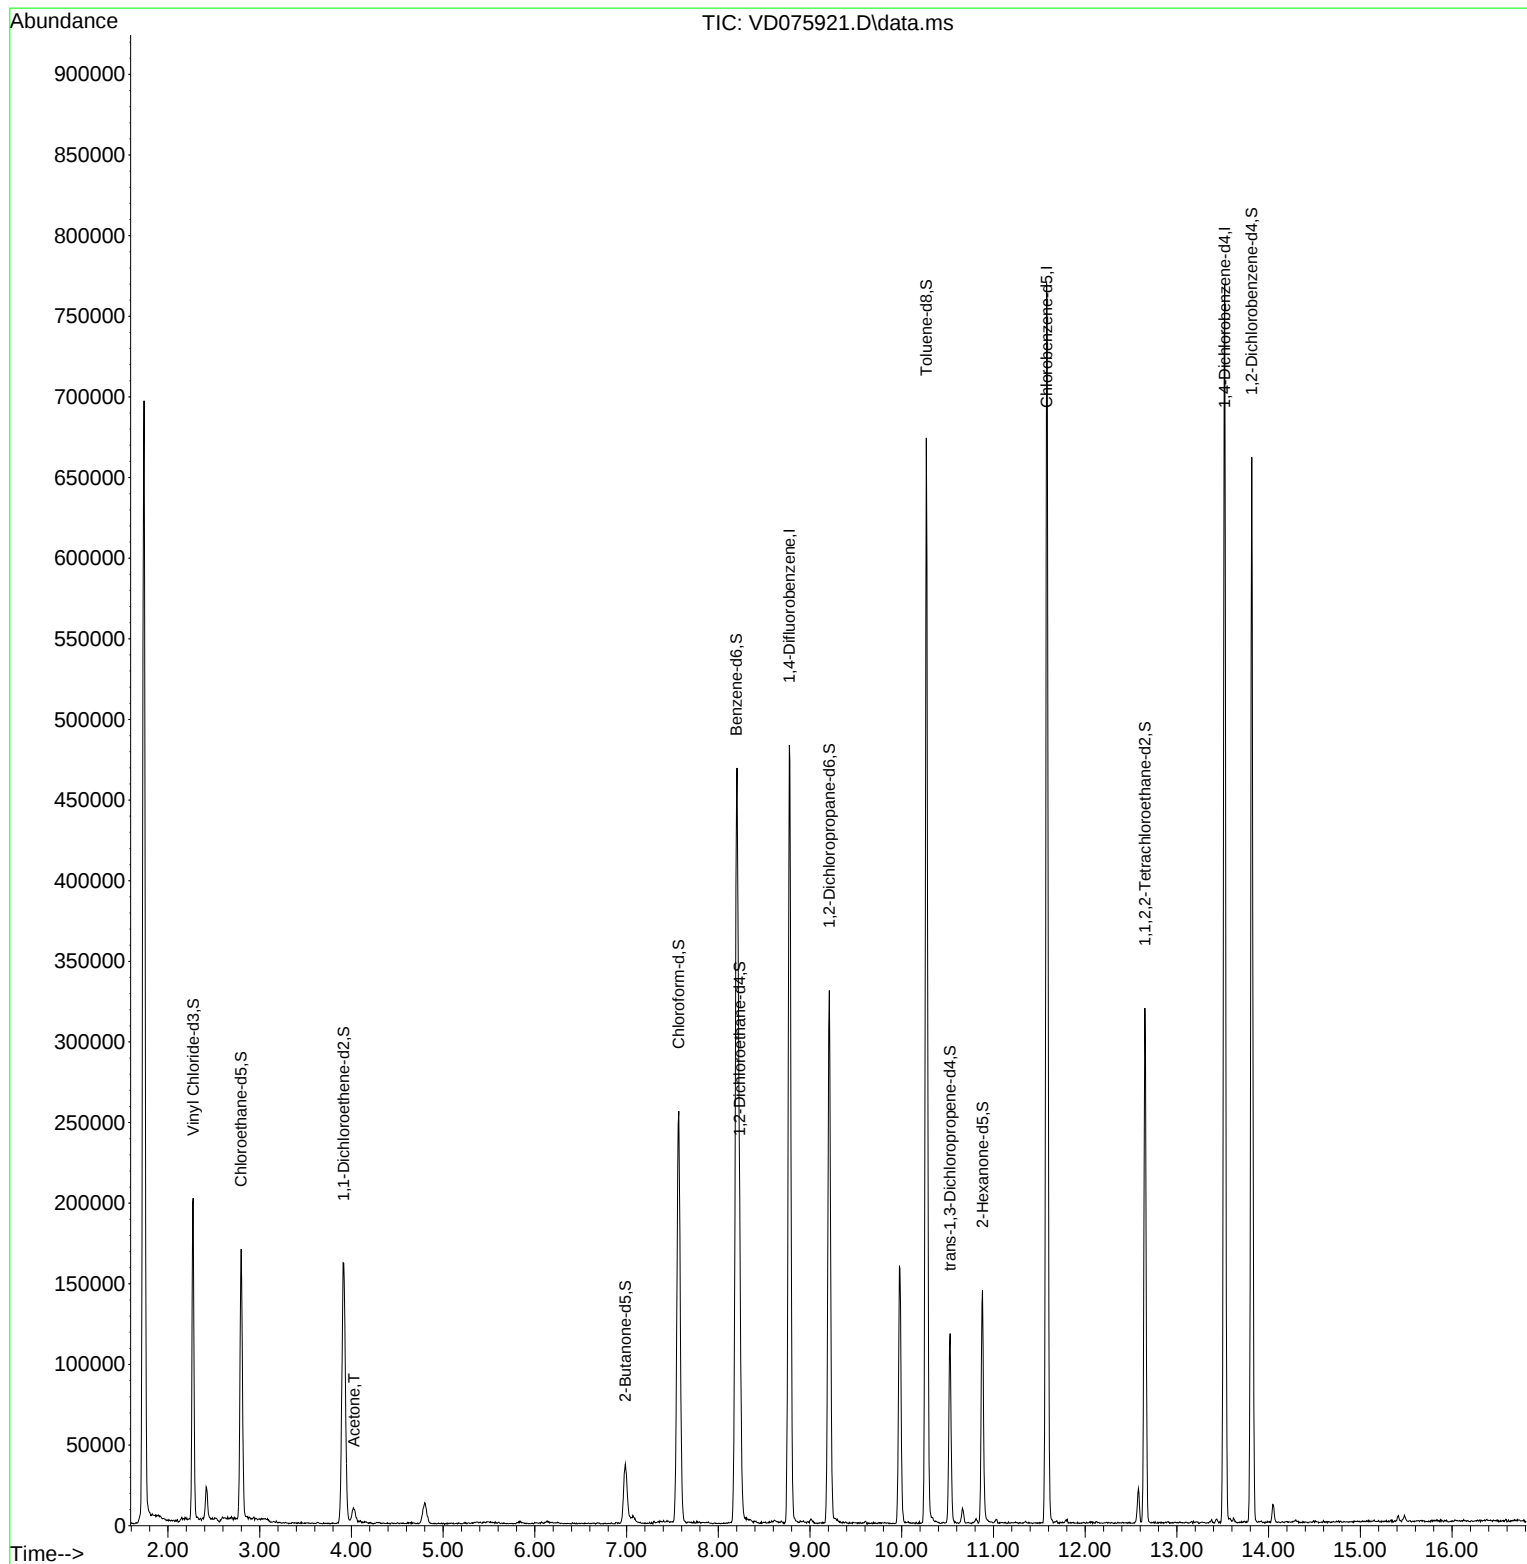

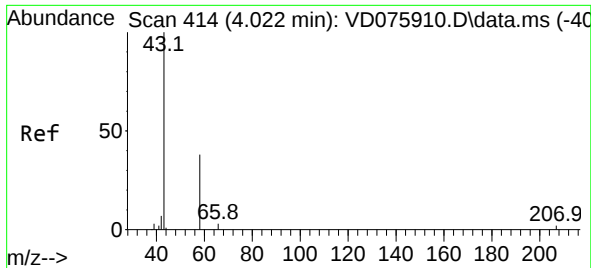

#13
 Acetone
 Concen: 20.563 ug/L
 RT: 4.028 min Scan# 41
 Delta R.T. 0.006 min
 Lab File: VD075921.D
 Acq: 29 Apr 2023 17:20

Instrument :
 MSVOA_D
 ClientSampleId :
 DCCR6

Tgt Ion: 43 Resp: 16007
 Ion Ratio Lower Upper
 43 100
 58 40.4 0.0 87.4

