

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042923\
 Data File : VD075914.D
 Acq On : 29 Apr 2023 13:54
 Operator : KP/SY
 Sample : 02548-45
 Misc : 4.30G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DCCT0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Title : SFAM01.0

Signal : TIC: VD075914.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.740	14	26	36	rBV	704255	1381982	100.00%	12.555%
2	2.275	111	117	129	rVB	243435	360444	26.08%	3.275%
3	2.805	200	207	216	rVB	185833	345567	25.01%	3.139%
4	3.287	287	289	290	rBV	709	576	0.04%	0.005%
5	3.716	361	362	367	rBV2	734	677	0.05%	0.006%
6	3.822	378	380	383	rVB2	753	556	0.04%	0.005%
7	3.916	383	396	407	rBV	188941	500370	36.21%	4.546%
8	4.010	410	412	413	rBV2	1262	945	0.07%	0.009%
9	4.146	431	435	436	rVB2	628	605	0.04%	0.005%
10	4.252	451	453	455	rBV2	537	534	0.04%	0.005%
11	4.281	455	458	461	rBV3	824	948	0.07%	0.009%
12	4.305	461	462	465	rVB	792	462	0.03%	0.004%
13	4.375	472	474	478	rVB3	637	529	0.04%	0.005%
14	4.410	478	480	484	rBV2	633	729	0.05%	0.007%
15	4.552	503	504	507	rBV2	727	464	0.03%	0.004%
16	4.799	535	546	557	rBV3	15125	48798	3.53%	0.443%
17	4.910	564	565	568	rVB	825	507	0.04%	0.005%
18	4.952	570	572	574	rBV2	797	797	0.06%	0.007%
19	5.246	620	622	625	rBV2	712	734	0.05%	0.007%
20	5.357	639	641	644	rVB2	683	664	0.05%	0.006%
21	5.387	644	646	648	rBV2	540	640	0.05%	0.006%
22	5.587	678	680	682	rBV	524	482	0.03%	0.004%
23	5.728	703	704	707	rVB	759	528	0.04%	0.005%
24	5.752	707	708	712	rBV2	459	474	0.03%	0.004%
25	5.793	712	715	716	rBV	653	489	0.04%	0.004%
26	5.981	746	747	750	rBV2	565	558	0.04%	0.005%
27	6.163	775	778	779	rBV	554	502	0.04%	0.005%
28	6.204	783	785	788	rBV2	746	701	0.05%	0.006%
29	6.316	801	804	807	rBV2	754	1054	0.08%	0.010%
30	6.499	830	835	839	rBV2	488	955	0.07%	0.009%
31	6.552	841	844	847	rBV	605	527	0.04%	0.005%
32	6.663	860	863	865	rBV	517	601	0.04%	0.005%
33	6.699	867	869	870	rBV	740	457	0.03%	0.004%
34	6.993	908	919	927	rBV	21658	63124	4.57%	0.573%
35	7.216	954	957	959	rBV	483	489	0.04%	0.004%
36	7.340	974	978	980	rBV2	597	693	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042923\
 Data File : VD075914.D
 Acq On : 29 Apr 2023 13:54
 Operator : KP/SY
 Sample : 02548-45
 Misc : 4.30G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DCCT0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Title : SFAM01.0

37	7.381	983	985	987	rBV2	706	793	0.06%	0.007%
38	7.434	992	994	997	rBV	730	692	0.05%	0.006%
39	7.463	997	999	1003	rVB3	873	1088	0.08%	0.010%
40	7.569	1006	1017	1027	rBV	228106	581242	42.06%	5.280%
41	7.693	1035	1038	1039	rBV2	752	682	0.05%	0.006%
42	7.940	1077	1080	1082	rBV	738	796	0.06%	0.007%
43	8.087	1103	1105	1108	rVB	682	461	0.03%	0.004%
44	8.204	1114	1125	1142	rBV2	472934	1344818	97.31%	12.217%
45	8.393	1156	1157	1160	rBV3	985	908	0.07%	0.008%
46	8.528	1176	1180	1182	rBV2	841	946	0.07%	0.009%
47	8.557	1182	1185	1188	rVV2	1181	1212	0.09%	0.011%
48	8.598	1190	1192	1193	rVV2	1063	738	0.05%	0.007%
49	8.616	1193	1195	1199	rVV3	1379	1688	0.12%	0.015%
50	8.646	1199	1200	1204	rVB2	1274	975	0.07%	0.009%
51	8.781	1212	1223	1234	rBV	421638	861154	62.31%	7.823%
52	9.016	1261	1263	1264	rBV	1349	696	0.05%	0.006%
53	9.063	1270	1271	1273	rBV	674	487	0.04%	0.004%
54	9.210	1288	1296	1308	rBV	291627	595512	43.09%	5.410%
55	9.410	1329	1330	1333	rBV	742	704	0.05%	0.006%
56	9.434	1333	1334	1335	rVV	976	452	0.03%	0.004%
57	9.451	1335	1337	1339	rVV	934	847	0.06%	0.008%
58	9.498	1342	1345	1347	rBV	375	483	0.03%	0.004%
59	9.651	1368	1371	1374	rBV2	610	1064	0.08%	0.010%
60	9.681	1374	1376	1379	rVB2	949	943	0.07%	0.009%
61	9.810	1392	1398	1399	rBV3	852	1245	0.09%	0.011%
62	9.863	1405	1407	1408	rVB	798	526	0.04%	0.005%
63	9.910	1412	1415	1418	rBV2	594	857	0.06%	0.008%
64	9.981	1419	1427	1438	rBV2	146357	273728	19.81%	2.487%
65	10.187	1460	1462	1463	rVV	897	451	0.03%	0.004%
66	10.269	1468	1476	1489	rBV	693860	1219840	88.27%	11.082%
67	10.528	1513	1520	1529	rBV	96039	166214	12.03%	1.510%
68	10.622	1534	1536	1537	rBV	843	528	0.04%	0.005%
69	10.669	1539	1544	1549	rVV3	4928	9030	0.65%	0.082%
70	10.804	1565	1567	1568	rBV	512	464	0.03%	0.004%
71	10.881	1573	1580	1592	rVV	85320	145738	10.55%	1.324%
72	11.228	1636	1639	1641	rBV2	903	1208	0.09%	0.011%
73	11.298	1649	1651	1652	rBV2	687	529	0.04%	0.005%
74	11.345	1658	1659	1665	rVB	1514	1669	0.12%	0.015%
75	11.434	1673	1674	1676	rBV	735	652	0.05%	0.006%
76	11.534	1689	1691	1692	rBV	813	766	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042923\
 Data File : VD075914.D
 Acq On : 29 Apr 2023 13:54
 Operator : KP/SY
 Sample : 02548-45
 Misc : 4.30G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DCCT0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Title : SFAM01.0

77	11.581	1692	1699	1712	rVB	593423	1005821	72.78%	9.138%
78	12.051	1777	1779	1783	rVB2	1870	1977	0.14%	0.018%
79	12.087	1783	1785	1787	rBV2	618	611	0.04%	0.006%
80	12.122	1789	1791	1792	rBV	709	454	0.03%	0.004%
81	12.157	1794	1797	1798	rBV	800	741	0.05%	0.007%
82	12.198	1803	1804	1806	rBV	611	468	0.03%	0.004%
83	12.263	1813	1815	1816	rBV2	738	467	0.03%	0.004%
84	12.304	1820	1822	1826	rVB2	1124	1407	0.10%	0.013%
85	12.339	1826	1828	1831	rBV	431	469	0.03%	0.004%
86	12.404	1838	1839	1841	rBV2	775	539	0.04%	0.005%
87	12.581	1860	1869	1875	rVB4	16579	28969	2.10%	0.263%
88	12.651	1875	1881	1890	rVB	201073	338860	24.52%	3.078%
89	12.734	1890	1895	1897	rBV3	1276	1614	0.12%	0.015%
90	12.904	1921	1924	1926	rBV2	729	668	0.05%	0.006%
91	13.257	1982	1984	1986	rBV	1111	688	0.05%	0.006%
92	13.522	2022	2029	2036	rBV	517482	820666	59.38%	7.456%
93	13.734	2062	2065	2067	rBV2	996	1170	0.08%	0.011%
94	13.816	2072	2079	2091	rBV	496147	823155	59.56%	7.478%
95	13.975	2104	2106	2107	rBV	904	560	0.04%	0.005%
96	14.051	2114	2119	2128	rBV2	12765	21259	1.54%	0.193%
97	14.151	2135	2136	2138	rBV	1675	959	0.07%	0.009%
98	15.051	2287	2289	2291	rBV2	1031	799	0.06%	0.007%
99	15.410	2347	2350	2354	rBV2	4458	5734	0.41%	0.052%
100	15.475	2359	2361	2367	rVB4	4389	7322	0.53%	0.067%




Sum of corrected areas: 11007365

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042923\
Data File : VD075914.D
Acq On : 29 Apr 2023 13:54
Operator : KP/SY
Sample : 02548-45
Misc : 4.30G/10.00ml/MSVOA_D/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
DCCT0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Quant Title : SFAM01.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

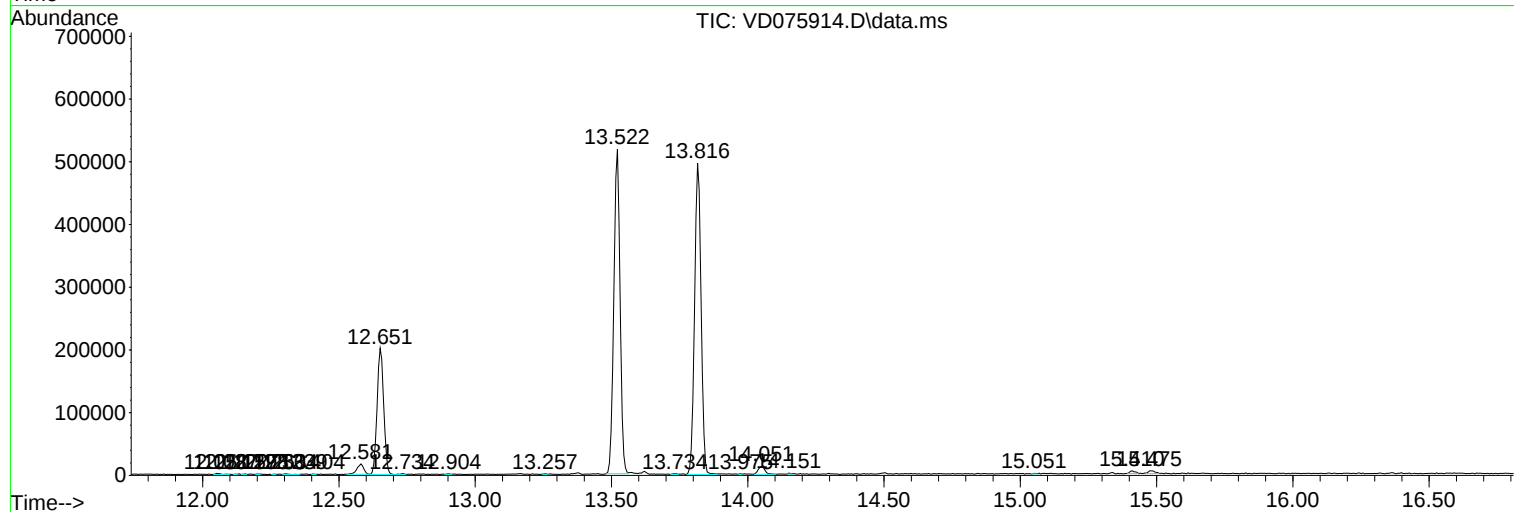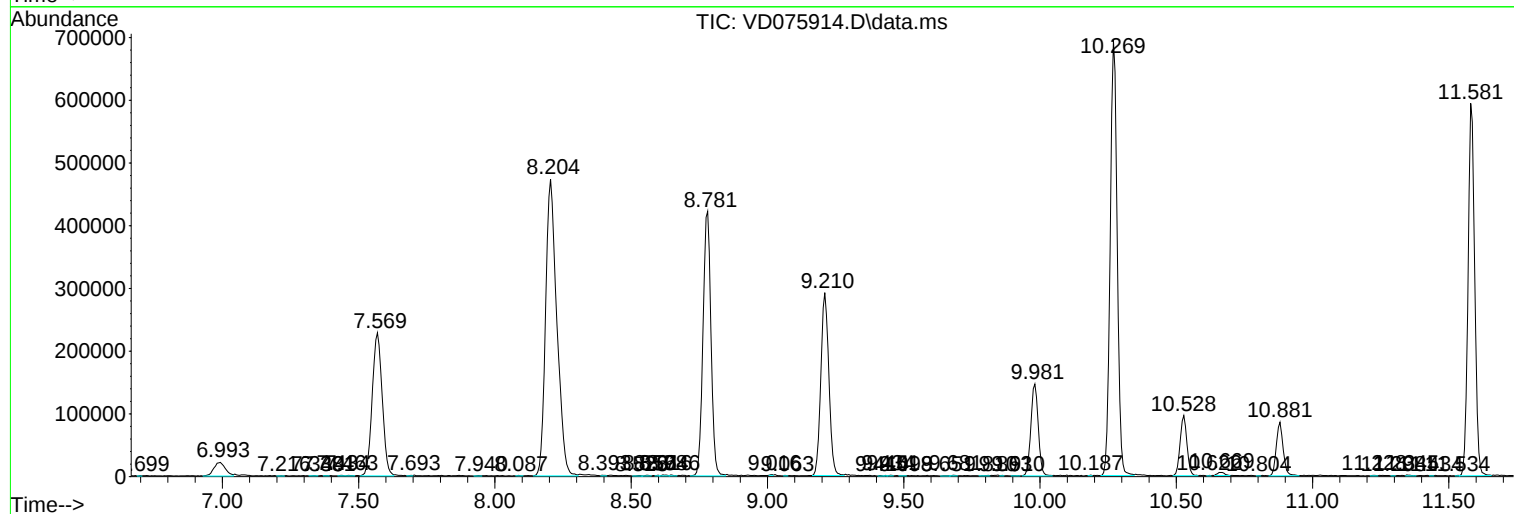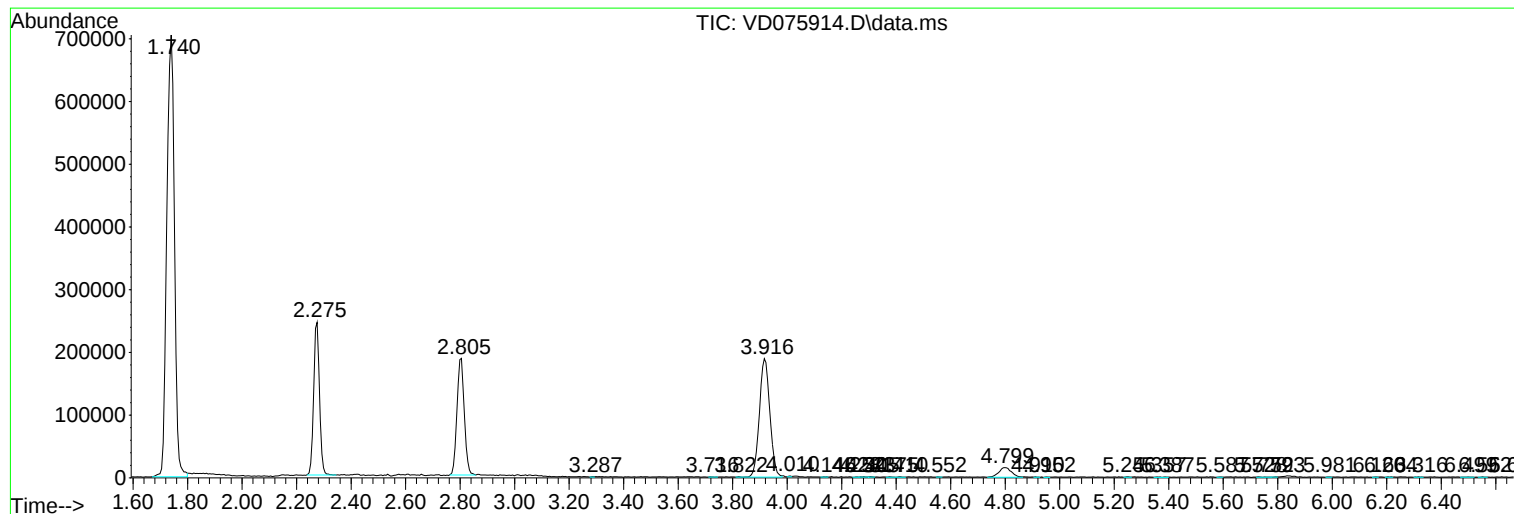

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042923\
Data File : VD075914.D
Acq On : 29 Apr 2023 13:54
Operator : KP/SY
Sample : 02548-45
Misc : 4.30G/10.00ml/MSVOA_D/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
DCCT0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Quant Title : SFAM01.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042923\
Data File : VD075914.D
Acq On : 29 Apr 2023 13:54
Operator : KP/SY
Sample : 02548-45
Misc : 4.30G/10.00ml/MSVOA_D/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
DCCT0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Quant Title : SFAM01.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------