

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042923\
 Data File : VD075916.D
 Acq On : 29 Apr 2023 14:53
 Operator : KP/SY
 Sample : 02525-06
 Misc : 5.52G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DCCC6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Title : SFAM01.0

Signal : TIC: VD075916.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.740	14	26	37	rBV	765947	1477062	100.00%	11.557%
2	2.275	111	117	127	rVB	202734	295920	20.03%	2.315%
3	2.422	137	142	148	rVB	20703	34483	2.33%	0.270%
4	2.599	167	172	173	rBV2	2856	4118	0.28%	0.032%
5	2.799	199	206	218	rBV	166999	311913	21.12%	2.440%
6	3.181	269	271	274	rBV2	898	922	0.06%	0.007%
7	3.317	291	294	297	rBV2	463	705	0.05%	0.006%
8	3.387	305	306	309	rBV2	509	462	0.03%	0.004%
9	3.722	360	363	364	rBV2	655	642	0.04%	0.005%
10	3.758	367	369	371	rVB2	766	641	0.04%	0.005%
11	3.840	380	383	385	rBV	591	660	0.04%	0.005%
12	3.917	385	396	408	rBV	171668	441189	29.87%	3.452%
13	4.028	408	415	424	rVB	13910	38876	2.63%	0.304%
14	4.152	434	436	438	rBV2	998	838	0.06%	0.007%
15	4.440	482	485	486	rBV2	487	493	0.03%	0.004%
16	4.458	486	488	489	rVB	939	475	0.03%	0.004%
17	4.481	491	492	494	rBV2	579	474	0.03%	0.004%
18	4.575	507	508	511	rVV2	498	441	0.03%	0.003%
19	4.722	532	533	537	rVB2	527	462	0.03%	0.004%
20	4.799	537	546	557	rBV4	11493	36513	2.47%	0.286%
21	4.899	560	563	566	rBV	768	858	0.06%	0.007%
22	4.940	568	570	573	rVB3	818	596	0.04%	0.005%
23	4.975	573	576	577	rVB	812	493	0.03%	0.004%
24	4.993	577	579	581	rBV2	483	500	0.03%	0.004%
25	5.116	597	600	602	rBV2	541	512	0.03%	0.004%
26	5.269	622	626	627	rVB2	783	851	0.06%	0.007%
27	5.328	634	636	639	rBV	598	701	0.05%	0.005%
28	5.411	648	650	652	rBV	523	486	0.03%	0.004%
29	5.440	652	655	656	rVV2	671	599	0.04%	0.005%
30	5.487	662	663	666	rBV2	505	525	0.04%	0.004%
31	5.569	675	677	683	rVB2	692	843	0.06%	0.007%
32	5.793	712	715	717	rBV	618	829	0.06%	0.006%
33	5.822	719	720	722	rBV2	1160	963	0.07%	0.008%
34	6.105	766	768	771	rVB2	517	498	0.03%	0.004%
35	6.293	798	800	803	rBV2	549	628	0.04%	0.005%
36	6.363	810	812	815	rVB	990	736	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042923\
 Data File : VD075916.D
 Acq On : 29 Apr 2023 14:53
 Operator : KP/SY
 Sample : 02525-06
 Misc : 5.52G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DCCC6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Title : SFAM01.0

37	6.387	815	816	819	rBV3	734	693	0.05%	0.005%
38	6.428	819	823	825	rVV2	645	795	0.05%	0.006%
39	6.569	844	847	848	rBV2	412	460	0.03%	0.004%
40	6.734	872	875	876	rBV	765	553	0.04%	0.004%
41	6.810	887	888	890	rBV	586	457	0.03%	0.004%
42	6.887	897	901	902	rVB	471	502	0.03%	0.004%
43	6.916	904	906	907	rBV	799	611	0.04%	0.005%
44	6.987	907	918	930	rBV	36768	106888	7.24%	0.836%
45	7.163	945	948	949	rBV	554	503	0.03%	0.004%
46	7.263	963	965	968	rVB2	472	525	0.04%	0.004%
47	7.310	969	973	976	rBV2	559	631	0.04%	0.005%
48	7.334	976	977	982	rVB2	503	593	0.04%	0.005%
49	7.452	995	997	1000	rVB2	927	932	0.06%	0.007%
50	7.493	1000	1004	1005	rBV	806	690	0.05%	0.005%
51	7.569	1007	1017	1030	rVV2	251955	653498	44.24%	5.113%
52	7.810	1054	1058	1060	rBV2	491	593	0.04%	0.005%
53	8.057	1098	1100	1102	rBV	558	593	0.04%	0.005%
54	8.205	1114	1125	1140	rBV2	470568	1406839	95.25%	11.007%
55	8.516	1176	1178	1181	rVB	586	559	0.04%	0.004%
56	8.546	1181	1183	1185	rBV	804	521	0.04%	0.004%
57	8.781	1214	1223	1233	rVV	512458	1024793	69.38%	8.018%
58	8.981	1254	1257	1260	rBV2	929	1258	0.09%	0.010%
59	9.016	1260	1263	1269	rVV2	2544	3512	0.24%	0.027%
60	9.210	1288	1296	1305	rBV	329946	682757	46.22%	5.342%
61	9.481	1340	1342	1347	rVB	1279	1755	0.12%	0.014%
62	9.557	1354	1355	1359	rBV2	534	477	0.03%	0.004%
63	9.604	1359	1363	1367	rBV2	920	1549	0.10%	0.012%
64	9.646	1367	1370	1373	rBV2	692	808	0.05%	0.006%
65	9.669	1373	1374	1376	rBV	755	472	0.03%	0.004%
66	9.981	1420	1427	1435	rBV	164892	308071	20.86%	2.410%
67	10.099	1446	1447	1450	rBV2	864	946	0.06%	0.007%
68	10.269	1468	1476	1486	rBV	669748	1204908	81.57%	9.427%
69	10.469	1506	1510	1511	rVB2	991	1025	0.07%	0.008%
70	10.528	1513	1520	1527	rVV	113312	197824	13.39%	1.548%
71	10.669	1539	1544	1549	rVB3	8130	14602	0.99%	0.114%
72	10.881	1573	1580	1589	rBV	145604	245585	16.63%	1.921%
73	11.075	1612	1613	1614	rBV	1070	489	0.03%	0.004%
74	11.351	1658	1660	1666	rVB2	1585	2072	0.14%	0.016%
75	11.393	1666	1667	1669	rBV	1010	634	0.04%	0.005%
76	11.451	1675	1677	1680	rVB2	717	573	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042923\
 Data File : VD075916.D
 Acq On : 29 Apr 2023 14:53
 Operator : KP/SY
 Sample : 02525-06
 Misc : 5.52G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DCCC6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Title : SFAM01.0

77	11.475	1680	1681	1682	rBV	1093	444	0.03%	0.003%
78	11.581	1692	1699	1711	rBV	774188	1334133	90.32%	10.438%
79	11.781	1731	1733	1734	rBV	1811	1133	0.08%	0.009%
80	11.840	1742	1743	1745	rBV	720	600	0.04%	0.005%
81	12.051	1777	1779	1782	rBV2	701	914	0.06%	0.007%
82	12.198	1802	1804	1806	rBV2	641	601	0.04%	0.005%
83	12.240	1809	1811	1814	rBV	646	811	0.05%	0.006%
84	12.581	1863	1869	1874	rVV2	21441	33606	2.28%	0.263%
85	12.651	1874	1881	1889	rVB	306252	510508	34.56%	3.994%
86	12.775	1901	1902	1904	rBV	660	495	0.03%	0.004%
87	12.904	1920	1924	1928	rBV2	1848	2189	0.15%	0.017%
88	13.057	1948	1950	1954	rBV	783	1215	0.08%	0.010%
89	13.428	2010	2013	2016	rBV3	3980	4889	0.33%	0.038%
90	13.522	2021	2029	2037	rVV	795151	1265744	85.69%	9.903%
91	13.616	2040	2045	2049	rVB4	1813	3153	0.21%	0.025%
92	13.681	2055	2056	2058	rBV2	1042	614	0.04%	0.005%
93	13.816	2072	2079	2089	rVB	657449	1058151	71.64%	8.279%
94	14.051	2114	2119	2125	rVB2	11862	18948	1.28%	0.148%
95	14.298	2158	2161	2165	rBV3	2525	3243	0.22%	0.025%
96	14.345	2167	2169	2170	rBV	841	572	0.04%	0.004%
97	14.492	2193	2194	2195	rBV	1367	646	0.04%	0.005%
98	15.416	2346	2351	2354	rVB3	4853	7495	0.51%	0.059%
99	15.569	2376	2377	2379	rBV	1132	955	0.06%	0.007%
100	16.598	2551	2552	2553	rBV	1218	479	0.03%	0.004%




Sum of corrected areas: 12780991

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042923\
Data File : VD075916.D
Acq On : 29 Apr 2023 14:53
Operator : KP/SY
Sample : 02525-06
Misc : 5.52G/10.00ml/MSVOA_D/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
DCCC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Quant Title : SFAM01.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

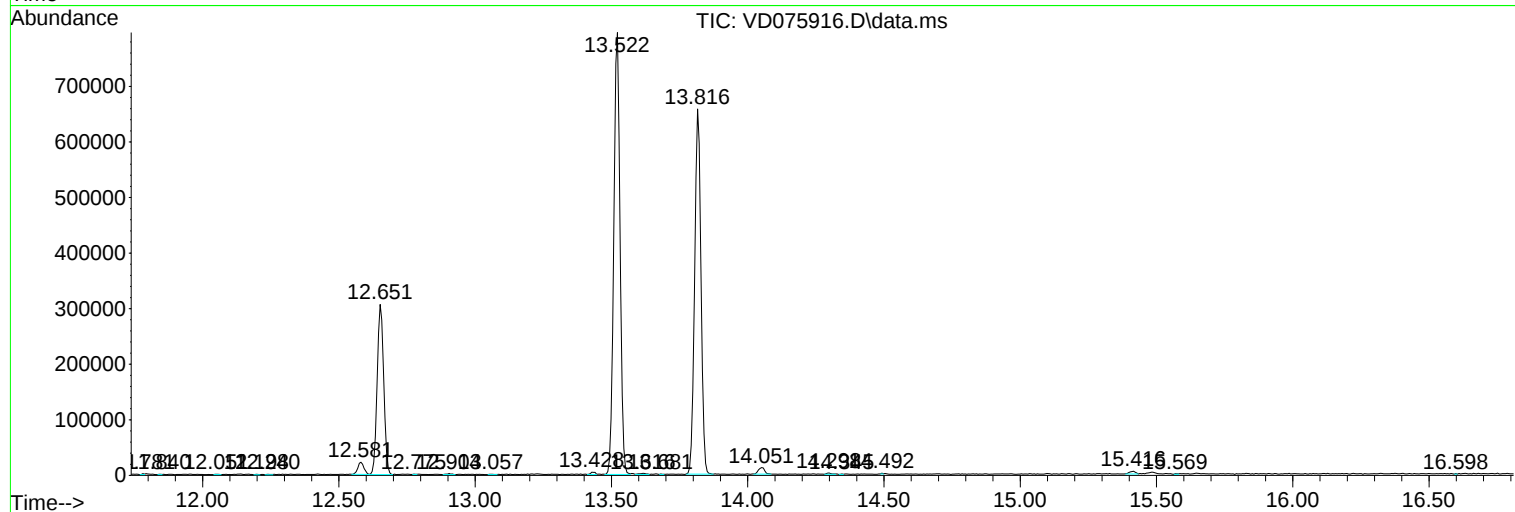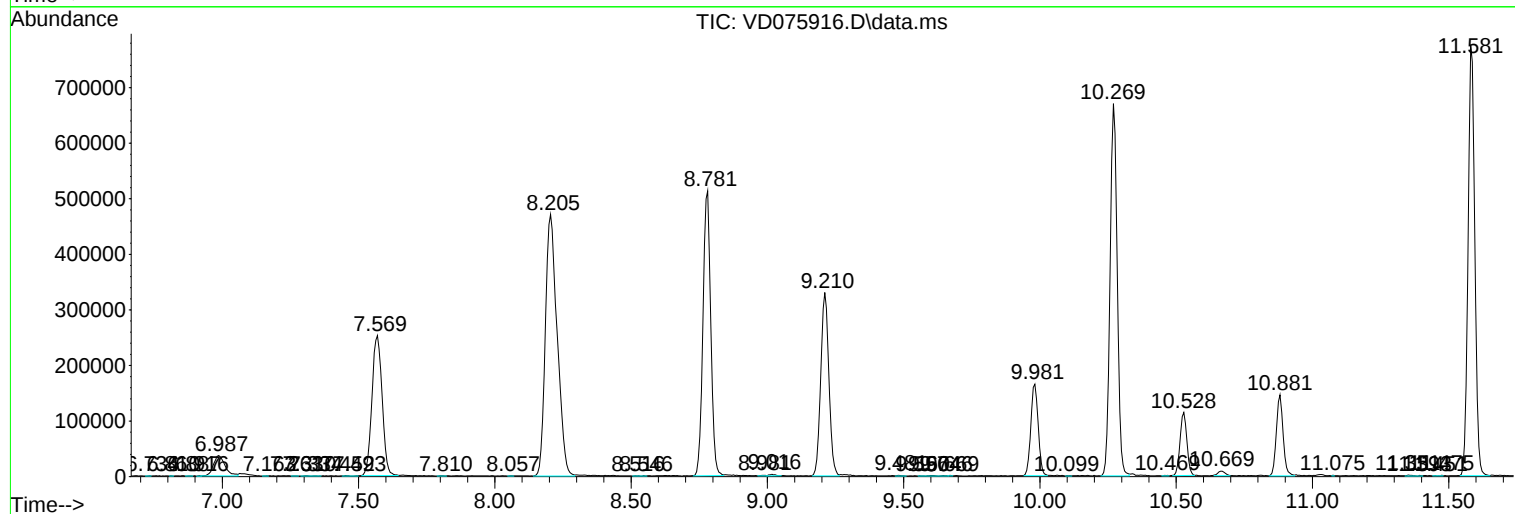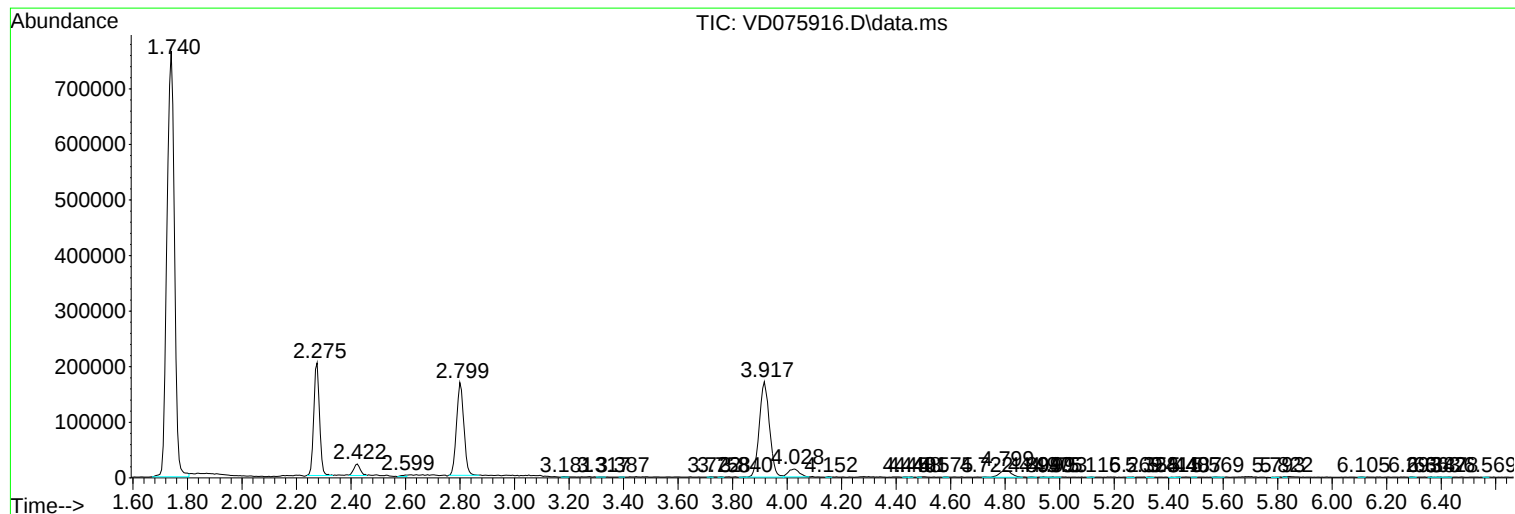

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042923\
Data File : VD075916.D
Acq On : 29 Apr 2023 14:53
Operator : KP/SY
Sample : 02525-06
Misc : 5.52G/10.00ml/MSVOA_D/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
DCCC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Quant Title : SFAM01.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042923\
Data File : VD075916.D
Acq On : 29 Apr 2023 14:53
Operator : KP/SY
Sample : 02525-06
Misc : 5.52G/10.00ml/MSVOA_D/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
DCCC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Quant Title : SFAM01.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc