


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042923\
Data File : VD075909.D
Acq On : 29 Apr 2023 11:19
Operator : KP/SY
Sample : BFB122
Misc : 5.00G/10.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB122

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Title : SFAM01.0
Last Update : Mon May 01 00:14:49 2023

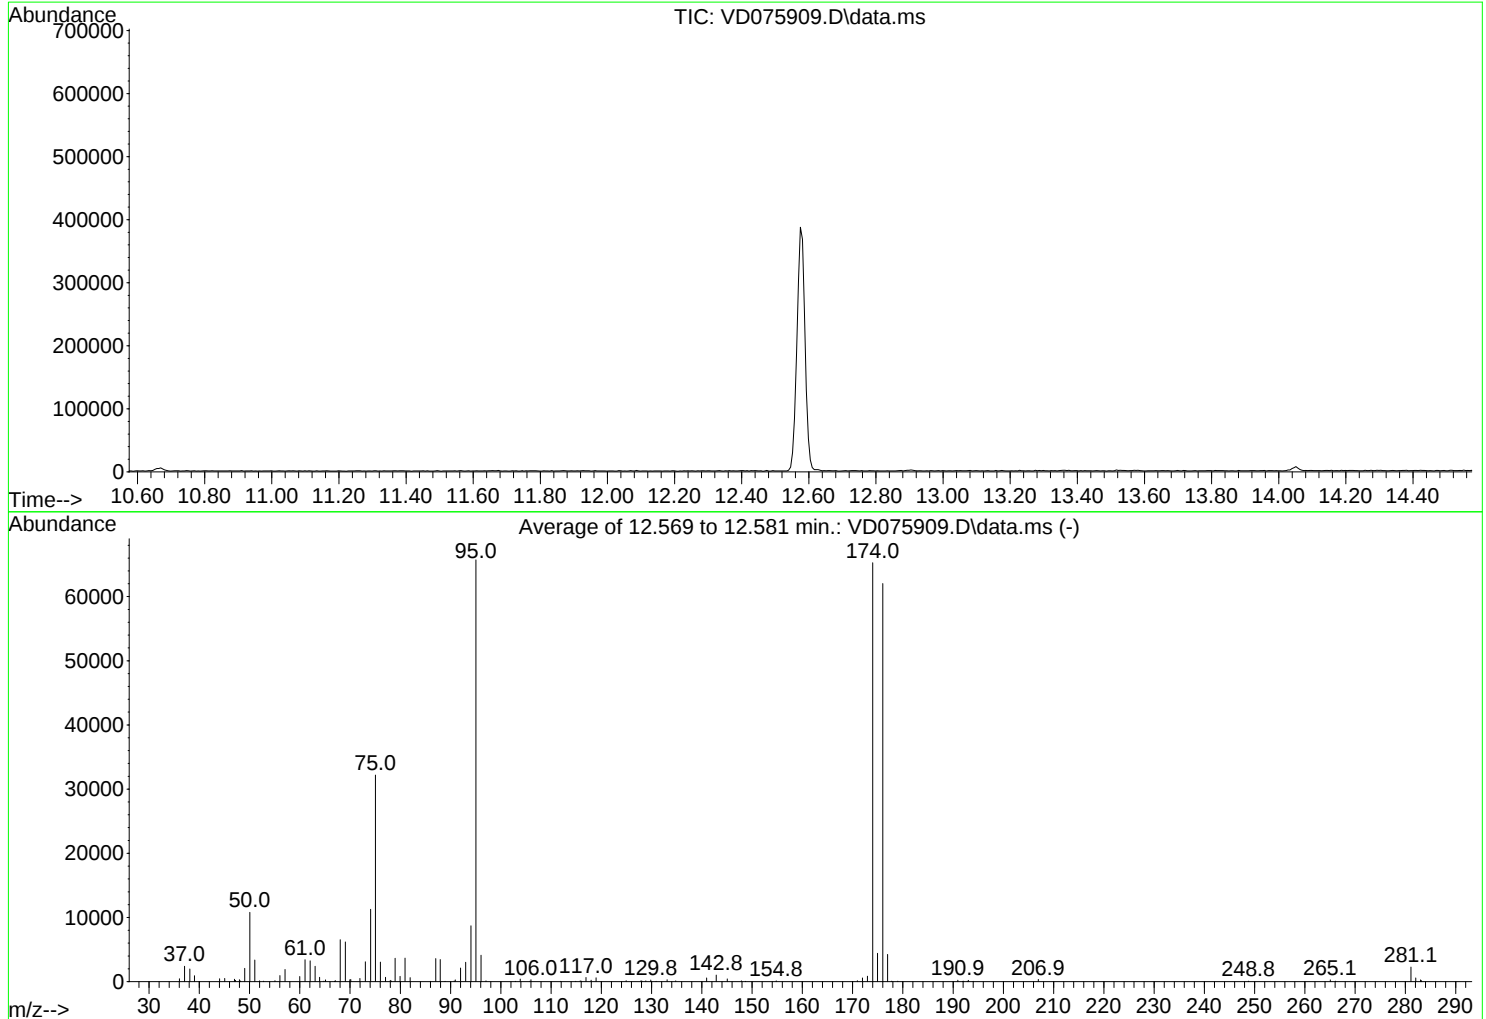

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	10804	PASS
75	95	30	80	49.0	32203	PASS
95	95	100	100	100.0	65728	PASS
96	95	5	9	6.3	4108	PASS
173	174	0.00	2	1.3	860	PASS
174	95	50	120	99.3	65283	PASS
175	174	5	9	6.8	4411	PASS
176	174	95	105	95.0	62035	PASS
177	176	5	10	6.8	4231	PASS

m/z	Abundance
40.10	913.0
44.00	614.0

Instrument :
MSVOA_D
ClientSampleId :
BFB122

m/z	Abundance
36.00	383.0
37.10	2161.0
38.10	1660.0
39.10	830.0
40.10	1032.0
44.20	928.0
45.00	400.0
47.00	560.0
48.00	402.0
49.10	1615.0
50.00	9764.0
51.10	3191.0
56.00	898.0
57.10	1288.0
60.00	580.0
61.00	2921.0
62.10	2890.0
63.00	1923.0
63.90	687.0
64.80	194.0
66.90	209.0
68.00	5872.0
69.00	5381.0
69.90	298.0
70.30	292.0
71.90	496.0
73.00	2503.0
74.10	10099.0
75.00	28896.0
76.10	2799.0
77.10	555.0
78.10	319.0
79.00	3526.0
79.90	635.0
80.90	3060.0
82.00	657.0
87.00	3133.0
88.00	2957.0
88.90	150.0
90.70	284.0
92.00	1964.0
93.00	2540.0
94.10	7743.0
95.10	56856.0
96.00	3755.0
103.90	450.0
105.80	208.0
117.00	614.0
118.90	532.0
127.90	199.0
128.90	216.0
129.80	393.0
133.20	244.0
141.00	389.0
142.80	994.0
145.00	363.0
147.80	203.0
172.10	436.0
173.00	852.0
174.00	54400.0
175.00	3801.0
176.00	51744.0
176.90	3327.0
177.80	192.0
191.10	202.0
192.80	247.0
207.00	409.0
265.00	155.0
281.10	1493.0
282.00	485.0
283.00	382.0

Instrument :
MSVOA_D
ClientSampleId :
BFB122

m/z	Abundance
36.10	361.0
37.10	2567.0
38.10	2168.0
39.00	1010.0
40.00	934.0
44.10	1052.0
45.10	484.0
47.00	569.0
48.00	473.0
49.10	2216.0
50.00	11848.0
51.10	3964.0
52.00	413.0
52.80	219.0
55.00	281.0
56.00	1017.0
57.10	2244.0
60.10	918.0
61.10	3757.0
62.00	3187.0
63.00	2724.0
64.00	745.0
65.10	357.0
67.10	453.0
68.00	6749.0
69.10	6402.0
70.10	720.0
72.00	332.0
73.10	3997.0
74.10	12192.0
75.10	34888.0
76.10	3608.0
77.00	671.0
77.90	325.0
79.00	3878.0
80.00	858.0
81.00	4322.0
82.00	647.0
86.00	188.0
87.10	4028.0
88.00	3790.0
90.90	532.0
92.00	2425.0
93.00	3489.0
94.00	9141.0
95.00	72872.0
96.10	4505.0
97.00	254.0
103.80	416.0
106.00	458.0
116.10	249.0
116.90	523.0
118.00	431.0
119.00	693.0
124.90	176.0
127.90	225.0
128.80	161.0
129.90	208.0
130.90	165.0
133.20	168.0
134.90	156.0
140.90	709.0
142.90	1097.0
145.10	625.0
147.90	210.0
148.70	158.0
154.80	172.0
170.90	198.0
171.90	681.0
173.00	763.0
174.00	71000.0
174.90	4549.0
176.00	69392.0
176.90	5097.0
190.90	205.0
191.90	159.0
193.10	283.0
206.90	278.0
265.10	288.0
281.10	2267.0
282.10	682.0
283.00	479.0

Instrument :
MSVOA_D
ClientSampleId :
BFB122

m/z	Abundance
36.00	623.0
37.00	2436.0
38.10	2065.0
39.00	916.0
40.10	858.0
44.10	1232.0
45.00	619.0
47.20	575.0
48.20	306.0
49.00	2404.0
50.10	10801.0
51.00	2947.0
55.10	178.0
56.10	899.0
57.00	2150.0
59.90	880.0
61.00	3587.0
62.00	3656.0
63.10	2555.0
64.00	587.0
65.10	475.0
68.10	7013.0
69.10	6799.0
70.00	949.0
71.90	637.0
73.00	2780.0
74.10	11530.0
75.10	32824.0
76.00	2709.0
77.10	785.0
78.20	287.0
78.90	3536.0
79.90	977.0
81.00	3626.0
81.90	564.0
87.00	3592.0
87.90	3602.0
91.00	300.0
92.00	1977.0
93.00	3033.0
94.00	9223.0
95.10	67456.0
96.10	4065.0
97.10	152.0
102.90	186.0
103.80	300.0
106.00	447.0
111.90	157.0
114.90	164.0
115.80	359.0
117.00	827.0
117.80	226.0
118.90	563.0
125.00	303.0
128.10	233.0
129.80	176.0
133.00	478.0
134.70	192.0
140.90	614.0
142.90	1013.0
145.00	318.0
154.80	194.0
171.00	288.0
171.90	584.0
172.80	966.0
174.00	70448.0
175.00	4884.0
176.00	64968.0
177.00	4270.0
179.00	192.0
190.90	298.0
192.10	202.0
193.00	353.0
194.00	162.0
207.00	337.0
248.80	216.0
265.10	387.0
266.10	234.0
281.10	3026.0
282.10	561.0
283.20	484.0

Instrument :
MSVOA_D
ClientSampleId :
BFB122