


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD050119\
 Data File : VD062095.D
 Acq On : 1 May 2019 9:47
 Operator : FY/SY
 Sample : BFB
 Misc : 5.00g/5mL/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D042319S.M
 Title : SW846 8260
 Last Update : Thu May 02 07:55:52 2019

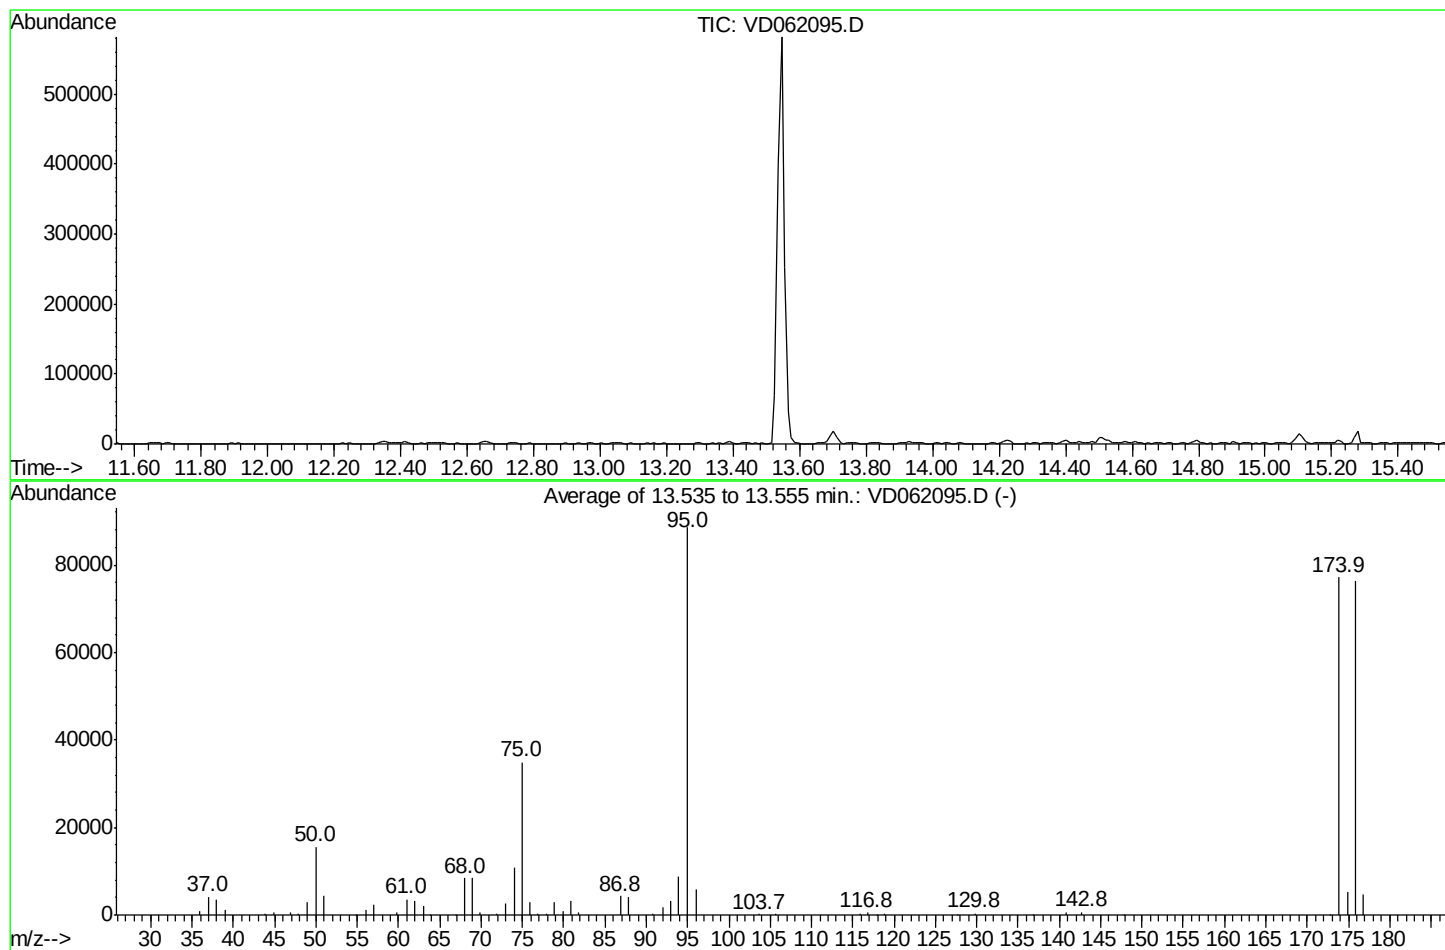

AutoFind: Scans 1230, 1231, 1232; Background Corrected with Scan 1225

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	15616	PASS
75	95	30	60	39.4	34866	PASS
95	95	100	100	100.0	88586	PASS
96	95	5	9	6.7	5941	PASS
173	174	0.00	2	0.1	106	PASS
174	95	50	100	87.1	77144	PASS
175	174	5	9	6.8	5254	PASS
176	174	95	101	99.1	76480	PASS
177	176	5	9	6.0	4556	PASS