


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD050120\
 Data File : VD065686.D
 Acq On : 01 May 2020 16:31
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA D/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D050120S.M
 Title : SW846 8260
 Last Update : Mon May 04 10:28:10 2020

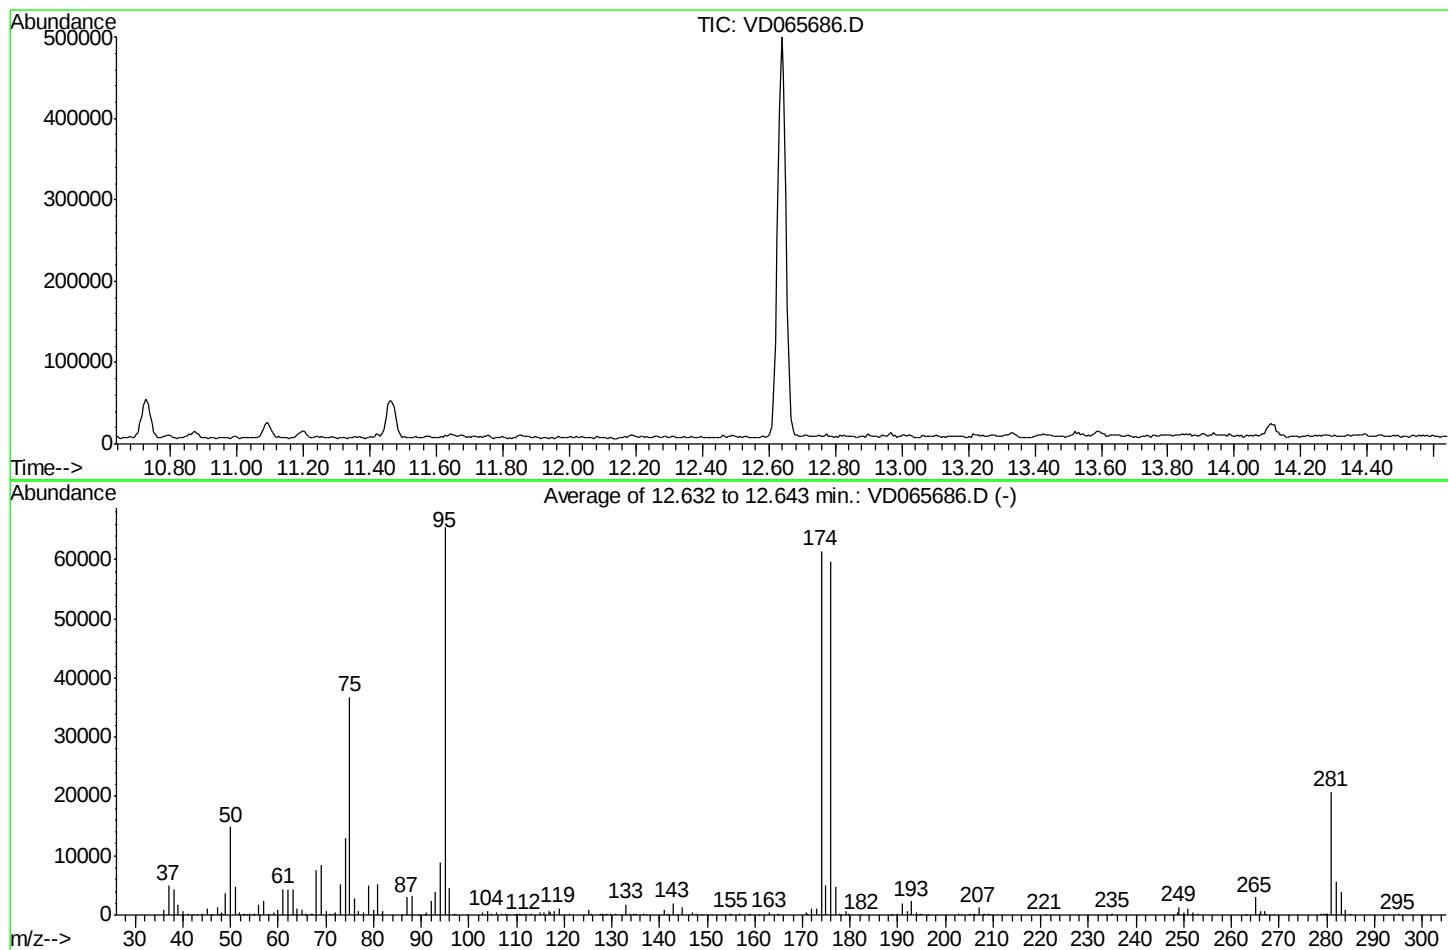

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1813

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.7	14867	PASS
75	95	30	60	56.2	36746	PASS
95	95	100	100	100.0	65442	PASS
96	95	5	9	6.9	4528	PASS
173	174	0.00	2	1.7	1074	PASS
174	95	50	100	93.9	61426	PASS
175	174	5	9	8.2	5025	PASS
176	174	95	101	97.3	59738	PASS
177	176	5	9	8.1	4814	PASS