


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD050219\
Data File : VD062107.D
Acq On : 2 May 2019 12:38
Operator : FY/SY
Sample : BFB
Misc : 5.00µ/5mL/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D042319S.M
Title : SW846 8260
Last Update : Thu May 02 07:55:52 2019

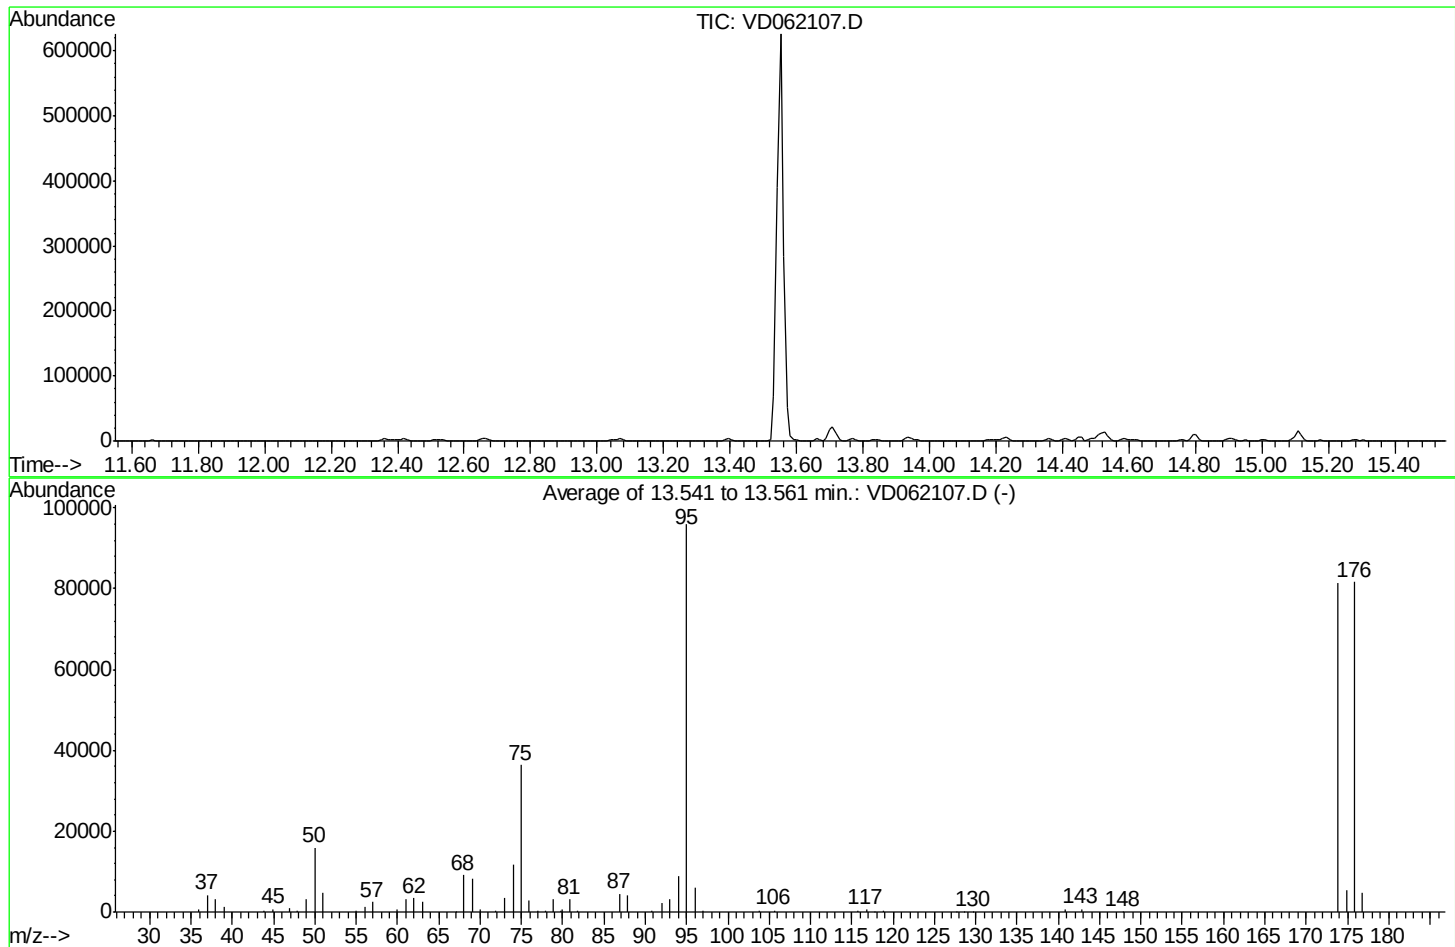

AutoFind: Scans 1231, 1232, 1233; Background Corrected with Scan 1226

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	15919	PASS
75	95	30	60	37.9	36357	PASS
95	95	100	100	100.0	95930	PASS
96	95	5	9	6.3	6061	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	84.8	81394	PASS
175	174	5	9	6.5	5330	PASS
176	174	95	101	100.2	81573	PASS
177	176	5	9	5.8	4748	PASS