




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD050223\
 Data File : VD075966.D
 Acq On : 02 May 2023 16:03
 Operator : KP/SY
 Sample : 02564-21
 Misc : 5.88G/10.00mL/MSVOA_D/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DCCN2

Manual IntegrationsAPPROVED

Quant Time: May 03 02:49:50 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 03 02:37:35 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/03/2023
 Supervised By :Mahesh Dadoda 05/03/2023

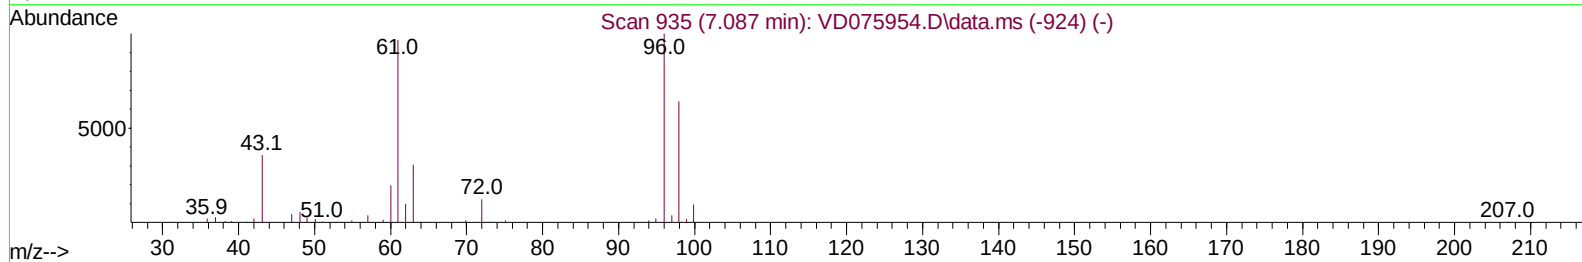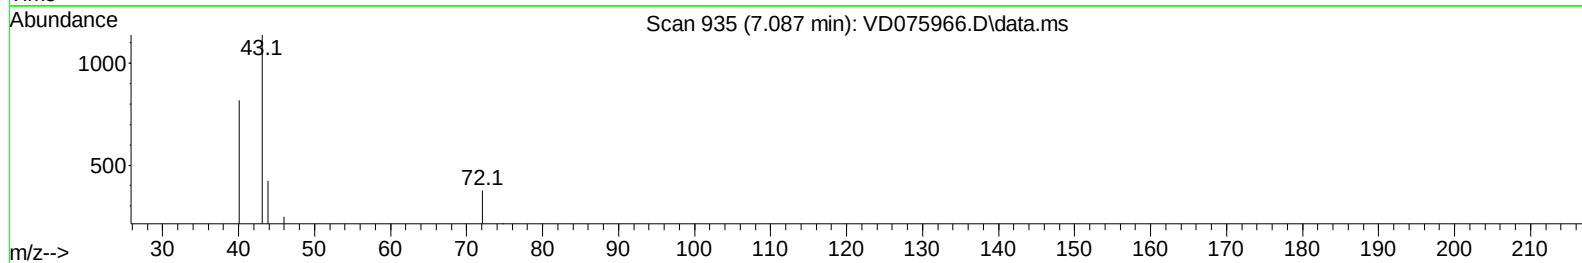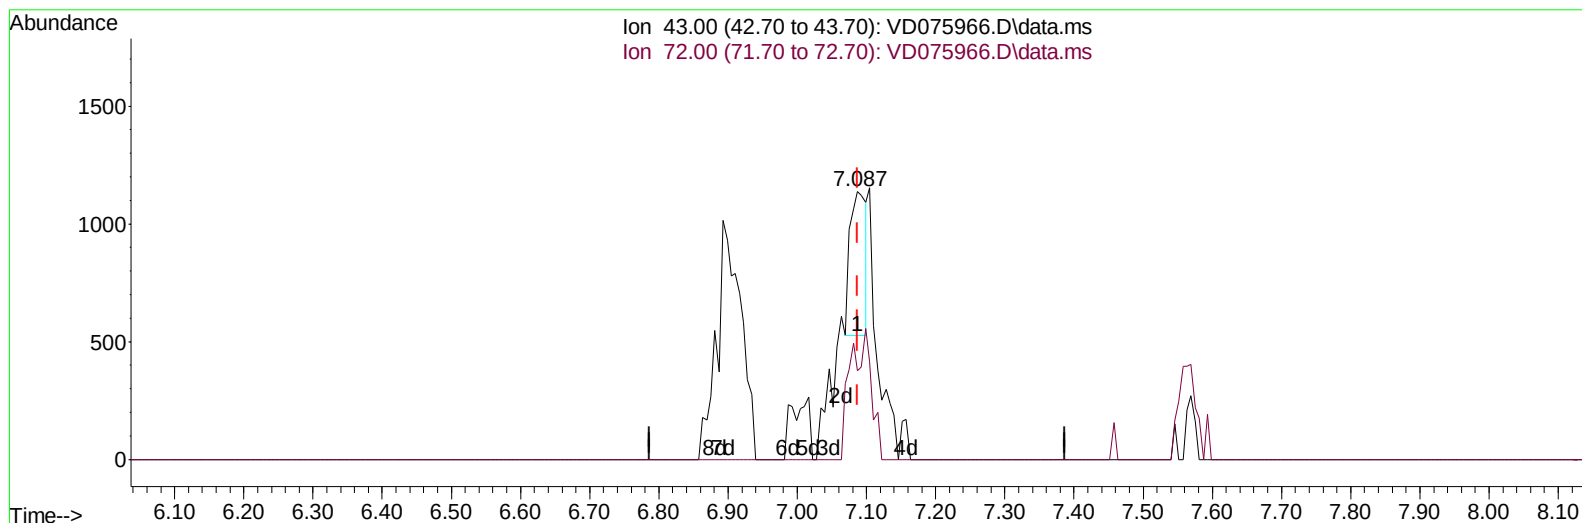

TIC: VD075966.D\data.ms

(22) 2-Butanone (T)

7.087min (+ 0.000) 2.22 ug/L

response 976

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	41.00	56.97
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD050223\
 Data File : VD075966.D
 Acq On : 02 May 2023 16:03
 Operator : KP/SY
 Sample : 02564-21
 Misc : 5.88G/10.00mL/MSVOA_D/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DCCN2

Manual IntegrationsAPPROVED

Quant Time: May 03 02:49:50 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 03 02:37:35 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/03/2023
 Supervised By :Mahesh Dadoda 05/03/2023

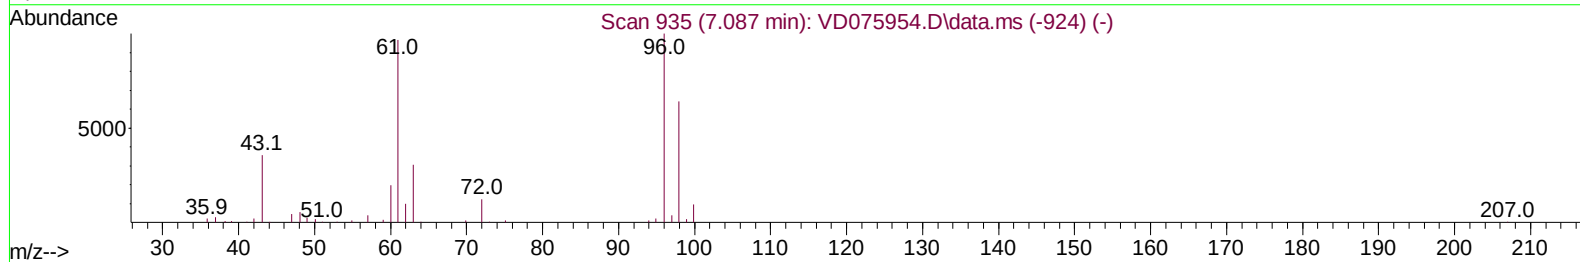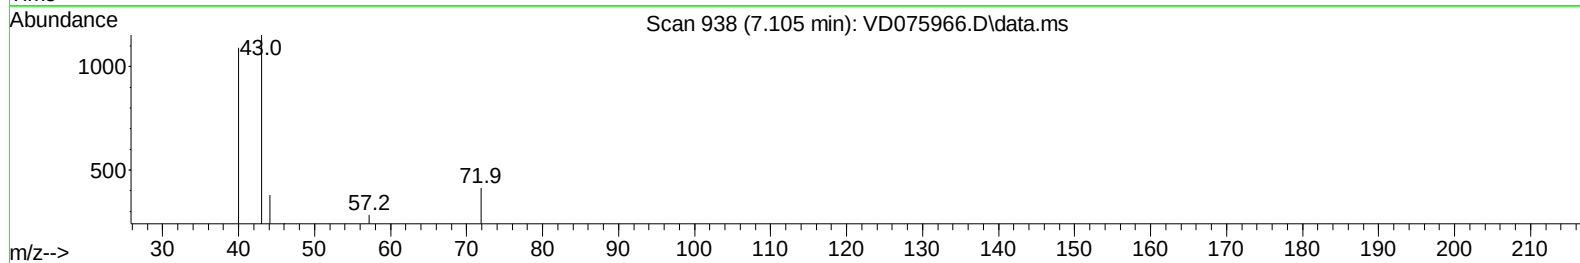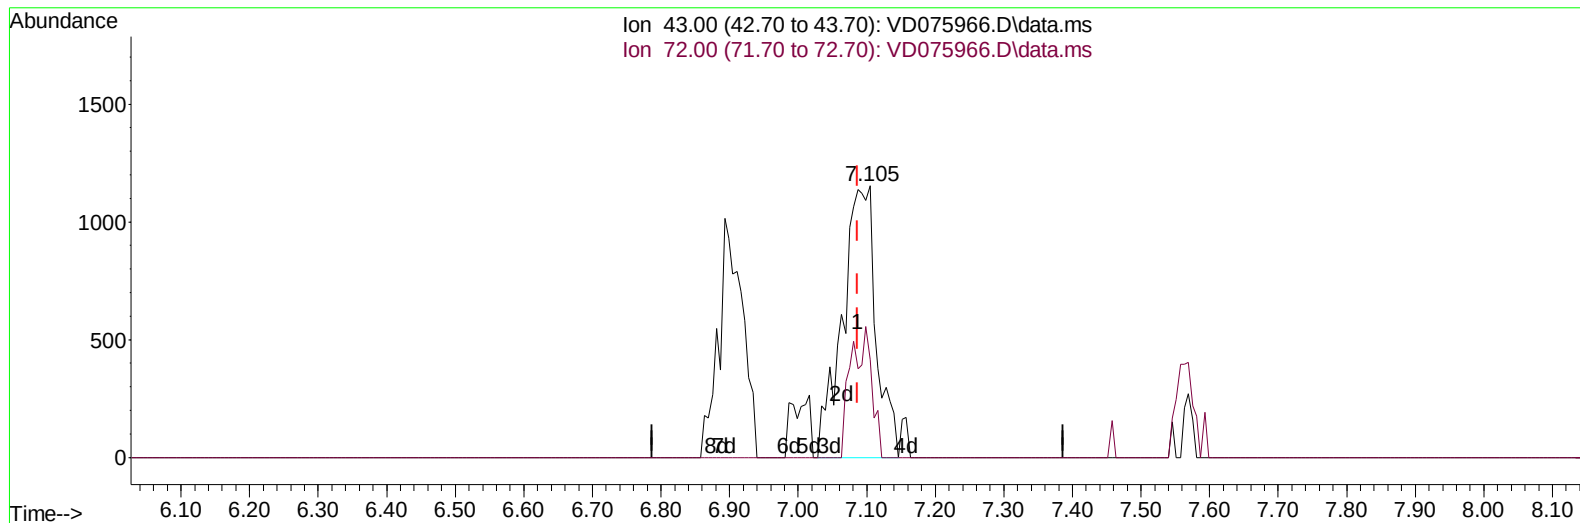

TIC: VD075966.D\data.ms

(22) 2-Butanone (T)

7.105min (+ 0.018) 8.92 ug/L m

response 3918

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	41.00	14.19#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD050223\
 Data File : VD075966.D
 Acq On : 02 May 2023 16:03
 Operator : KP/SY
 Sample : 02564-21
 Misc : 5.88G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DCCN2

Manual IntegrationsAPPROVED

Quant Time: May 03 02:49:50 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 03 02:37:35 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/03/2023
 Supervised By :Mahesh Dadoda 05/03/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.781	114	206709	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117	243042	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.522	152	105064	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.275	65	52387	11.553	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	46.200%	
7) Chloroethane-d5	2.799	69	65152	16.629	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	66.520%	
11) 1,1-Dichloroethene-d2	3.922	65	13472	12.886	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	51.560%	
21) 2-Butanone-d5	6.981	46	62146	157.865	ug/L	-0.01
Spiked Amount 50.000	Range 20	- 135	Recovery	=	315.740%#	
24) Chloroform-d	7.569	84	133677	25.861	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	103.440%	
26) 1,2-Dichloroethane-d4	8.234	65	82244	37.258	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	149.040%#	
32) Benzene-d6	8.205	84	220423	15.560	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	62.240%	
36) 1,2-Dichloropropane-d6	9.210	67	89196	22.749	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	91.000%	
41) Toluene-d8	10.269	98	188335	14.201	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	56.800%	
43) trans-1,3-Dichloroprop...	10.528	79	42895	26.468	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	105.880%	
47) 2-Hexanone-d5	10.881	63	48691	103.137	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	206.280%#	
56) 1,1,2,2-Tetrachloroeth...	12.651	84	137958	45.981	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	183.920%#	
66) 1,2-Dichlorobenzene-d4	13.816	152	103312	27.800	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	111.200%	
Target Compounds					Qvalue	
13) Acetone	4.022	43	43600	129.420	ug/L	99
16) Methylene chloride	4.805	84	13654	3.256	ug/L	96
22) 2-Butanone	7.105	43	3918m	8.921	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD050223\
Data File : VD075966.D
Acq On : 02 May 2023 16:03
Operator : KP/SY
Sample : 02564-21
Misc : 5.88G/10.00mL/MSVOA_D/SOIL
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
DCCN2

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 05/03/2023
Supervised By :Mahesh Dadoda 05/03/2023

Quant Time: May 03 02:49:50 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 03 02:37:35 2023
Response via : Initial Calibration

